

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061218\
 Data File : VV006248.D
 Acq On : 12 Jun 2018 15:43
 Operator : SY/MD
 Sample : J3405-09
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jun 13 01:28:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 13 01:21:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	304544	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	265202	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	123980	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	75660	4.55	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.00%
7) Chloroethane-d5	1.58	69	71213	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.00%
11) 1,1-Dichloroethene-d2	2.13	63	109759	3.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.00%
20) 2-Butanone-d5	3.95	46	200194	56.68	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.36%
24) Chloroform-d	4.40	84	154293	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.09	65	77296	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.10	84	312838	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.12	67	97024	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.36	98	276918	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
43) trans-1,3-Dichloropropene-	7.67	79	37296	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.14	63	172534	46.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.22%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	65962	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	108122	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	5608	0.291 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061218\
Data File : VV006248.D
Acq On : 12 Jun 2018 15:43
Operator : SY/MD
Sample : J3405-09
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jun 13 01:28:54 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 13 01:21:06 2018
Response via : Initial Calibration

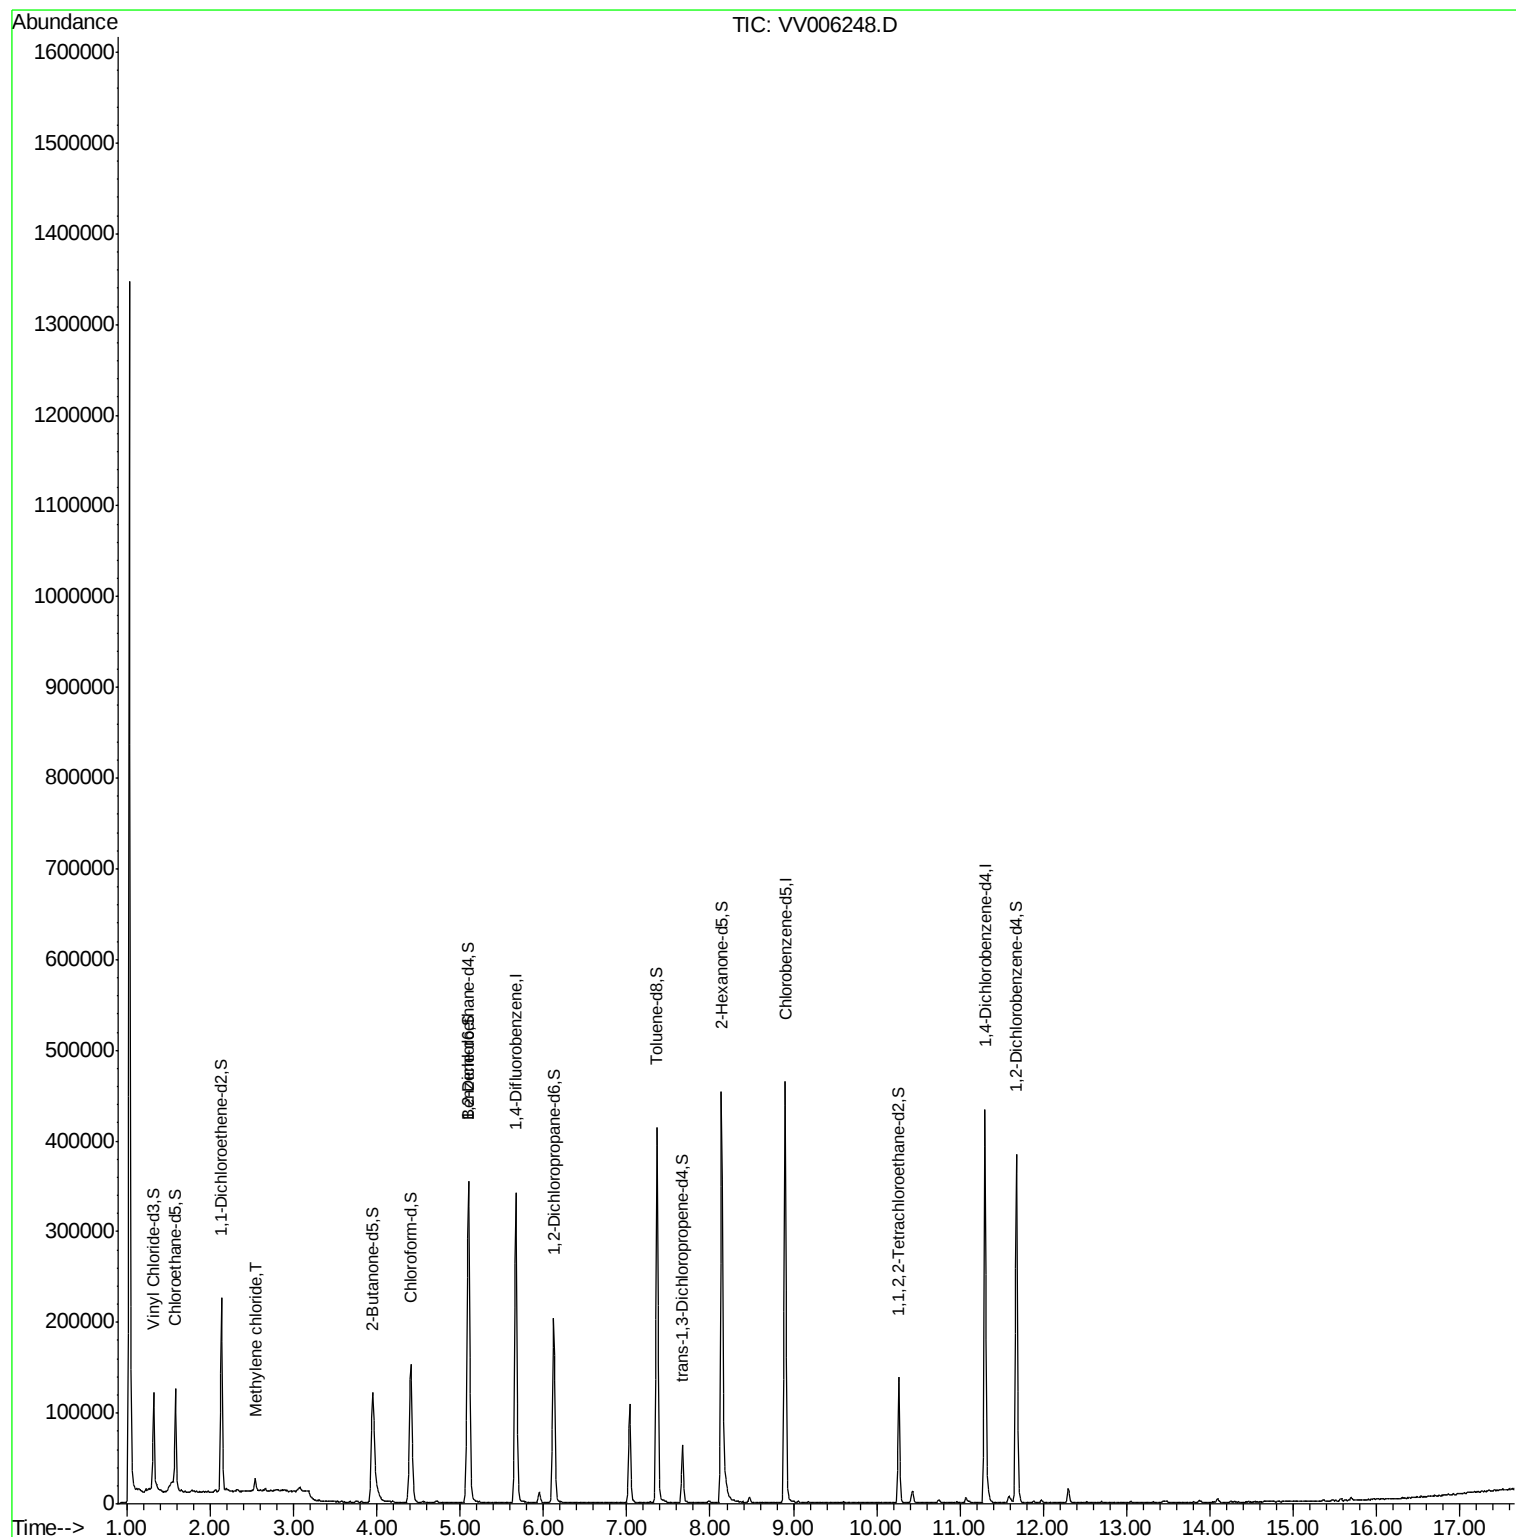

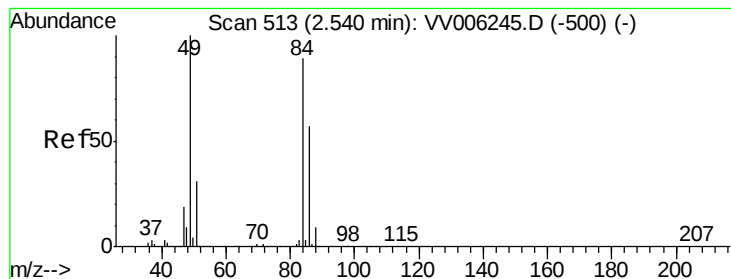

#16

Methylene chloride

Concen: 0.291 ug/L

RT: 2.54 min Scan# 513

Delta R.T. 0.00 min

Lab File: VV006248.D

Acq: 12 Jun 2018 15:43

Instrument :

MSVOA_V

ClientSampleId :

VHBLK01

Tot Ion: 84 Resp: 5608

Ion Ratio Lower Upper

84 100

86 60.5 44.2 82.0

49 109.9 78.8 146.4

