


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061218\
 Data File : VV006244.D
 Acq On : 12 Jun 2018 10:30
 Operator : SY/MD
 Sample : BFB70
 Misc : 25 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053118WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jun 22 05:38:08 2018

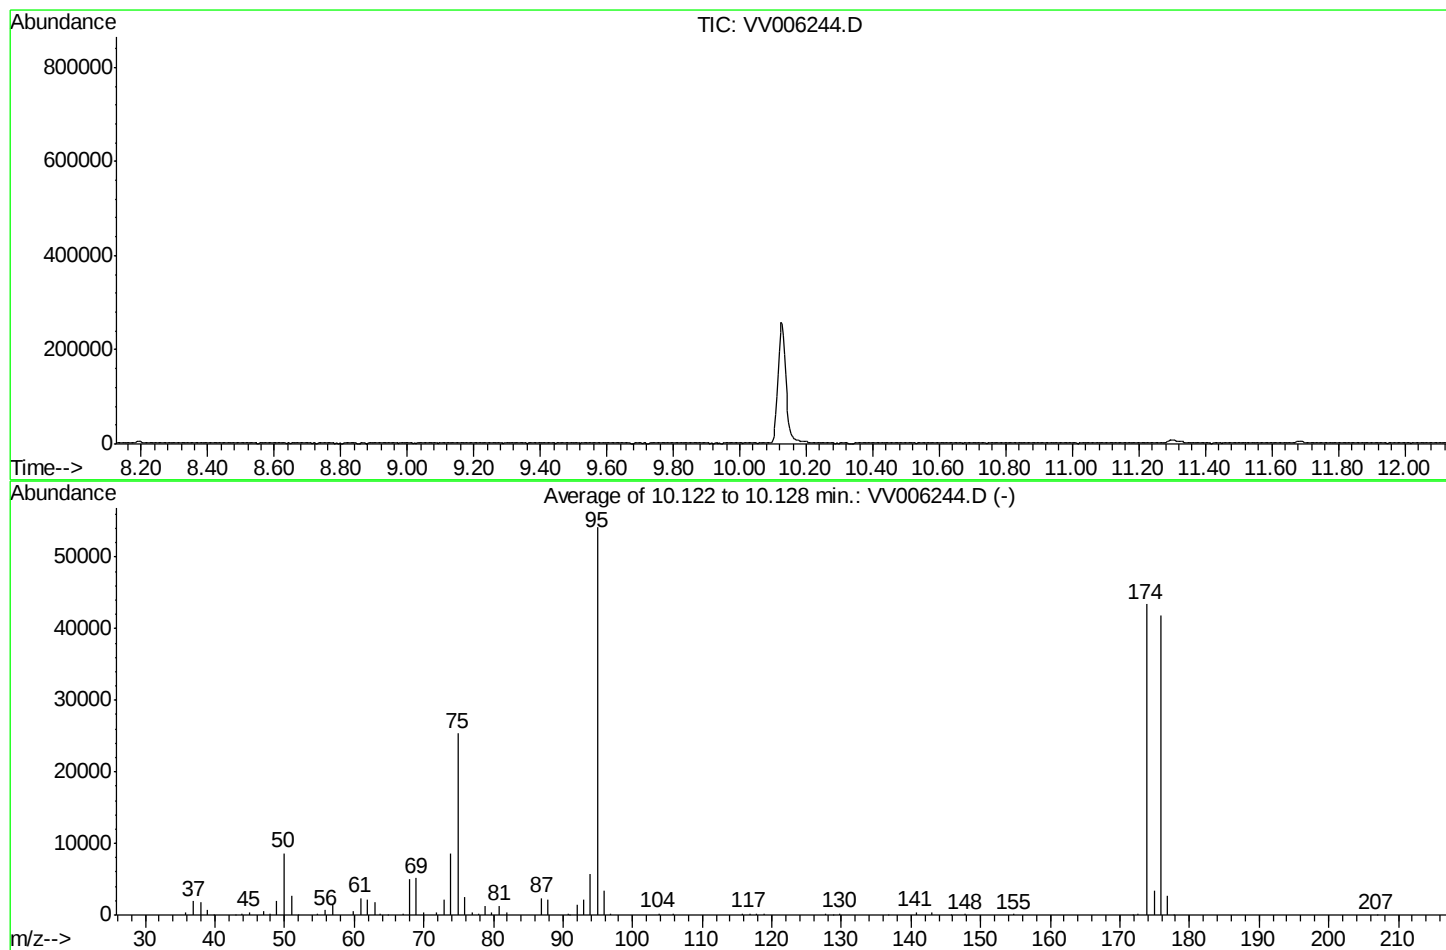

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	8625	PASS
75	95	30	80	46.8	25333	PASS
95	95	100	100	100.0	54157	PASS
96	95	5	9	6.4	3443	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.2	43450	PASS
175	174	5	9	7.7	3350	PASS
176	174	95	101	96.3	41826	PASS
177	176	5	9	6.4	2672	PASS

m/z	Abundance
38.80	122.0
39.80	181.0
40.90	213.0
41.90	110.0
42.80	167.0
43.90	829.0
54.80	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.80	326.0
36.90	1893.0
37.90	1712.0
38.90	853.0
39.80	174.0
41.00	152.0
43.00	189.0
43.90	1011.0
44.90	411.0
46.90	580.0
47.80	239.0
48.90	1838.0
49.90	8250.0
51.00	2709.0
51.90	102.0
54.80	249.0
55.90	659.0
56.90	1492.0
59.90	424.0
60.90	2336.0
61.90	2050.0
62.90	1736.0
63.80	161.0
67.10	148.0
67.90	4833.0
68.90	4883.0
69.90	378.0
71.80	315.0
72.90	1881.0
73.90	8288.0
74.90	24184.0
75.90	2361.0
76.90	358.0
77.90	247.0
78.80	1236.0
79.80	434.0
80.90	1271.0
81.90	316.0
86.90	2370.0
87.90	2100.0
90.80	215.0
92.00	1321.0
92.90	2061.0
93.90	5325.0
94.90	51256.0
95.90	3393.0
96.90	154.0
103.80	207.0
105.80	179.0
115.70	135.0
116.80	247.0
117.80	185.0
118.80	199.0
127.70	207.0
128.80	112.0
129.80	153.0
140.80	362.0
142.90	319.0
147.80	116.0
154.80	101.0
172.60	271.0
173.80	39936.0
174.90	3175.0
175.80	38664.0
176.90	2613.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.90	391.0
36.90	1992.0
37.90	1862.0
38.90	928.0
39.80	214.0
40.90	167.0
43.00	192.0
43.90	1028.0
44.90	465.0
46.90	654.0
47.90	253.0
48.90	1993.0
49.90	8799.0
50.90	2779.0
51.90	101.0
54.80	226.0
55.90	731.0
56.90	1588.0
59.90	473.0
60.90	2406.0
61.90	2277.0
62.90	1780.0
63.80	160.0
64.80	104.0
67.00	143.0
67.90	5132.0
68.90	5336.0
69.90	395.0
71.80	303.0
73.00	2157.0
73.90	8910.0
74.90	26184.0
75.90	2535.0
76.90	351.0
77.80	270.0
78.80	1246.0
79.80	439.0
80.90	1385.0
81.80	330.0
86.90	2446.0
87.80	2295.0
90.70	207.0
92.00	1416.0
92.90	2260.0
93.90	5842.0
94.90	56176.0
96.00	3501.0
96.90	145.0
103.80	220.0
105.80	184.0
115.70	152.0
116.90	264.0
117.70	210.0
118.80	225.0
127.80	174.0
128.80	102.0
129.80	190.0
140.70	416.0
142.90	313.0
147.80	131.0
154.80	106.0
172.70	301.0
173.80	44728.0
174.90	3498.0
175.80	43096.0
176.90	2726.0
206.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.90	394.0
36.90	1975.0
37.90	1872.0
38.90	904.0
39.80	239.0
40.90	180.0
43.00	184.0
43.90	1033.0
44.90	468.0
47.00	645.0
47.90	265.0
48.90	1918.0
49.90	8828.0
50.90	2611.0
54.80	194.0
55.90	744.0
56.90	1484.0
59.90	506.0
60.90	2275.0
61.90	2273.0
62.90	1650.0
63.80	144.0
64.80	128.0
66.90	153.0
67.90	4931.0
68.90	5298.0
69.90	392.0
71.90	264.0
72.90	2207.0
73.90	8666.0
74.90	25632.0
75.90	2397.0
76.90	344.0
77.70	288.0
78.90	1177.0
79.80	402.0
80.90	1354.0
81.80	327.0
86.90	2344.0
87.80	2264.0
90.70	181.0
91.00	161.0
91.90	1397.0
93.00	2297.0
93.90	5839.0
94.90	55040.0
96.00	3436.0
96.90	117.0
103.80	209.0
105.80	167.0
115.80	154.0
116.90	278.0
117.70	210.0
118.80	238.0
127.90	152.0
129.80	200.0
136.70	112.0
140.70	430.0
142.90	326.0
145.70	106.0
147.80	114.0
154.80	110.0
171.80	102.0
173.80	45688.0
174.90	3378.0
175.80	43720.0
176.90	2677.0
177.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70