
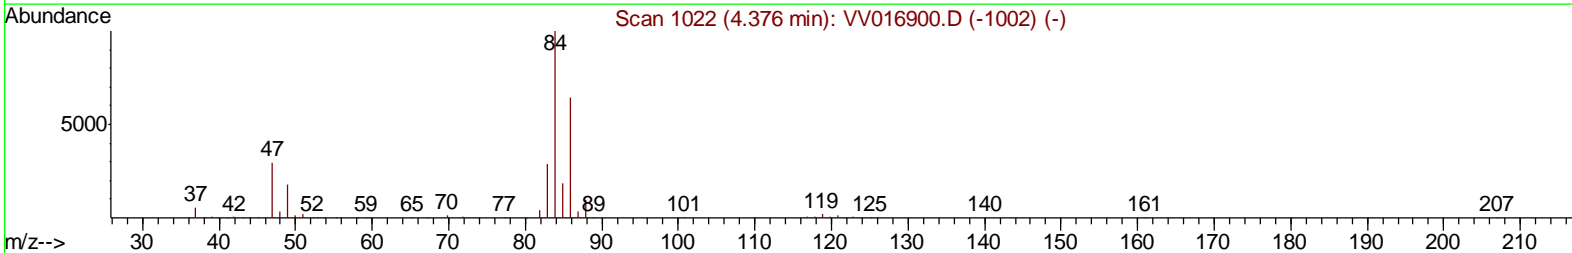
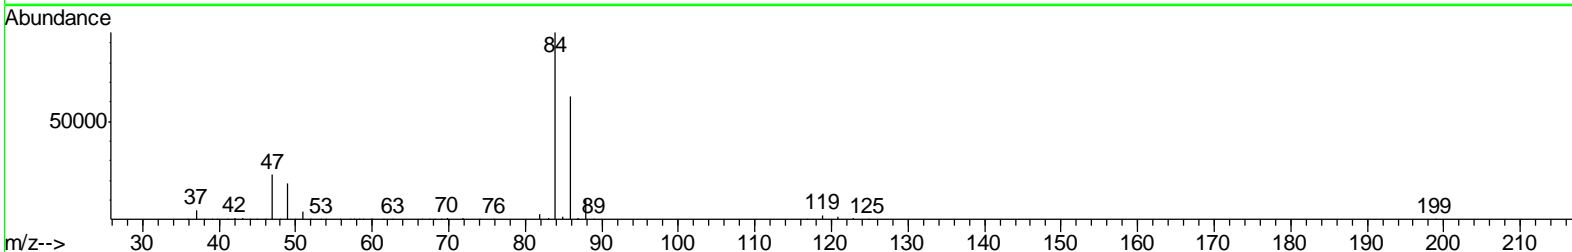


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016904.D
 Acq On : 13 Jun 2020 02:07
 Operator : SY/MD
 Sample : L2914-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Quant Time: Jun 13 06:25:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

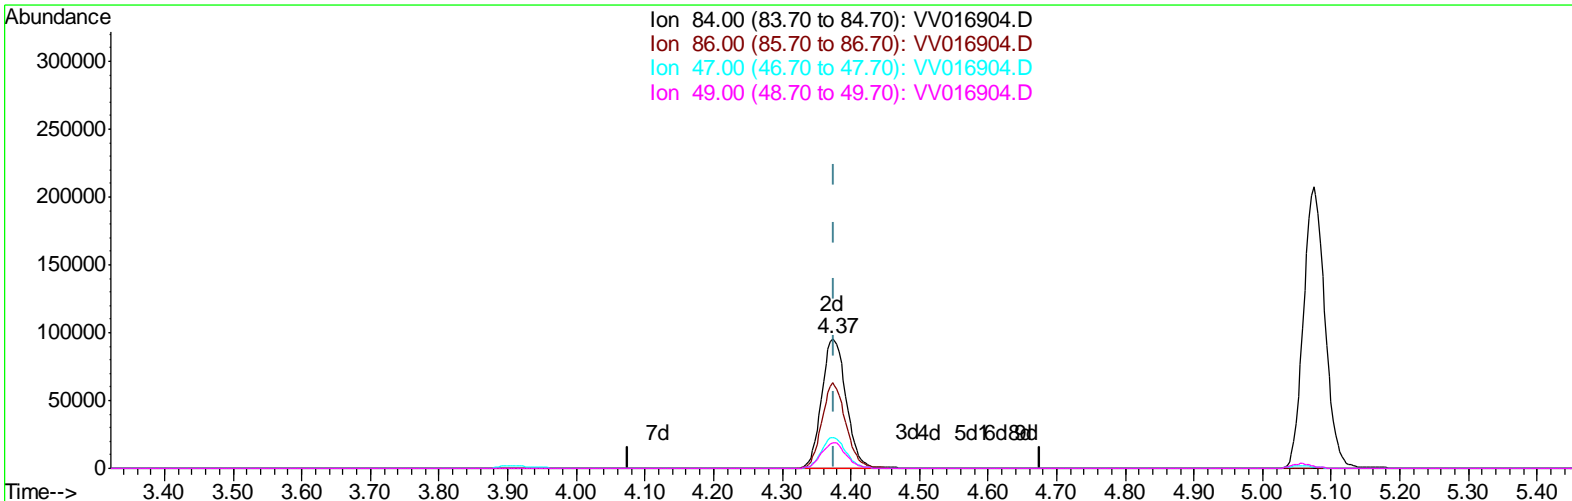

TIC: VV016904.D

(24) Chloroform-d (S)
 4.373min (-0.003) 44.16ug/L m
 response 236449

Ion	Exp%	Act%
84.00	100	100
86.00	62.80	0.04#
47.00	44.50	0.05#
49.00	27.40	0.02#