


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061220\
Data File : VV016887.D
Acq On : 12 Jun 2020 18:35
Operator : SY/MD
Sample : L2913-08 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jun 13 03:33:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 13 03:02:20 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
F9D95

Manual Integrations
APPROVED

MMDadoda
6/15/2020 12:22:34 PM

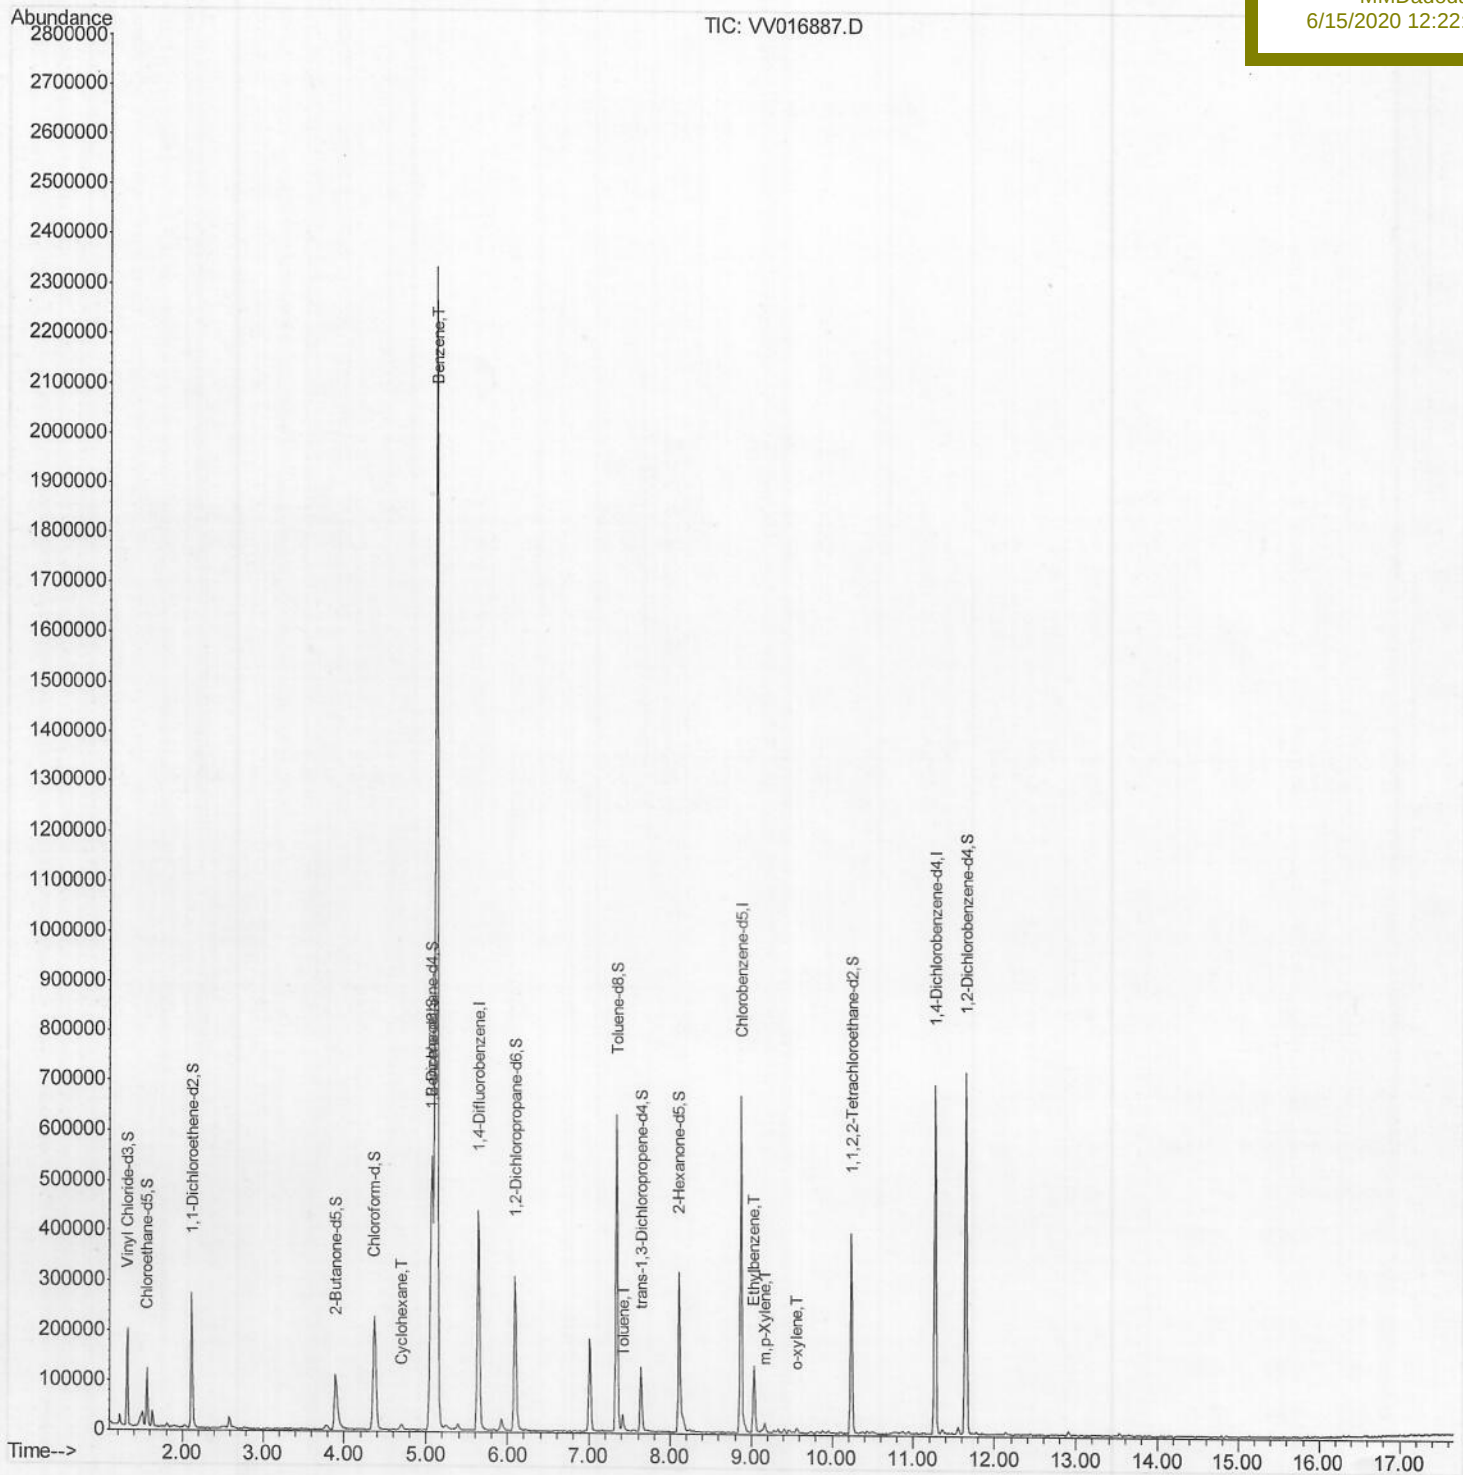

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061220\
Data File : VV016887.D
Acq On : 12 Jun 2020 18:35
Operator : SY/MD
Sample : L2913-08 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jun 17 03:40:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 17 02:00:28 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
F9D95

Manual Integrations
APPROVED

MMDadoda
6/15/2020 12:22:34 PM

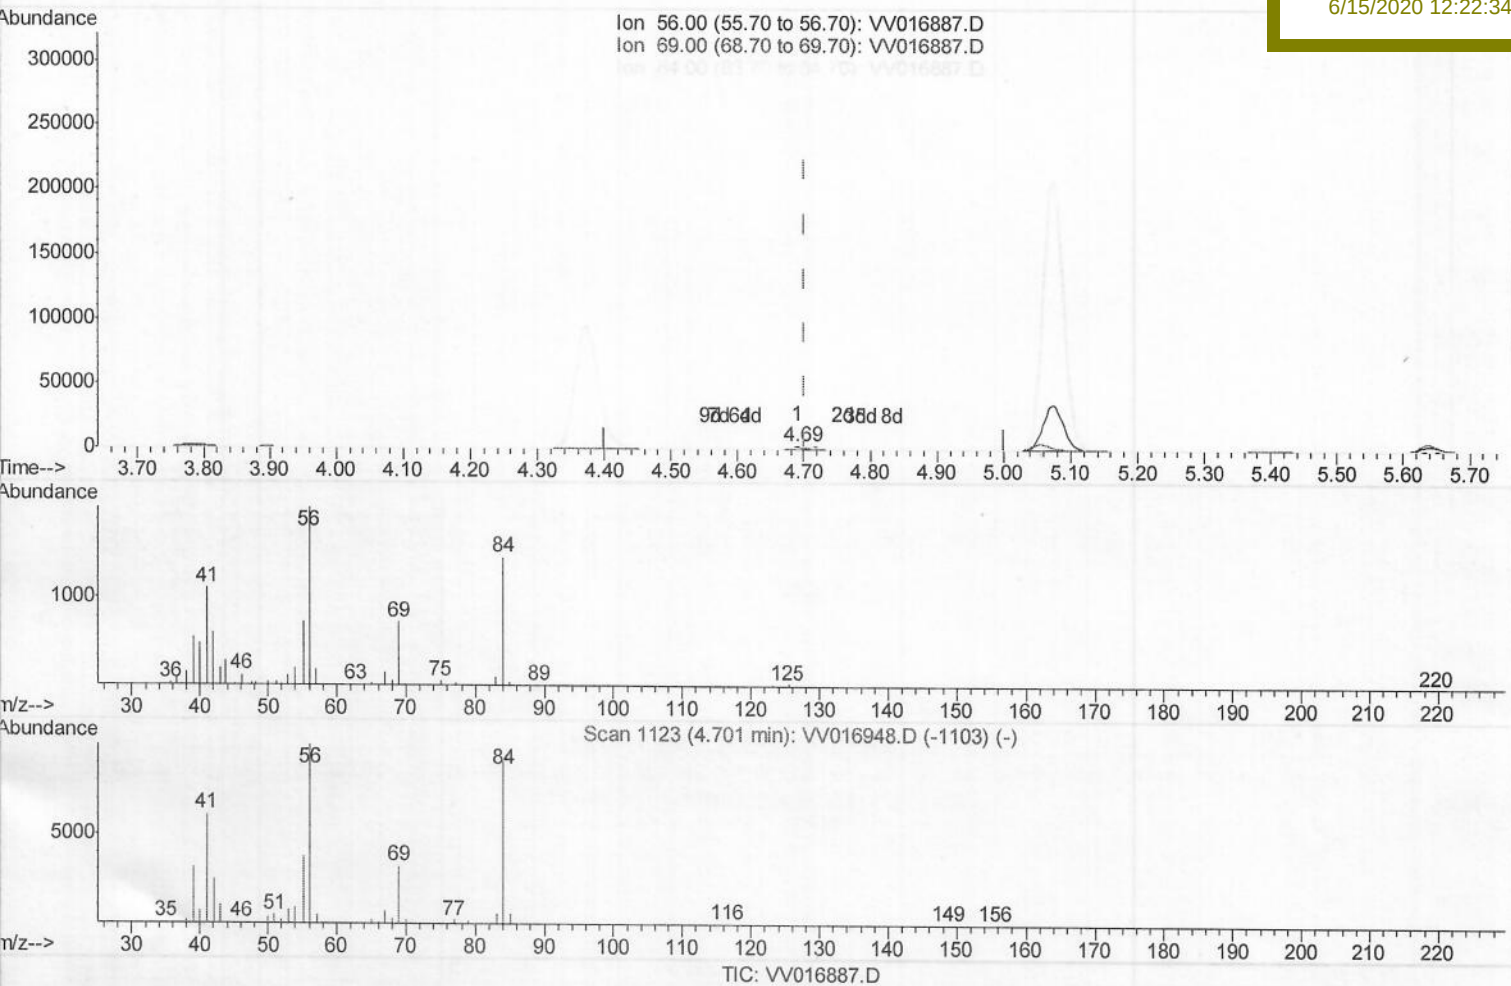

(29) Cyclohexane (T)

4.692min (-0.010) 0.64ug/L

response 2706

Ion	Exp%	Act%
56.00	100	100
69.00	31.20	56.91#
84.00	86.90	205.62#
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061220\
Data File : VV016887.D
Acq On : 12 Jun 2020 18:35
Operator : SY/MD
Sample : L2913-08 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jun 13 03:33:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 13 03:02:20 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
F9D95

Manual Integrations
APPROVED

MMDadoda
6/15/2020 12:22:34 PM

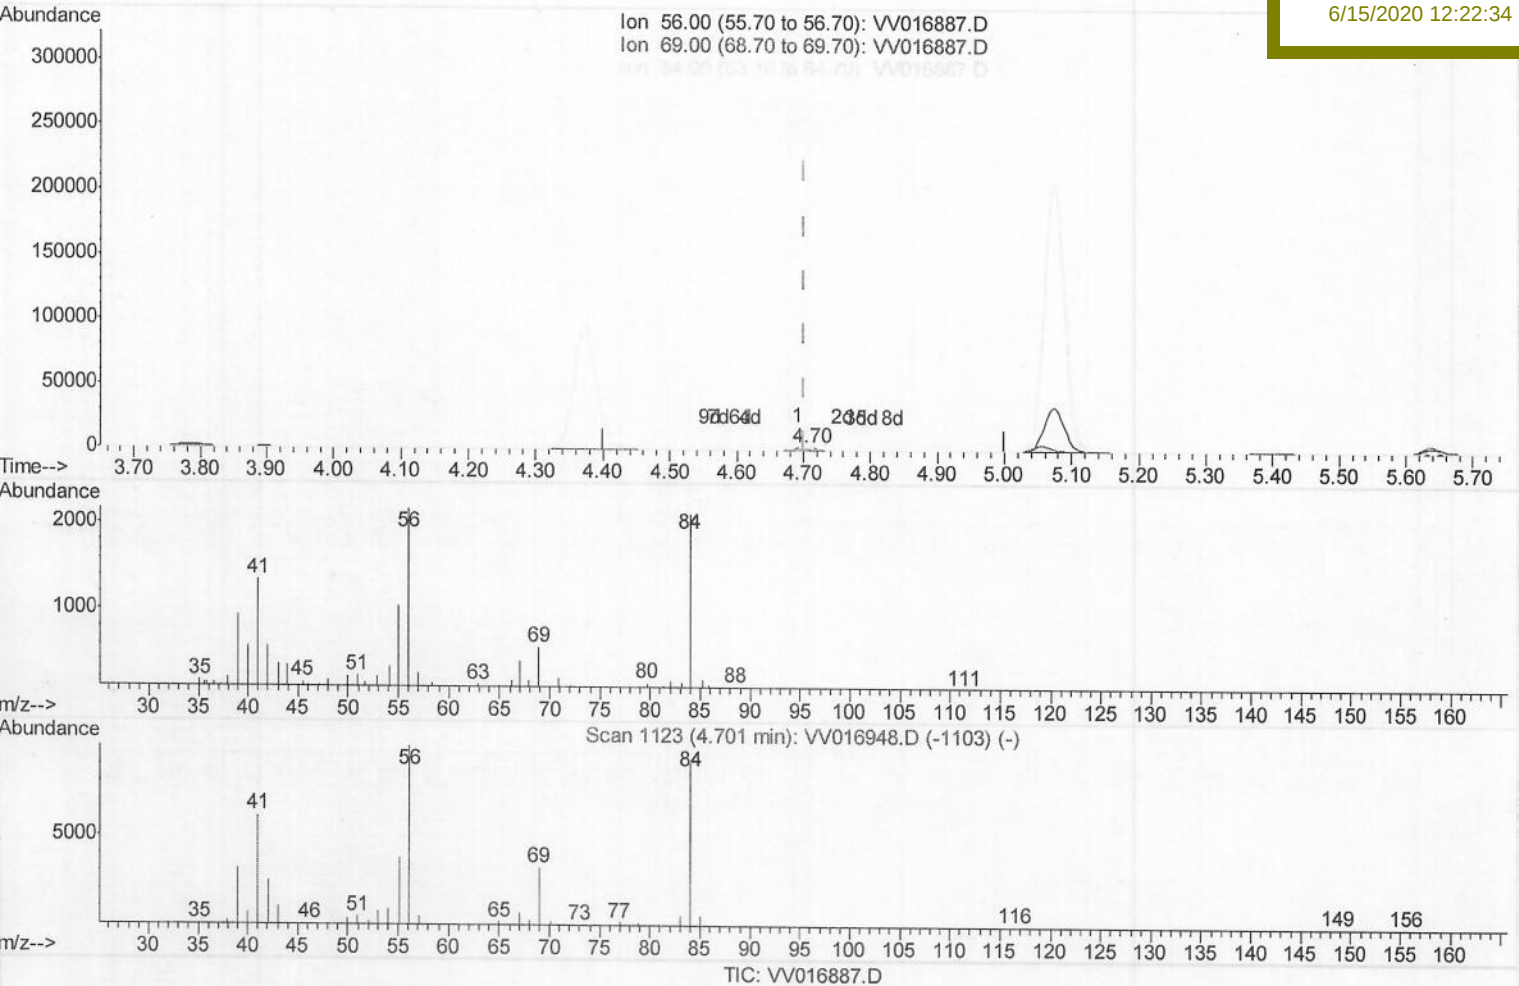

(29) Cyclohexane (T)

4.704min (+0.003) 1.39ug/L m

response 5896

Ion	Exp%	Act%
56.00	100	100
69.00	31.20	26.12
84.00	86.90	94.37
0.00	0.00	0.00

MD
06/15/20

Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061220\
 Data File : VV016887.D
 Acq On : 12 Jun 2020 18:35
 Operator : SY/MD
 Sample : L2913-08 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D95

Quant Time: Jun 13 03:33:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 03:02:20 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:22:34 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	362134	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	340428	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	173185	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	97223	38.05	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.10%		
7) Chloroethane-d5	1.56	69	74793	48.78	ug/L	-0.01
Spiked Amount 50.000	Range 70 - 130		Recovery =	97.56%		
11) 1,1-Dichloroethene-d2	2.12	63	140279	32.69	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.38%		
21) 2-Butanone-d5	3.89	46	173065	91.51	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.51%		
24) Chloroform-d	4.37	84	227925	43.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.74%		
26) 1,2-Dichloroethane-d4	5.05	65	166018	46.97	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.94%		
32) Benzene-d6	5.07	84	444958	45.34	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.68%		
36) 1,2-Dichloropropane-d6	6.09	67	135320	44.24	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.48%		
41) Toluene-d8	7.34	98	400353	44.46	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.92%		
43) trans-1,3-Dichloropropene-	7.64	79	70978	44.55	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.10%		
47) 2-Hexanone-d5	8.11	63	101575	76.17	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	76.17%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	177224	43.76	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.52%		
64) 1,2-Dichlorobenzene-d4	11.65	152	178074	48.18	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.36%		

Target Compounds

					Ovalue
29) Cyclohexane	4.70	56	5896m	1.394	ug/L
33) Benzene	5.12	78	2215001	219.910	ug/L
42) Toluene	7.41	91	22063	2.078	ug/L
52) Ethylbenzene	9.03	91	91856	7.810	ug/L
53) m,p-Xylene	9.16	106	4713	1.076	ug/L
54) o-xylene	9.56	106	2712	0.628	ug/L

> MD
 6/15/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed