

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016908.D
 Acq On : 13 Jun 2020 03:42
 Operator : SY/MD
 Sample : L2990-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG6

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:22:58 PM

Quant Time: Jun 13 06:56:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

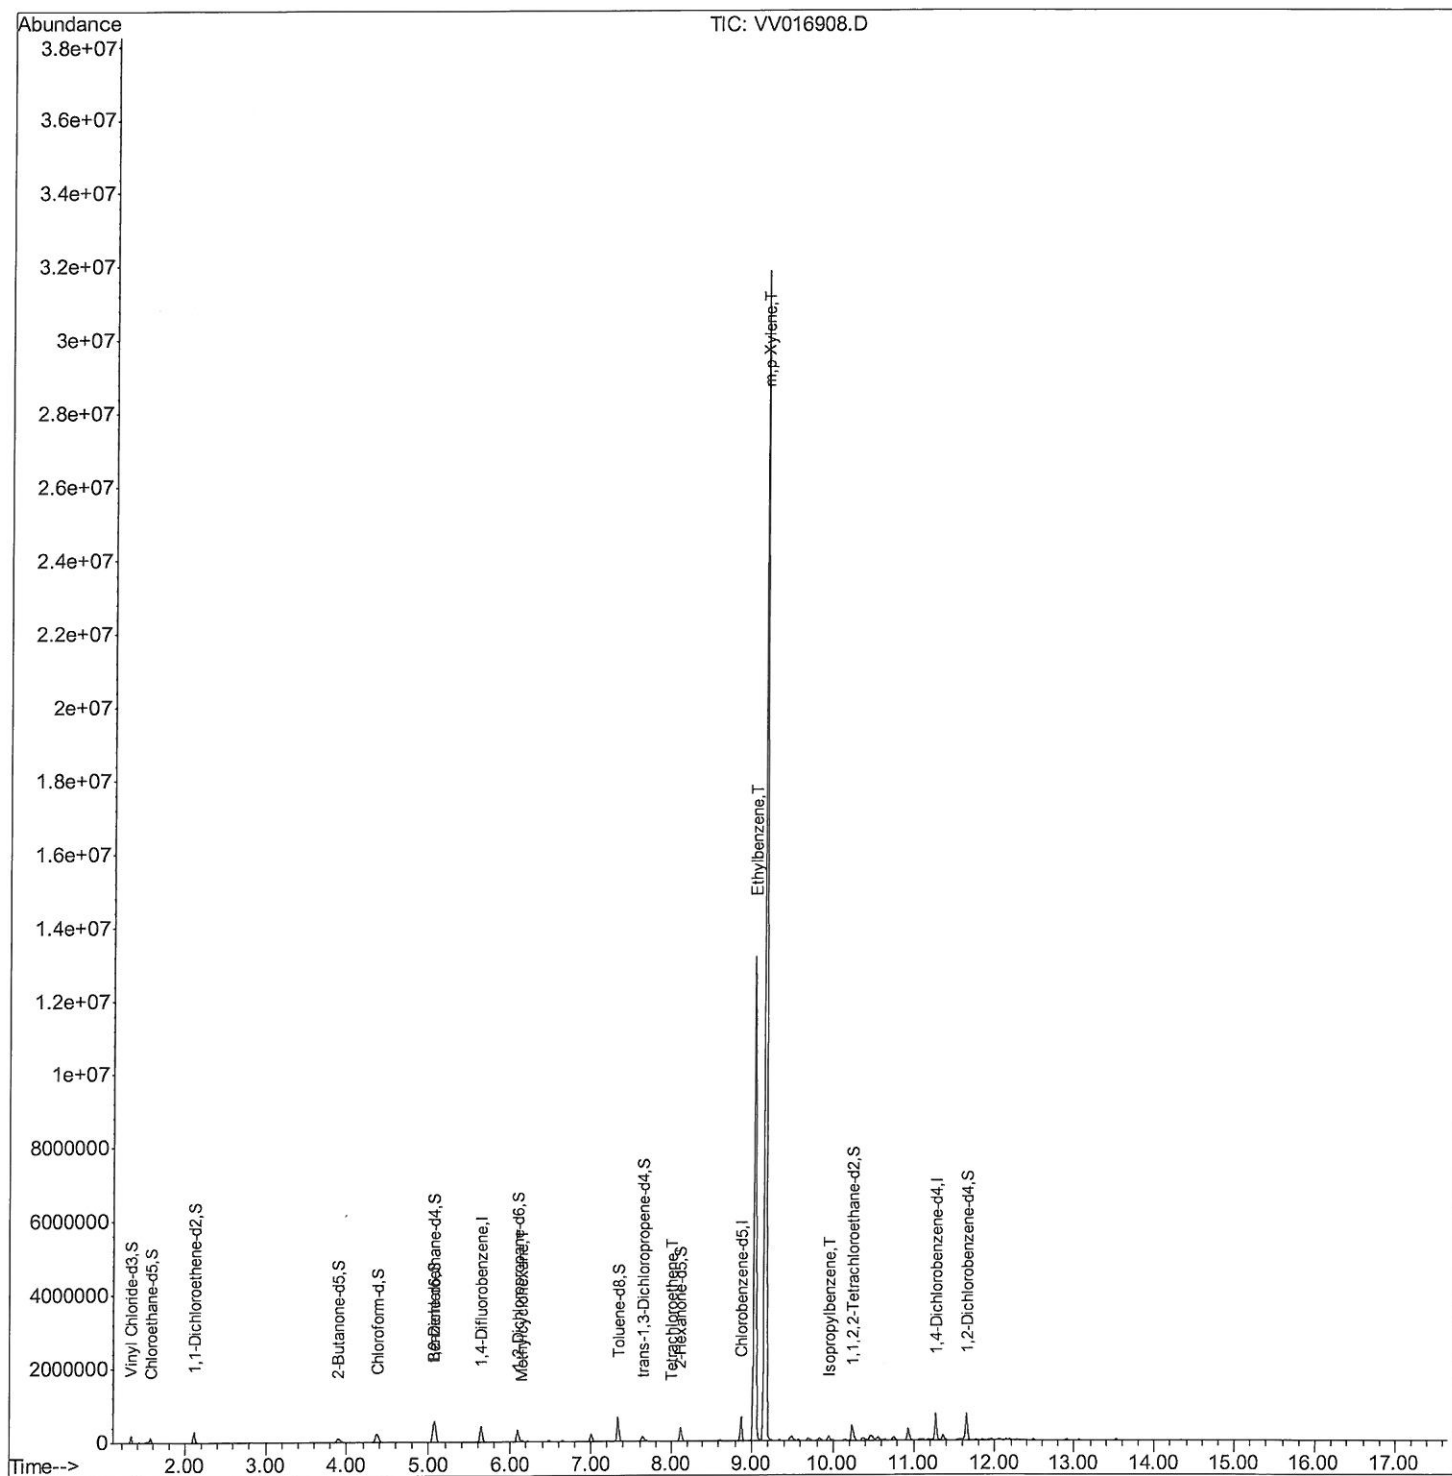

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016908.D
Acq On : 13 Jun 2020 03:42
Operator : SY/MD
Sample : L2990-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E3YG6

Manual Integrations
APPROVED

MMDadoda
6/15/2020 12:22:58 PM

Quant Time: Jun 13 06:16:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 13 06:09:05 2020
Response via : Initial Calibration

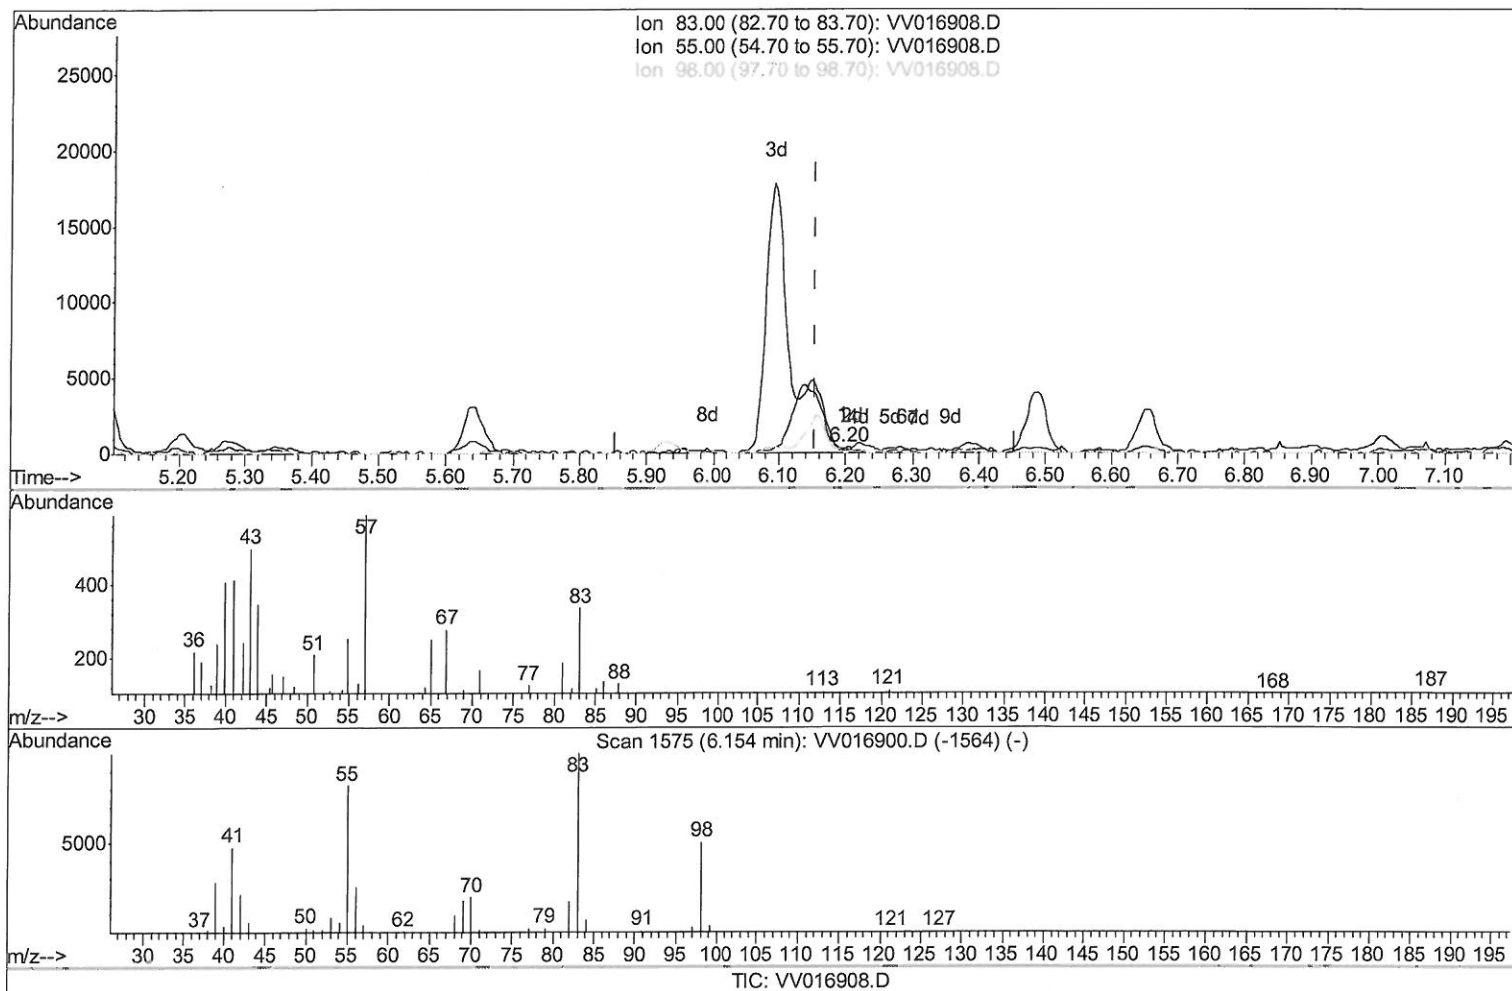

(35) Methylcyclohexane (T)

6.196min (+0.042) 0.02ug/L

response 101

Ion	Exp%	Act%
83.00	100	100
55.00	80.20	0.00#
98.00	50.40	180.20#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016908.D
 Acq On : 13 Jun 2020 03:42
 Operator : SY/MD
 Sample : L2990-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG6

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:22:58 PM

Quant Time: Jun 13 06:16:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

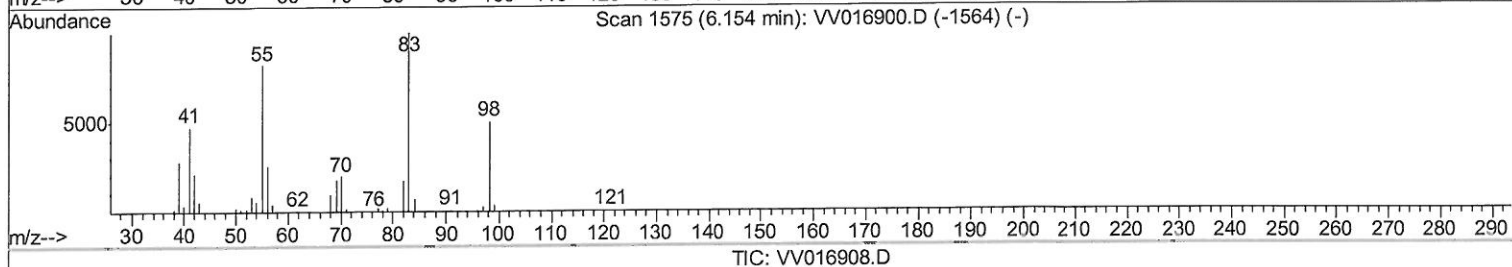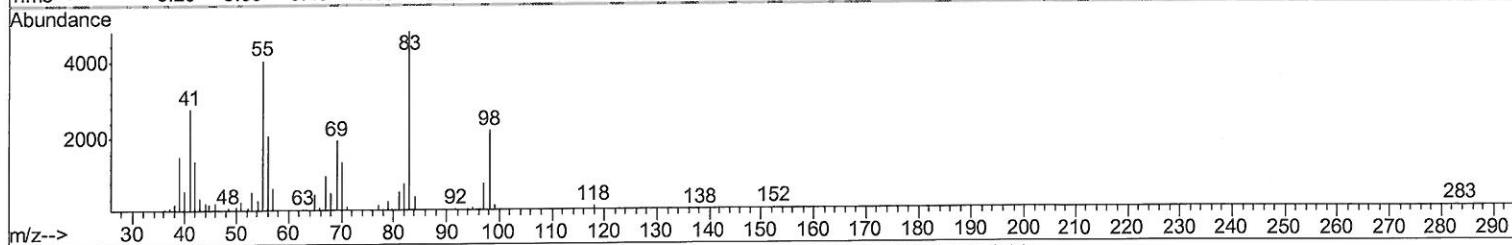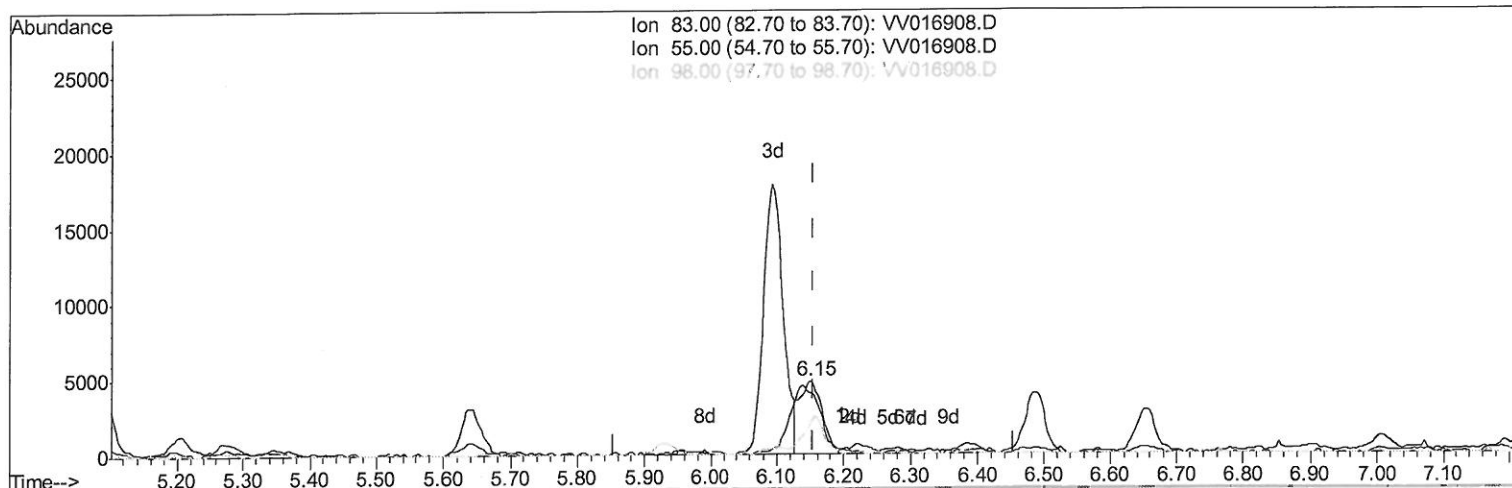

(35) Methylcyclohexane (T)

6.151min (-0.003) 2.71ug/L m

response 11436

MD
 06/15/20

Ion	Exp%	Act%
83.00	100	100
55.00	80.20	0.00#
98.00	50.40	1.59#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016908.D
 Acq On : 13 Jun 2020 03:42
 Operator : SY/MD
 Sample : L2990-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 E3YG6

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:22:58 PM

Quant Time: Jun 13 06:56:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	350006	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	338891	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	167872	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	106727	43.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.42%
7) Chloroethane-d5	1.57	69	61491	41.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.98%
11) 1,1-Dichloroethene-d2	2.12	63	149206	35.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.96%
21) 2-Butanone-d5	3.90	46	177286	96.99	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.99%
24) Chloroform-d	4.38	84	233911	46.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.16%
26) 1,2-Dichloroethane-d4	5.05	65	170898	50.03	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.06%
32) Benzene-d6	5.07	84	451618	46.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.46%
36) 1,2-Dichloropropane-d6	6.09	67	140056	45.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.98%
41) Toluene-d8	7.34	98	414633	46.25	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.50%
43) trans-1,3-Dichloropropene-	7.64	79	68645	43.28	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.56%
47) 2-Hexanone-d5	8.11	63	121399	91.44	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.44%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	179053	44.42	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.84%
64) 1,2-Dichlorobenzene-d4	11.65	152	173919	48.55	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.10%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
35) Methvlcvclohexane	6.15	83	11436m	2.711	ug/L	88
46) Tetrachloroethene	8.00	164	2105	0.995	ug/L	88
52) Ethvlbenzene	9.04	91	8844688	755.451	ug/L	97
53) m,p-Xylene	9.17	106	9138455	2096.363	ug/L	71
56) Isopropylbenzene	9.95	105	75442	6.531	ug/L	99

MD
 06/15/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed