

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG8MS

Quant Time: Jun 13 07:18:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

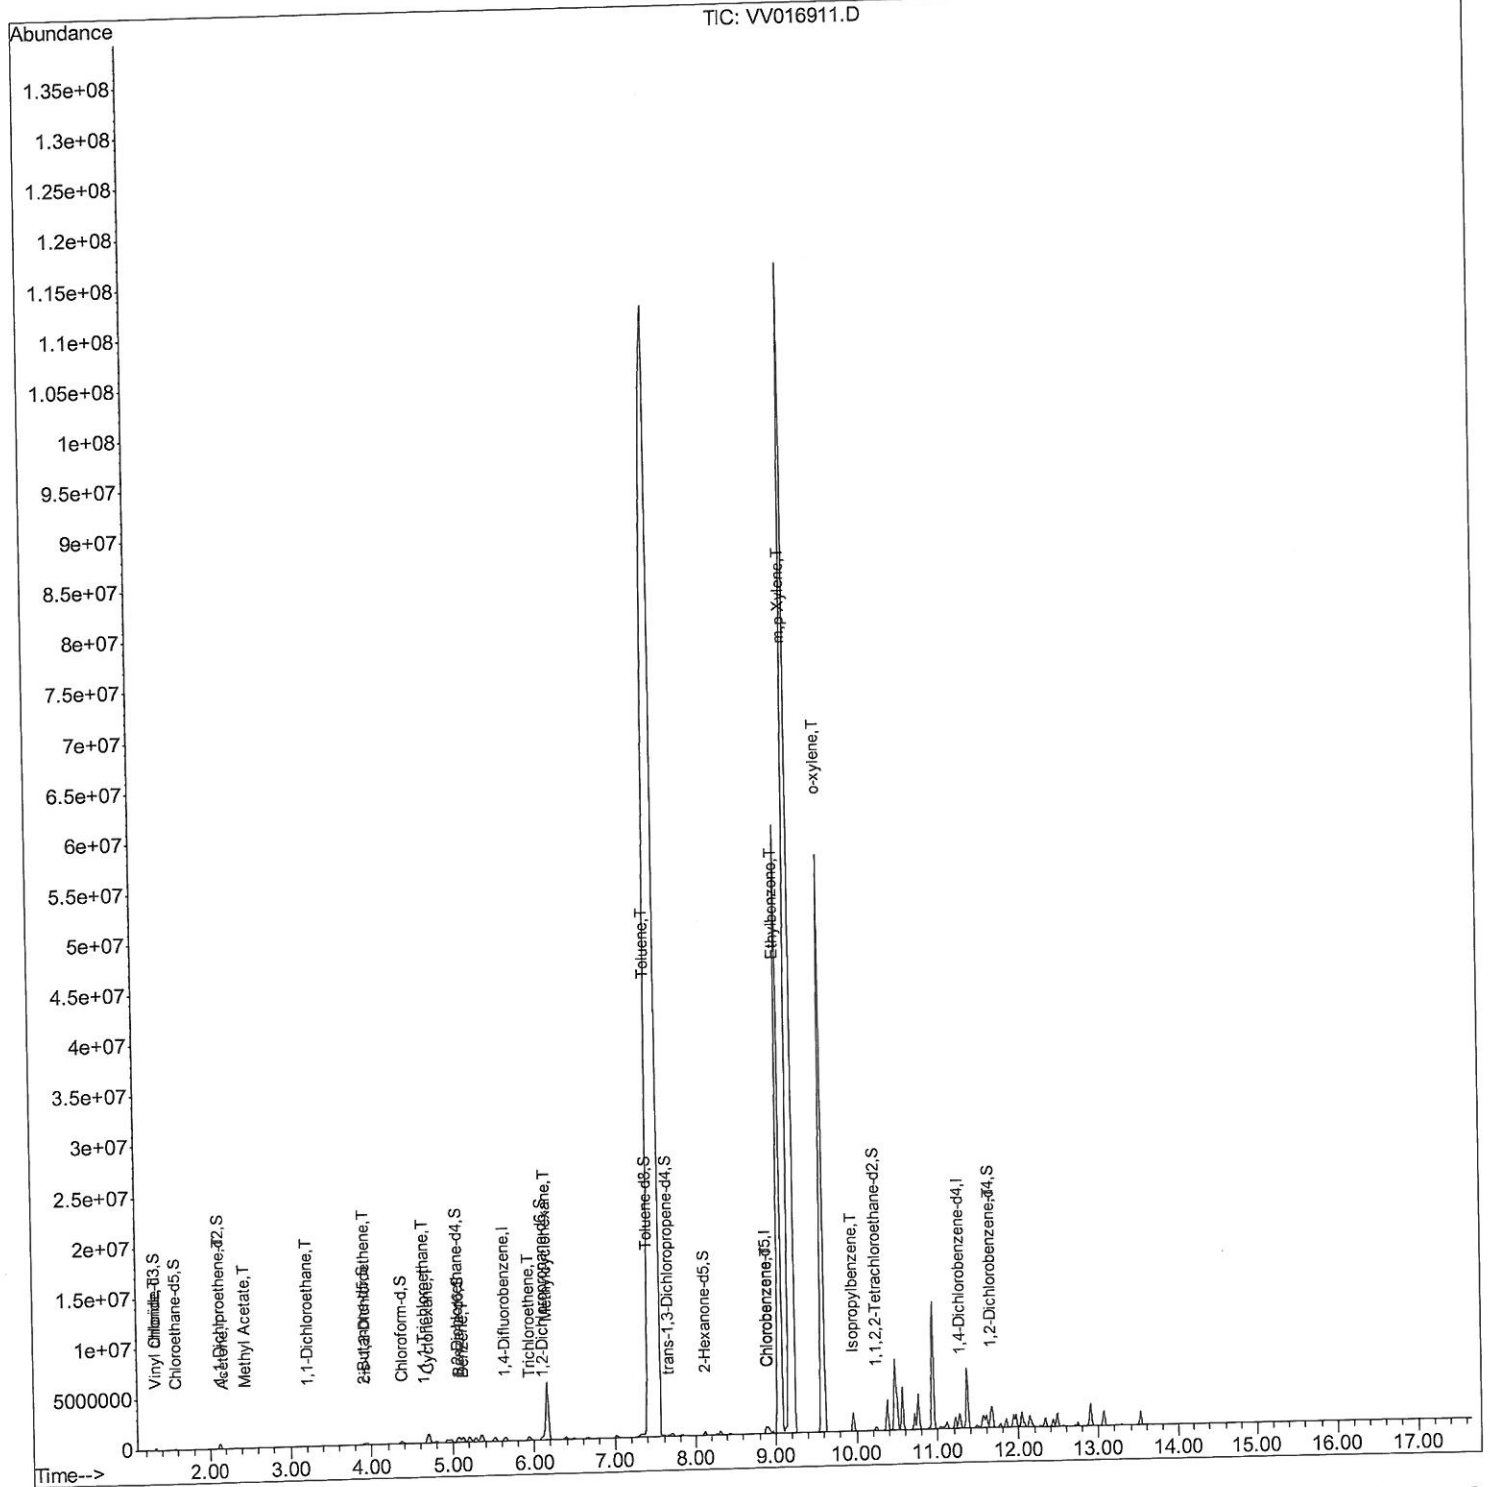

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG8MS

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

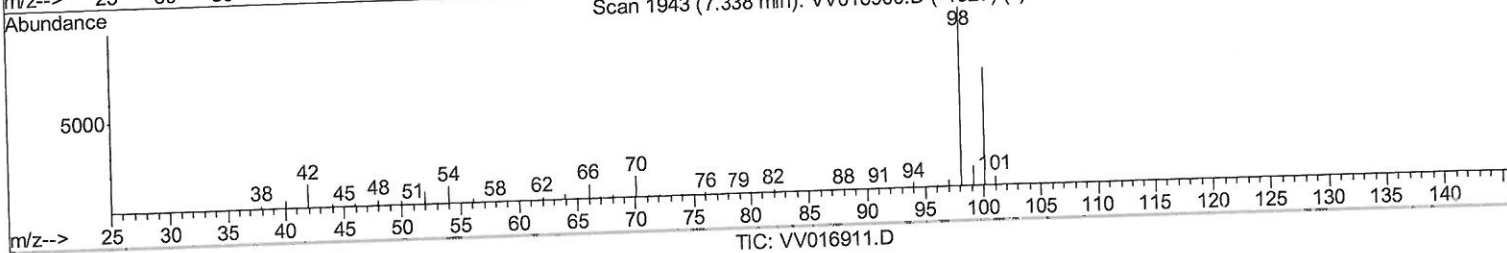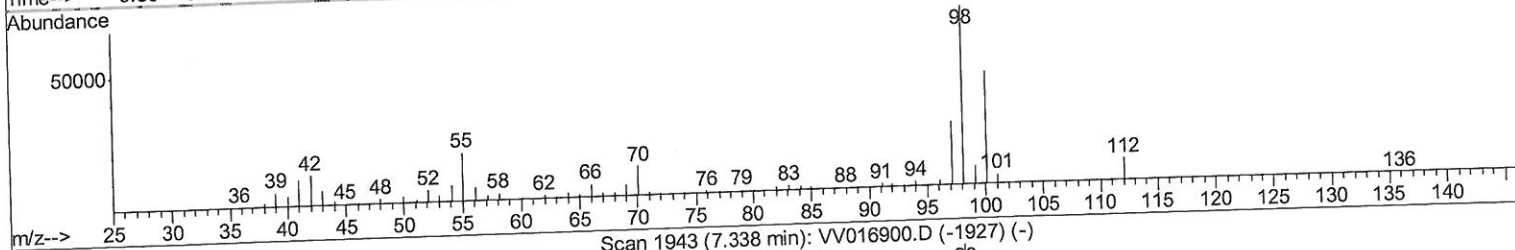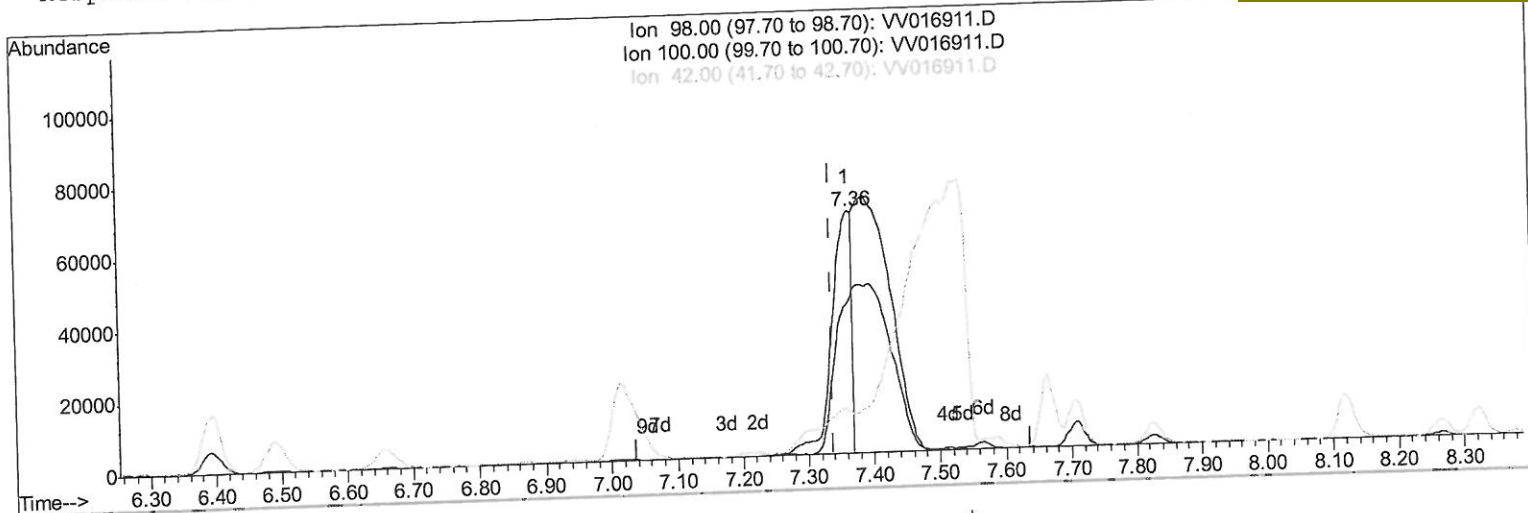

(41) Toluene-d8 (S)

7.364min (+0.026) 15.83ug/L

response 146473

Ion	Exp%	Act%
98.00	100	100
100.00	65.80	96.24#
42.00	12.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 E3YG8MS

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

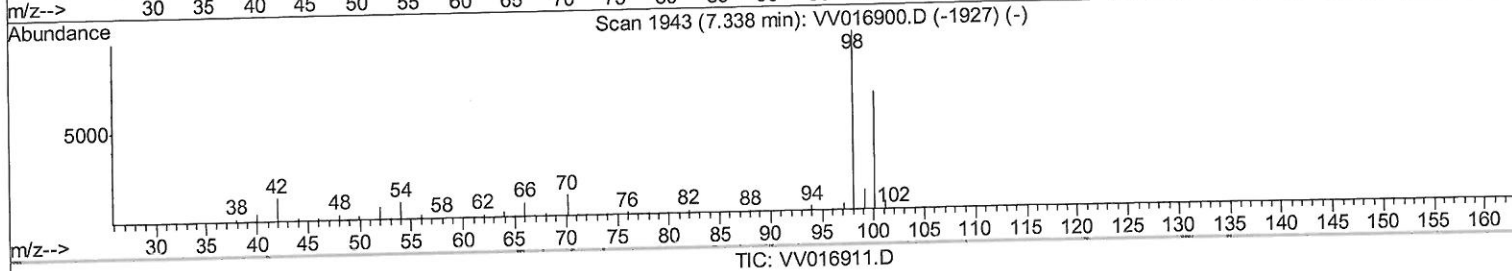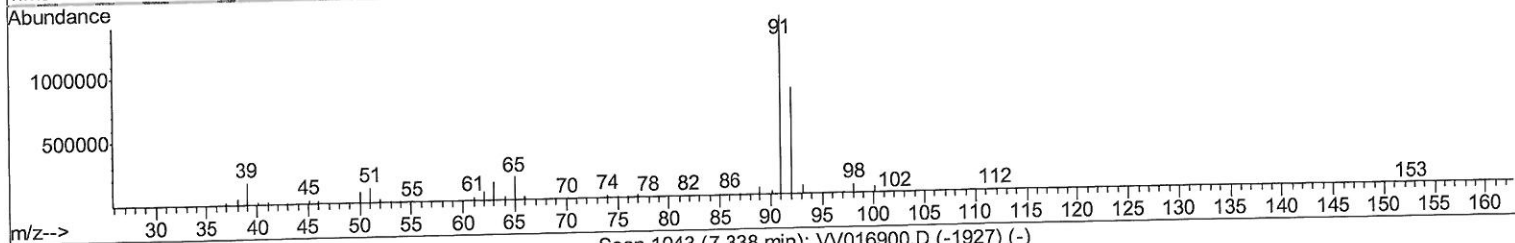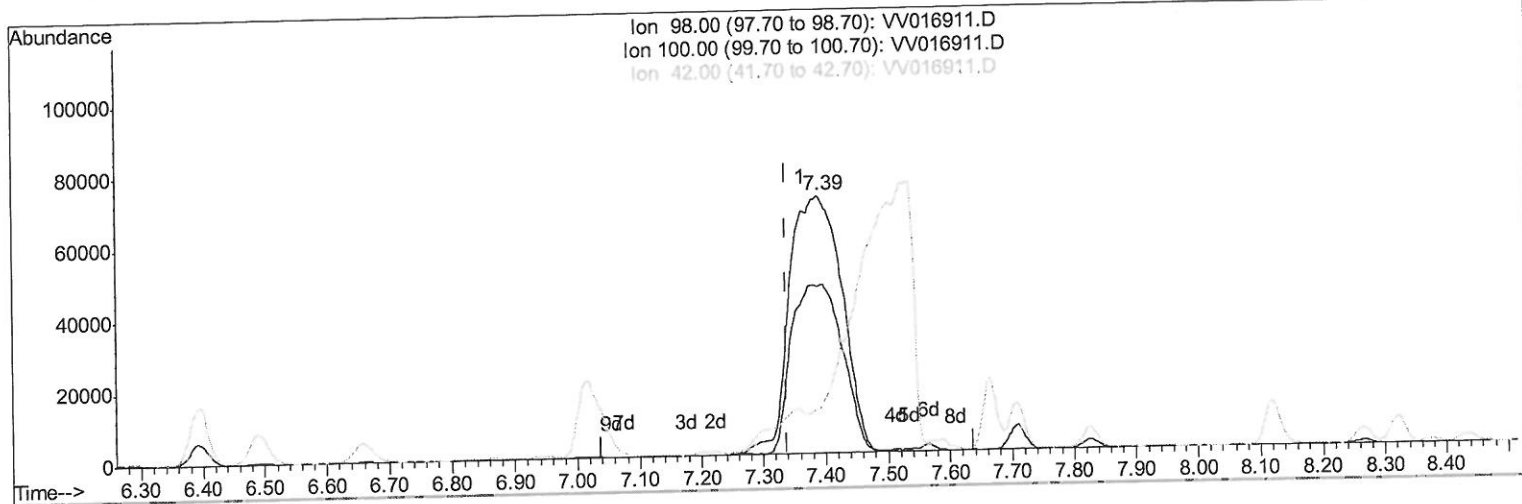

(41) Toluene-d8 (S)

7.389min (+0.052) 45.11ug/L m

response 417417

7 MD
 06/15/20

Ion	Exp%	Act%
98.00	100	100
100.00	65.80	33.77#
42.00	12.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG8MS

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

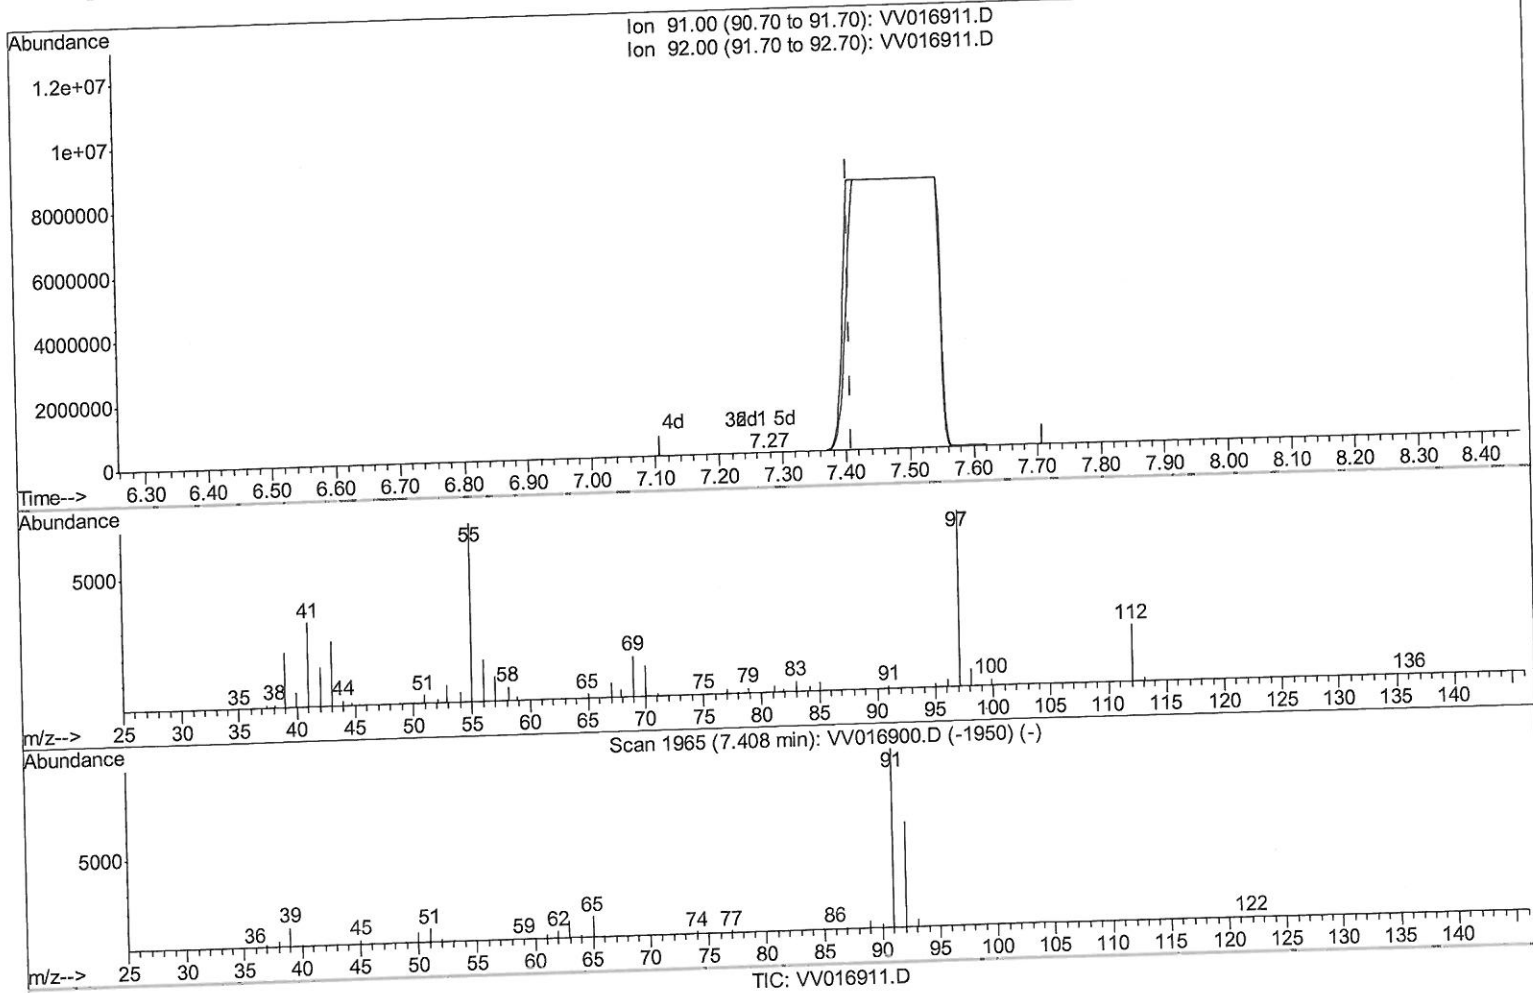

(42) Toluene (T)

7.270min (-0.138) 0.01ug/L

response 161

Ion	Exp%	Act%
91.00	100	100
92.00	57.70	52.48
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 E3YG8MS

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

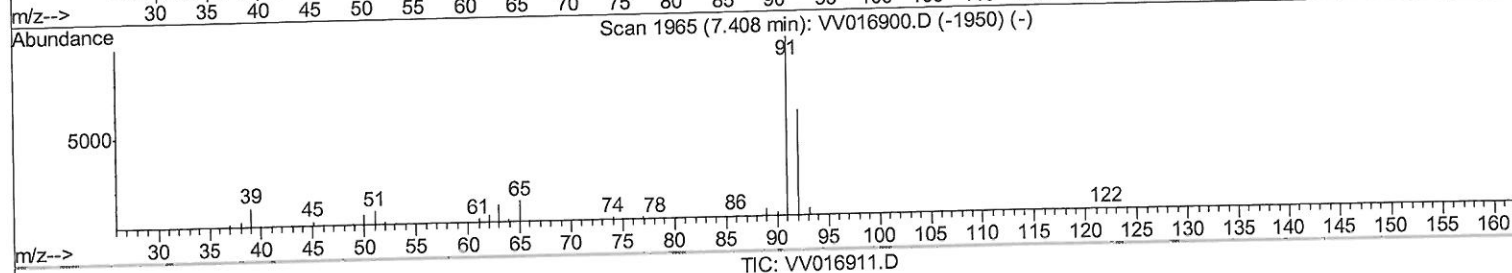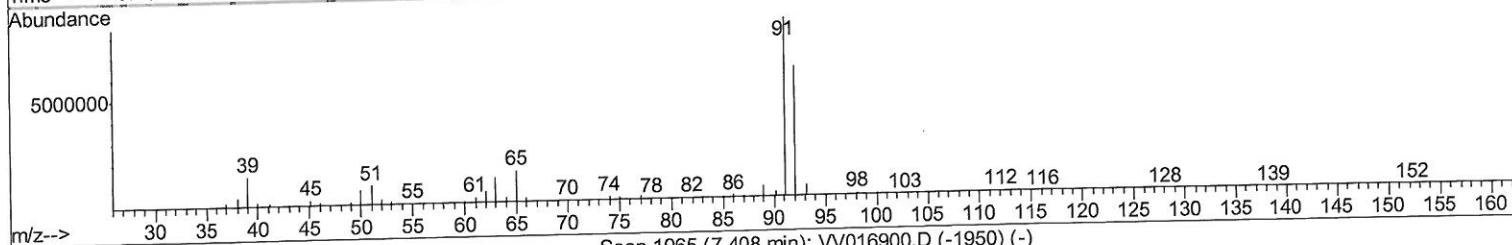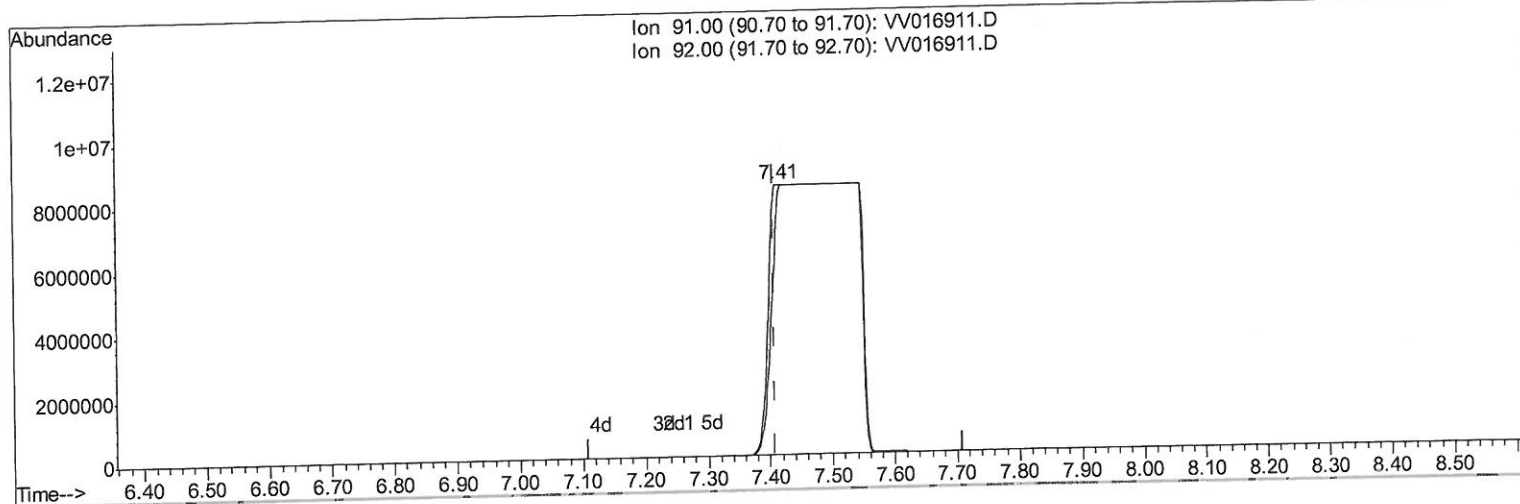

(42) Toluene (T)

7.409min (+0.000) 7217.04ug/L m

response 78742304

MD
06/15/20

Ion	Exp%	Act%
91.00	100	100
92.00	57.70	72.70
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG8MS

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

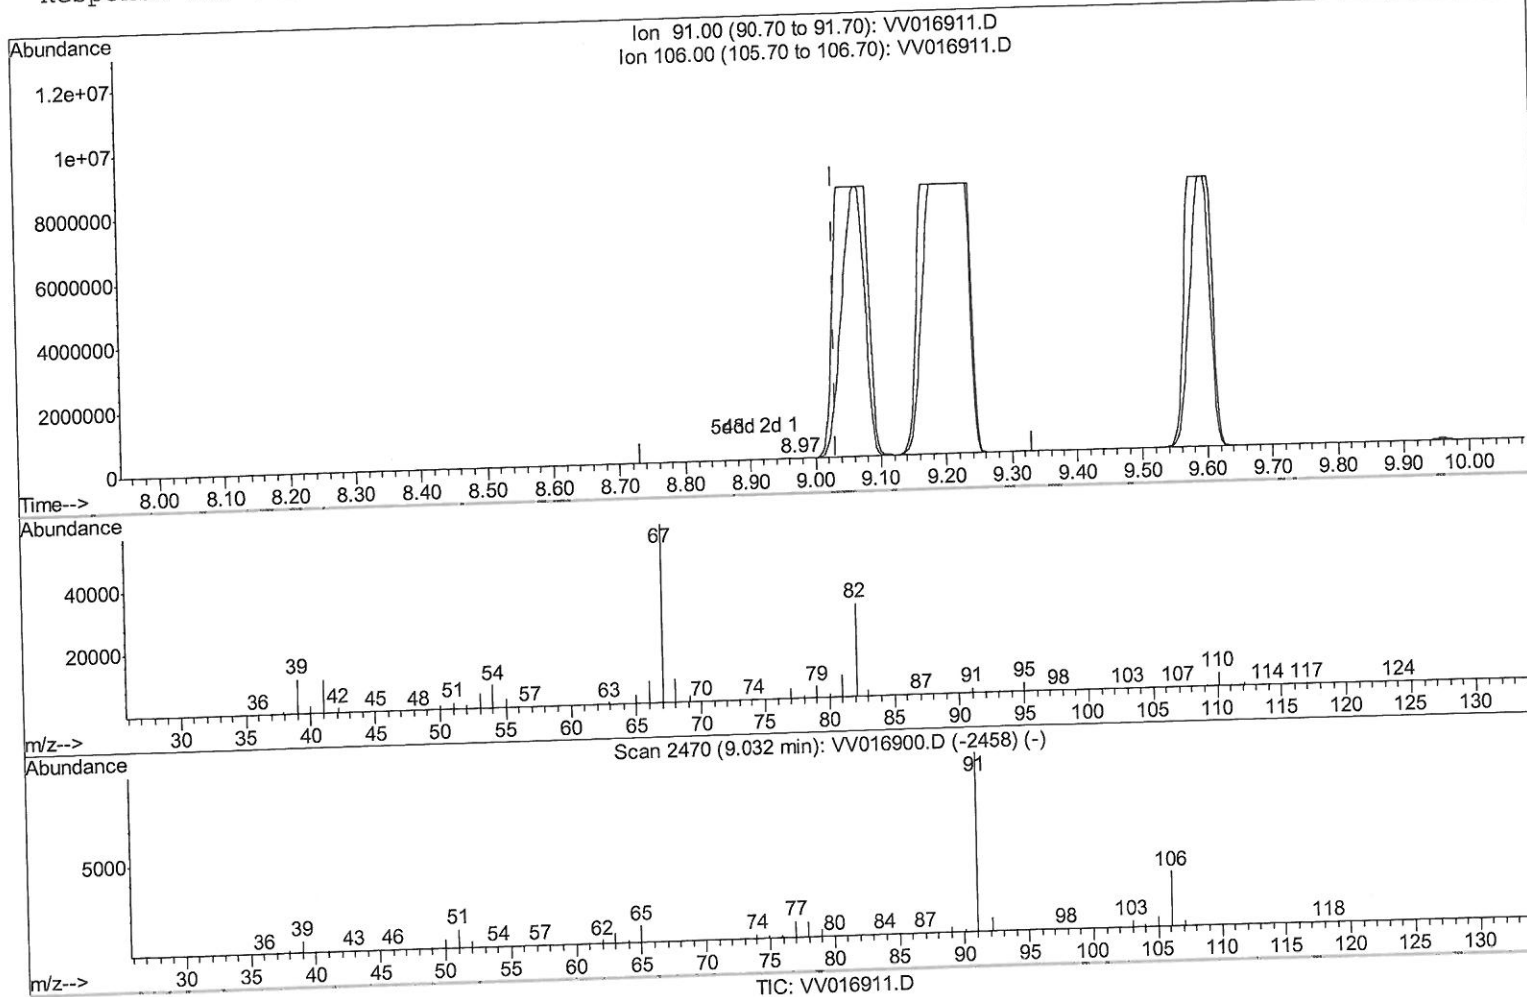

(52) Ethylbenzene (T)

8.968min (-0.064) 0.09ug/L

response 1035

Ion	Exp%	Act%
91.00	100	100
106.00	30.10	8.67#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG8MS

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

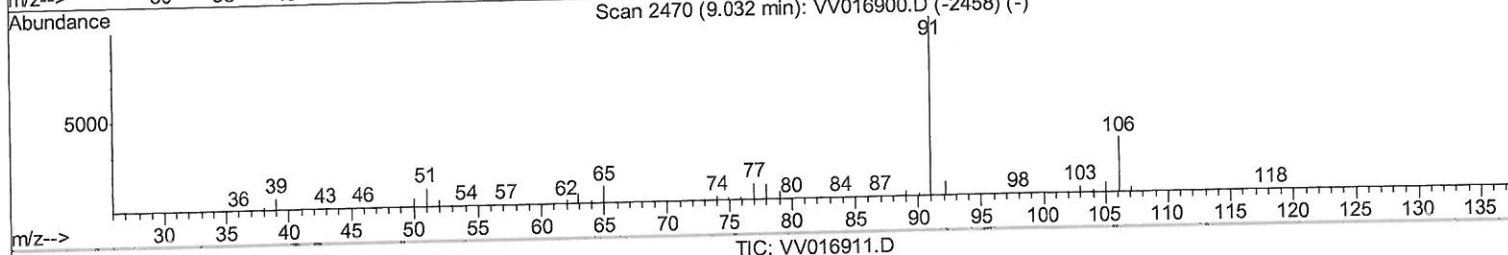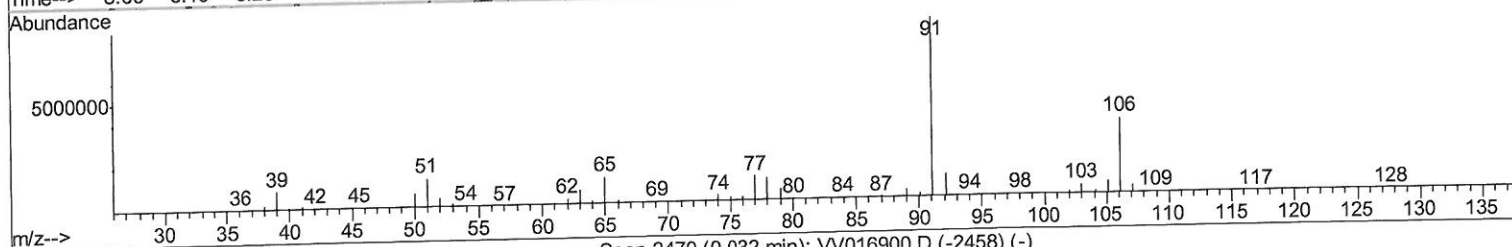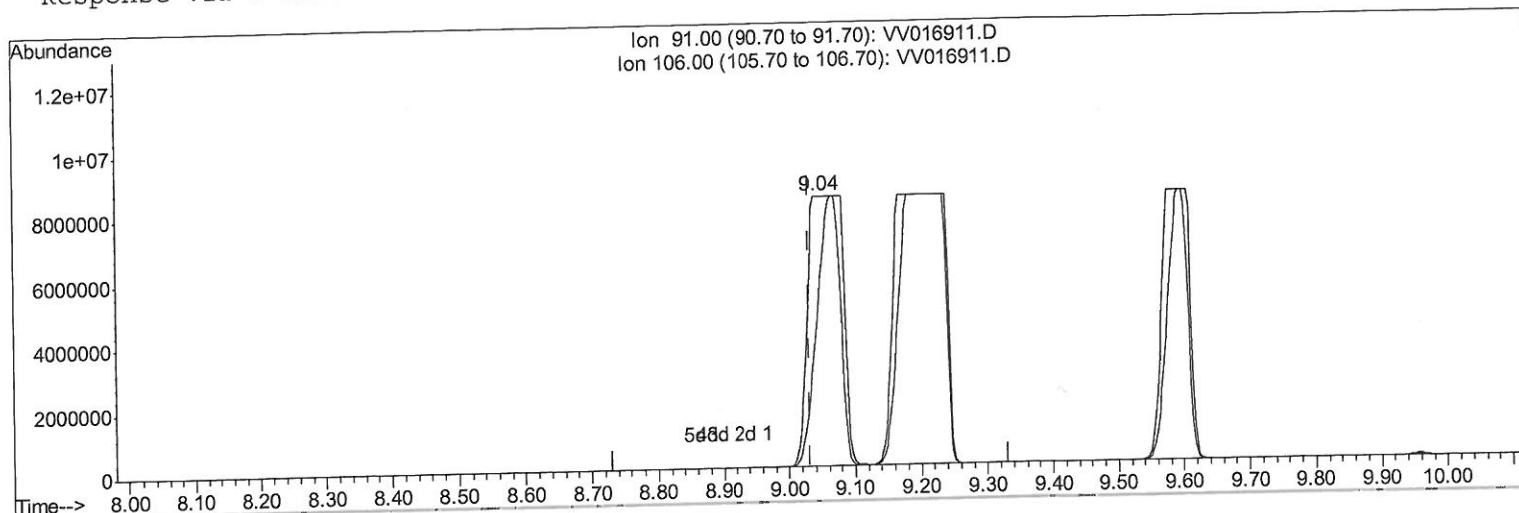

(52) Ethylbenzene (T)

9.039min (+0.007) 2538.80ug/L m

response 30681271

Ion Exp% Act%

91.00 100 100

106.00 30.10 42.08#

0.00 0.00 0.00

0.00 0.00 0.00

MD
 06/15/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 E3YG8MS

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

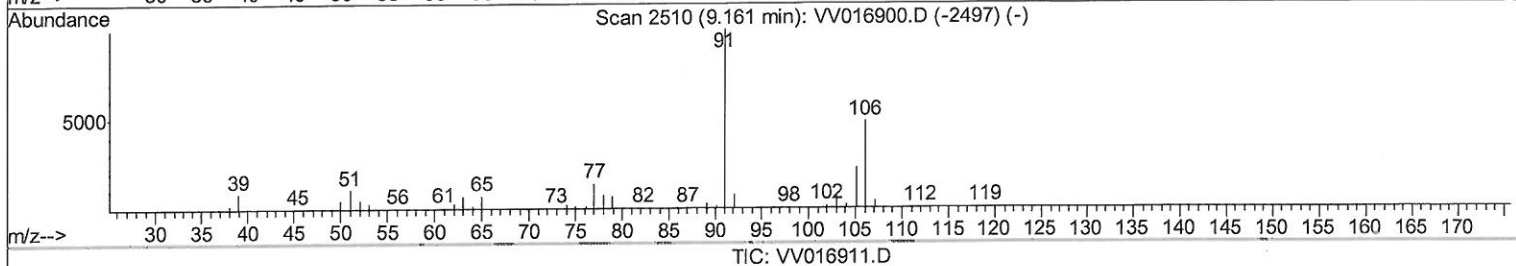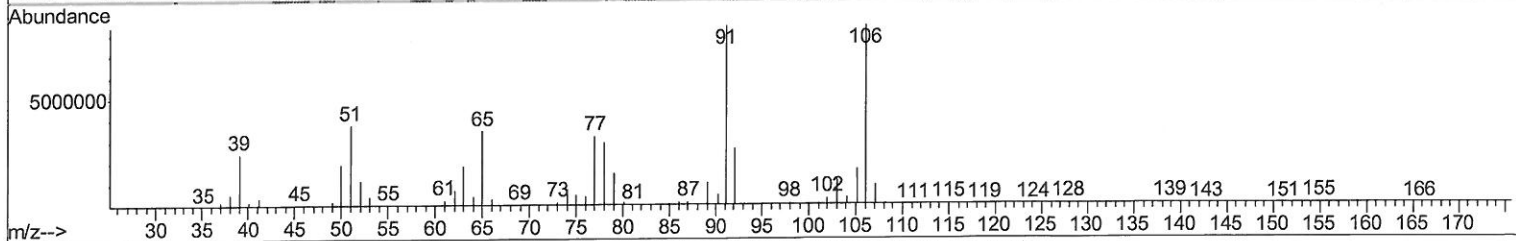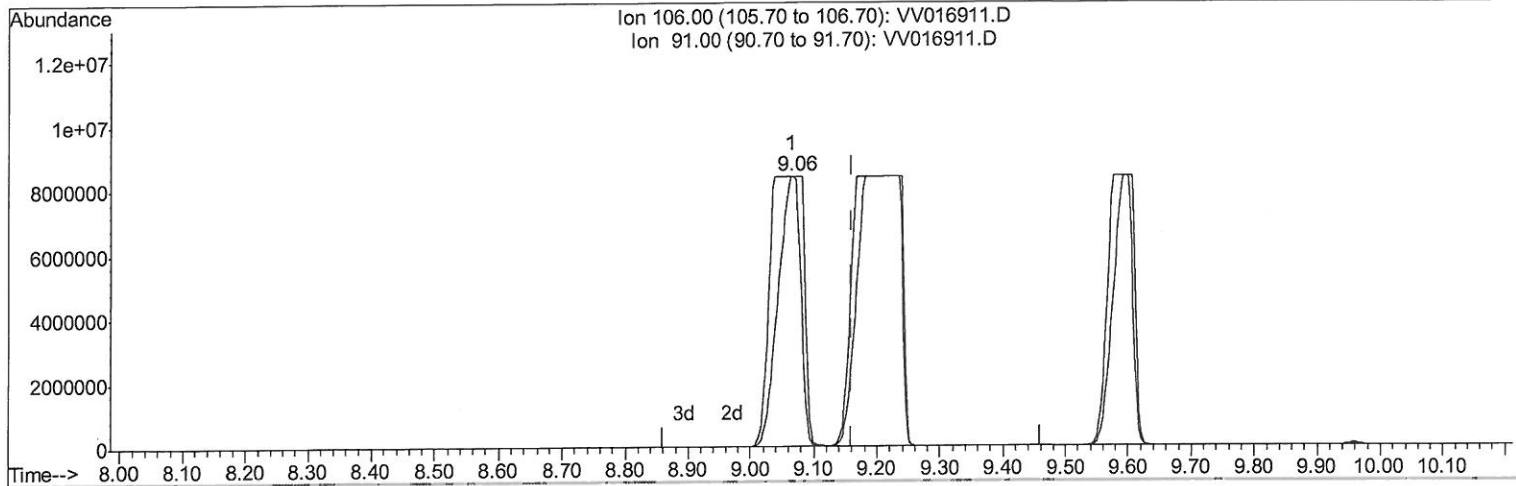

(53) m,p-Xylene (T)

9.064min (-0.096) 4512.56ug/L

response 20304737

Ion	Exp%	Act%
106.00	100	100
91.00	206.60	100.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 E3YG8MS

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

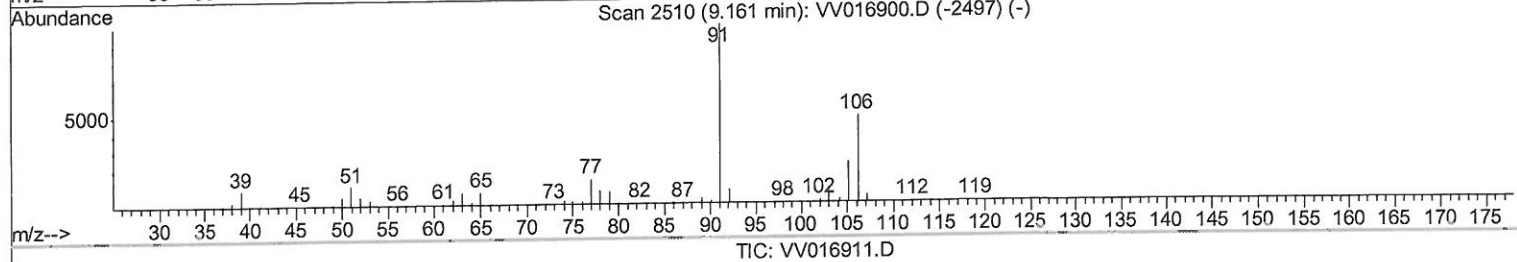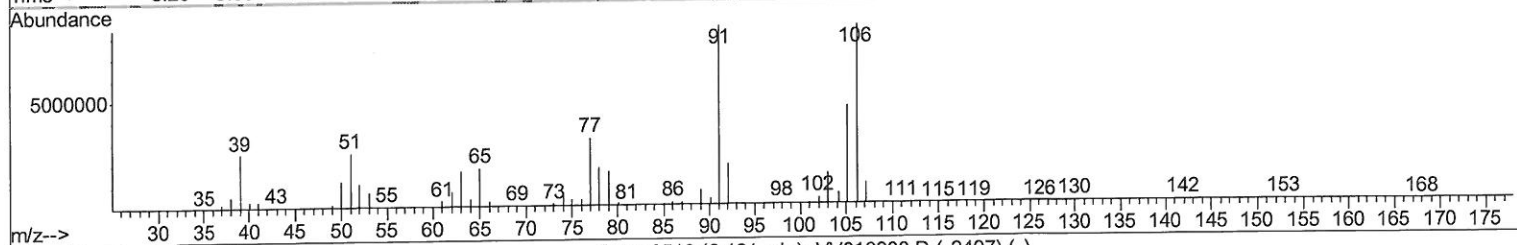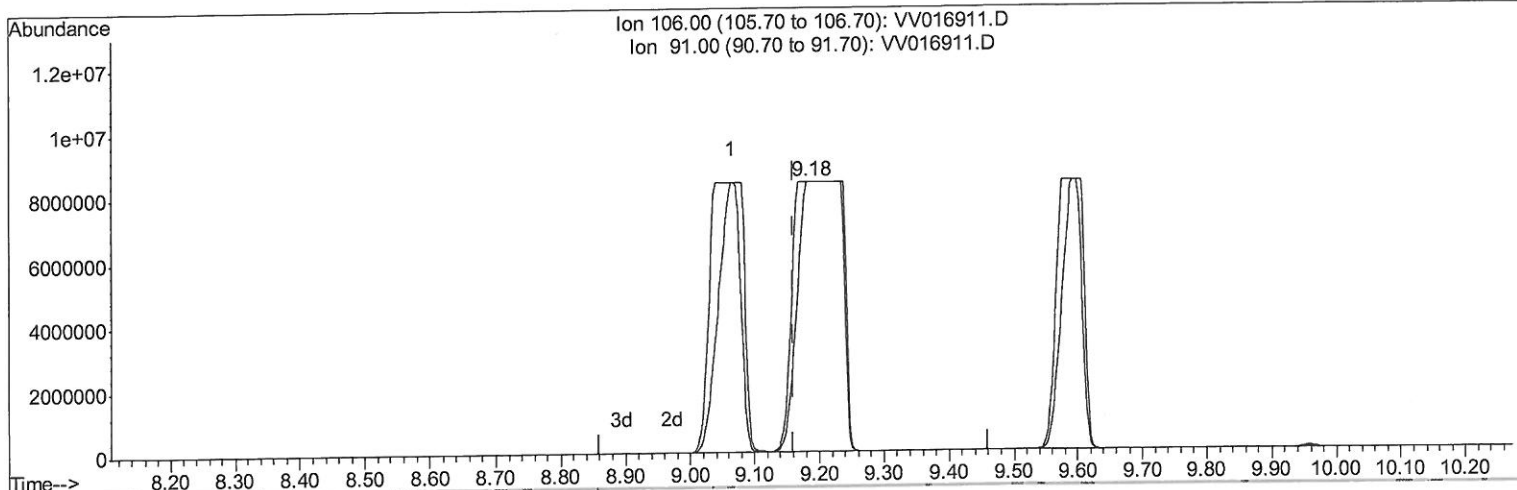

(53) m,p-Xylene (T)

9.180min (+0.019) 8689.34ug/L m

response 39098605

Ion	Exp%	Act%
106.00	100	100
91.00	206.60	100.00#
0.00	0.00	0.00
0.00	0.00	0.00

7 MB
06/15/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 E3YG8MS

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

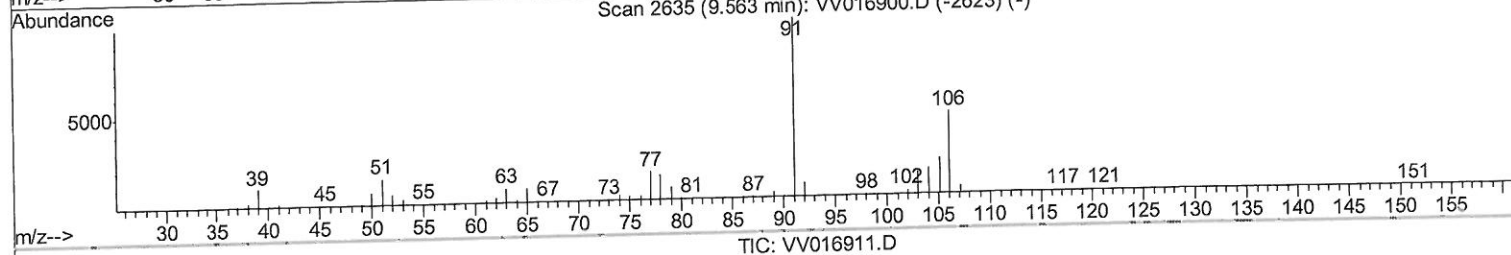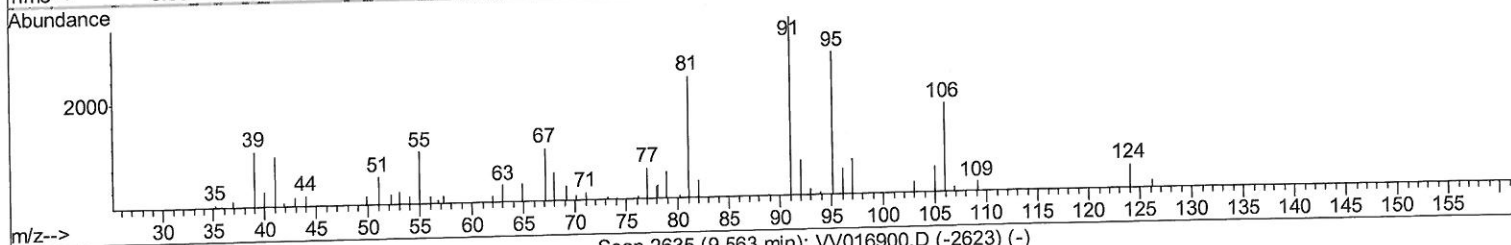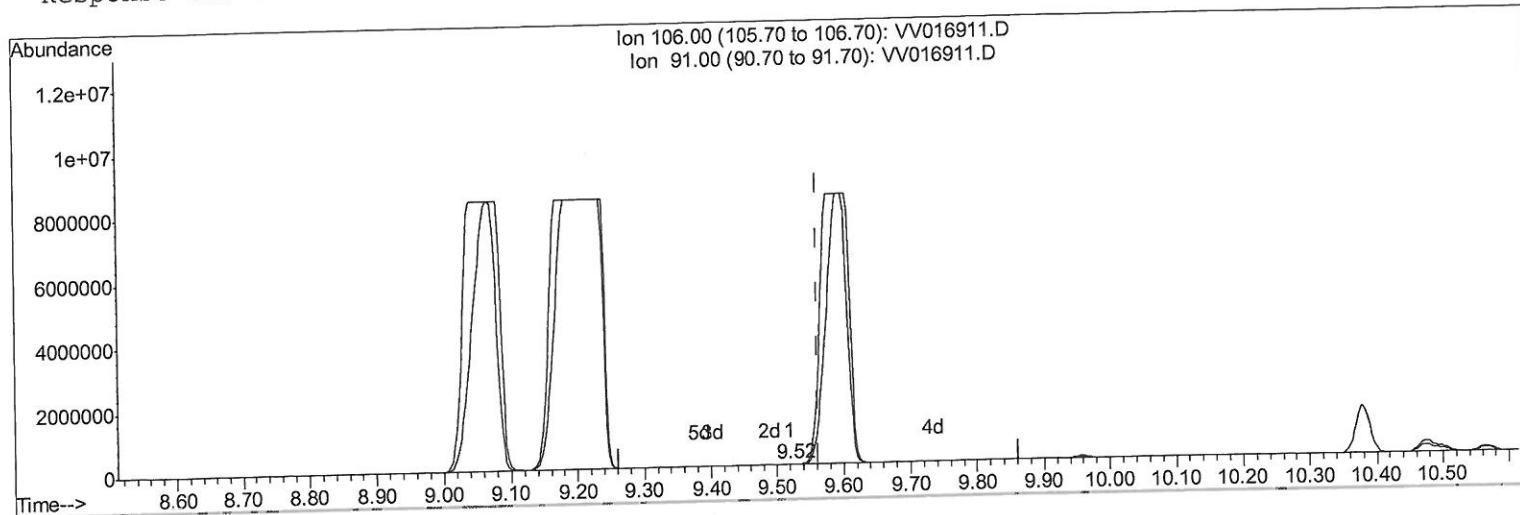

(54) o-xylene (T)

9.521min (-0.042) 0.04ug/L

response 187

Ion	Exp%	Act%
106.00	100	100
91.00	222.70	195.20
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG8MS

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

Quant Time: Jun 13 06:16:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

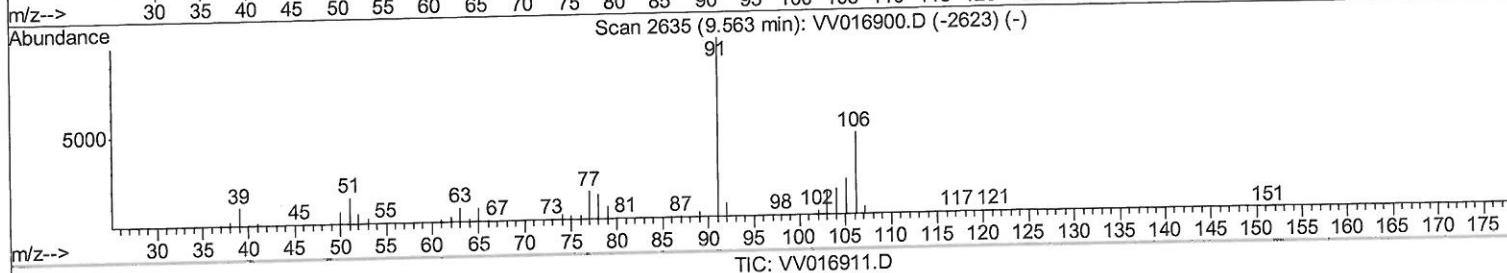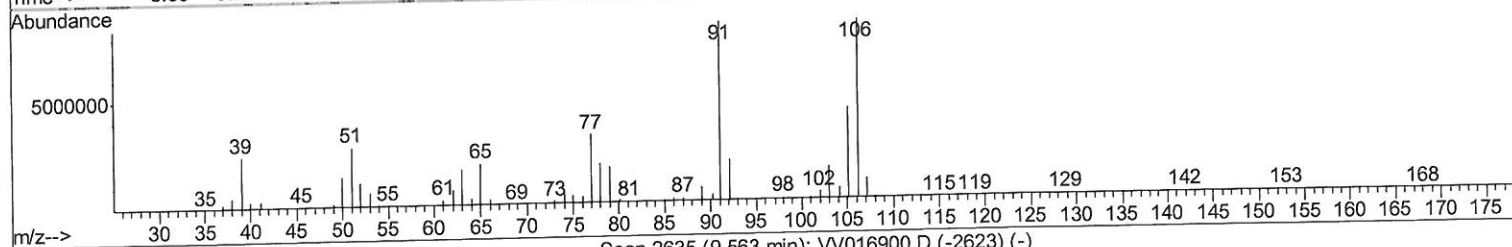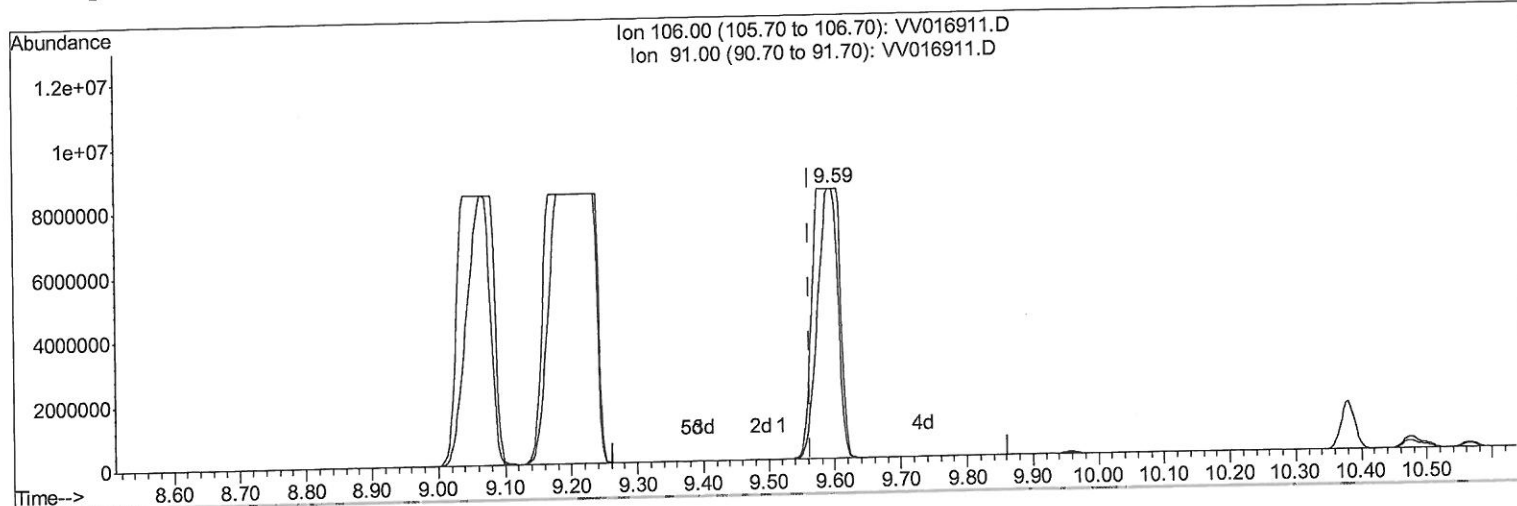

(54) o-xylene (T)

9.592min (+0.029) 4045.09ug/L m

response 17951114

Ion Exp% Act%

106.00 100 100

91.00 222.70 100.00#

0.00 0.00 0.00

0.00 0.00 0.00

7m8
06/15/20

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 E3YG8MS

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

Quant Time: Jun 13 07:18:13 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M

Quant Title : VOC Analysis

QLast Update : Sat Jun 13 06:09:05 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.65	114	370686	50.00	uq/L	0.00
28) Chlorobenzene-d5	8.88	117	349807	50.00	uq/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	191156	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	103136	39.43	uq/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.86%
7) Chloroethane-d5	1.57	69	62278	39.68	uq/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.36%
11) 1,1-Dichloroethane-d2	2.12	63	206634	47.05	uq/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.10%
21) 2-Butanone-d5	3.90	46	173724	89.74	uq/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.74%
24) Chloroform-d	4.38	84	224146	42.14	uq/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.28%
26) 1,2-Dichloroethane-d4	5.06	65	170633	47.17	uq/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.34%
32) Benzene-d6	5.08	84	434654	43.10	uq/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.20%
36) 1,2-Dichloropropane-d6	6.10	67	132828	42.26	uq/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.52%
41) Toluene-d8	7.39	98	417417m	45.11	uq/L	0.05
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.22%
43) trans-1,3-Dichloropropene-	7.66	79	66378	40.55	uq/L	0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.10%
47) 2-Hexanone-d5	8.12	63	113092	82.53	uq/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.53%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	169521	40.74	uq/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	81.48%
64) 1,2-Dichlorobenzene-d4	11.65	152	176895	43.36	uq/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.72%

MD
 06/15/20

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.32	62	11036	4.176	uq/L	# 78
12) 1,1-Dichloroethene	2.13	96	91994	50.002	uq/L	93
13) Acetone	2.18	43	3606	2.827	uq/L	75
15) Methyl Acetate	2.44	43	54932	19.322	uq/L	99
19) 1,1-Dichloroethane	3.21	63	28722	6.083	uq/L	99
20) cis-1,2-Dichloroethene	3.94	96	81321	29.736	uq/L	98
29) Cyclohexane	4.70	56	455113	104.698	uq/L	98
30) 1,1,1-Trichloroethane	4.64	97	4321	0.969	uq/L	# 86
33) Benzene	5.13	78	477978	46.182	uq/L	100
34) Trichloroethene	5.94	95	132206	47.629	uq/L	98
35) Methylcyclohexane	6.16	83	2579740	592.418	uq/L	98
42) Toluene	7.41	91	78742304m	7217.036	uq/L	98
51) Chlorobenzene	8.91	112	353808	49.704	uq/L	
52) Ethylbenzene	9.04	91	30681271m	2538.802	uq/L	
53) m,p-Xylene	9.18	106	39098605m	8689.336	uq/L	
54) o-xylene	9.59	106	17951114m	4045.093	uq/L	
56) Isopropylbenzene	9.96	105	1137689	95.411	ug/L	100

MD
 06/15/20

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016911.D
 Acq On : 13 Jun 2020 04:53
 Operator : SY/MD
 Sample : L2990-13MS
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E3YG8MS

Quant Time: Jun 13 07:18:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 06:09:05 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/15/2020 12:23:12 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
65) 1,2-Dichlorobenzene	11.67	146	29916	4.931	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed