

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016888.D
 Acq On : 12 Jun 2020 18:59
 Operator : SY/MD
 Sample : L2913-09 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E49

Quant Time: Jun 13 03:37:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 03:02:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	367147	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	341301	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	170208	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	95347	36.80	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.60%
7) Chloroethane-d5	1.56	69	72864	46.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.74%
11) 1,1-Dichloroethene-d2	2.12	63	137749	31.66	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.32%
21) 2-Butanone-d5	3.89	46	173065	90.26	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.26%
24) Chloroform-d	4.37	84	227773	43.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.48%
26) 1,2-Dichloroethane-d4	5.05	65	164175	45.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.64%
32) Benzene-d6	5.07	84	437082	44.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.86%
36) 1,2-Dichloropropane-d6	6.09	67	134811	43.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.92%
41) Toluene-d8	7.34	98	396705	43.94	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.88%
43) trans-1,3-Dichloropropene-	7.64	79	67787	42.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.88%
47) 2-Hexanone-d5	8.11	63	102772	76.87	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.87%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	175052	43.12	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.24%
64) 1,2-Dichlorobenzene-d4	11.65	152	170033	46.81	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.62%

Target Compounds


					Ovalue
15) Methyl Acetate	2.45	43	2656	0.943 ug/L	97
29) Cyclohexane	4.70	56	6889	1.624 ug/L	# 93
33) Benzene	5.12	78	1978559	195.933 ug/L	100
42) Toluene	7.41	91	61138	5.743 ug/L	94
52) Ethylbenzene	9.04	91	124974	10.599 ug/L	96
53) m,p-Xylene	9.16	106	17048	3.883 ug/L	99
54) o-xylene	9.57	106	16258	3.755 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016888.D
Acq On : 12 Jun 2020 18:59
Operator : SY/MD
Sample : L2913-09 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E49

Quant Time: Jun 13 03:37:05 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 13 03:02:20 2020
Response via : Initial Calibration




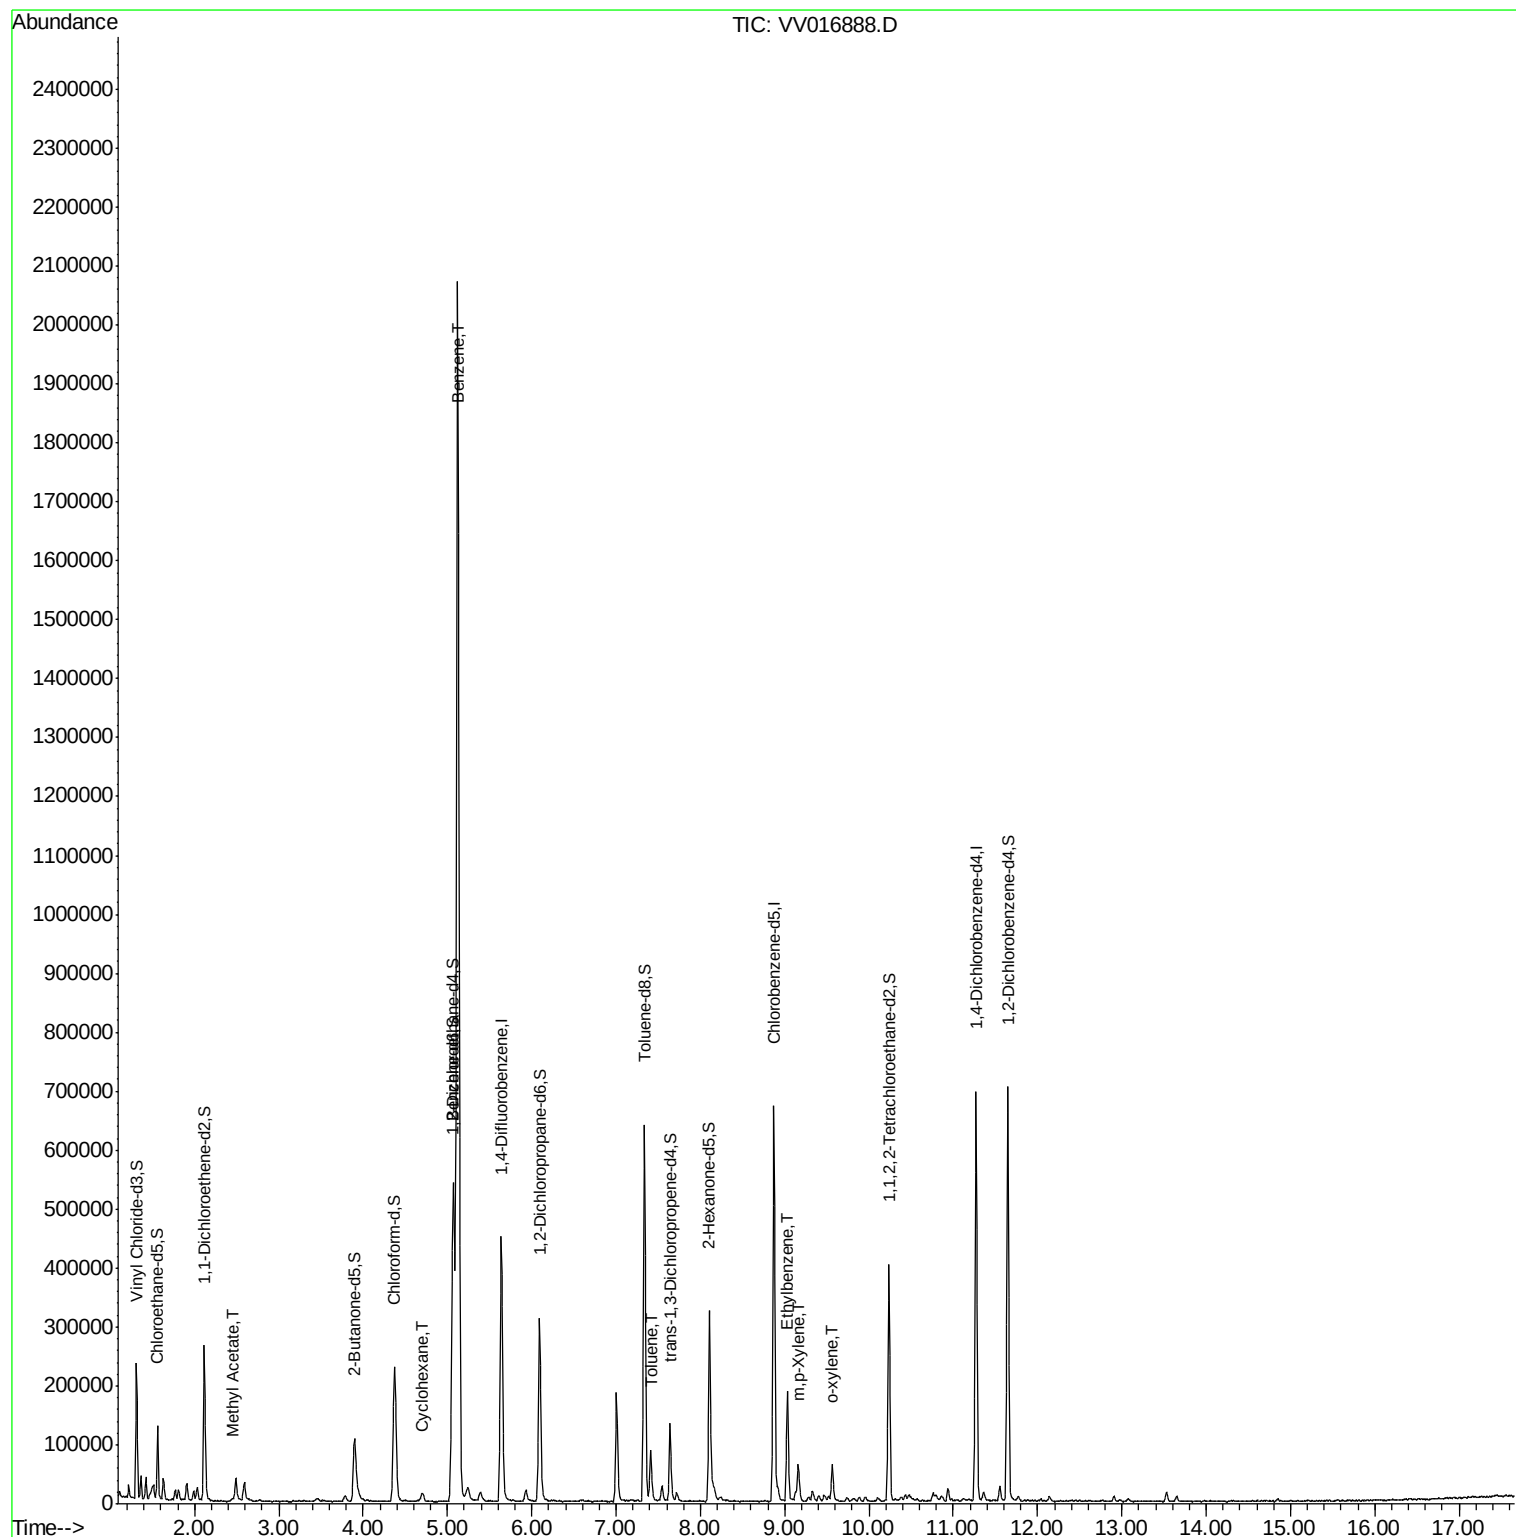


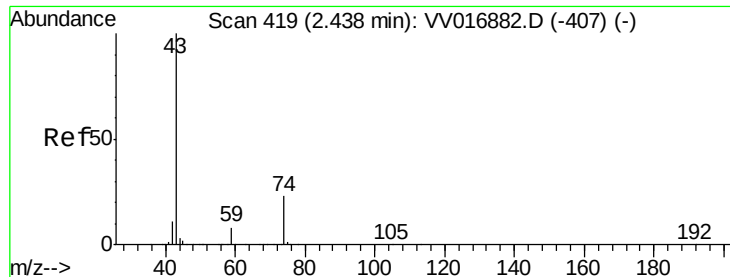

#15
Methvl Acetate
Concen: 0.943 ug/L
RT: 2.45 min Scan# 422
Delta R.T. 0.01 min
Lab File: VV016888.D
Acq: 12 Jun 2020 18:59




Instrument :
MSVOA_V
ClientSampled :
F9E49


Tot Ion: 43 Resp: 2656
Ion Ratio Lower Upper
43 100
74 21.0 17.9 26.9

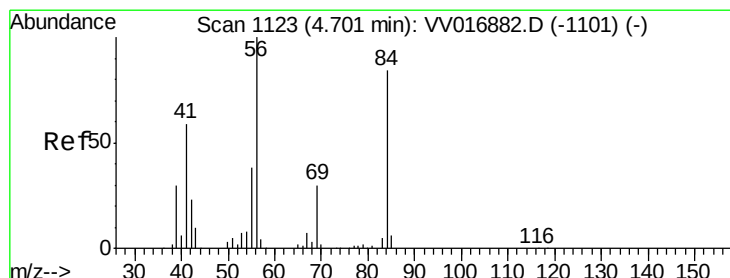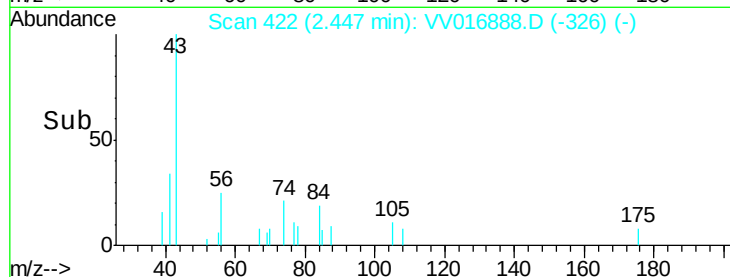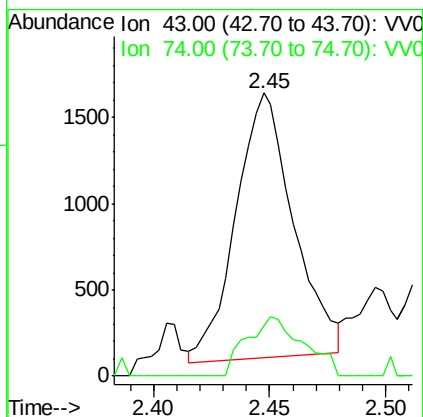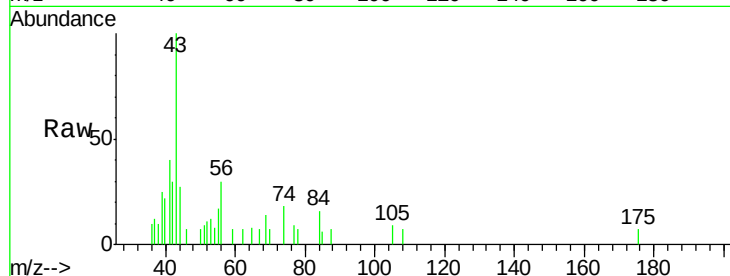

#29
Cyclohexane
Concen: 1.624 ug/L
RT: 4.70 min Scan# 1123
Delta R.T. 0.00 min
Lab File: VV016888.D
Acq: 12 Jun 2020 18:59

Tgt Ion: 56 Resp: 6889
Ion Ratio Lower Upper
56 100
69 21.6 25.0 37.4#
84 83.8 69.5 104.3

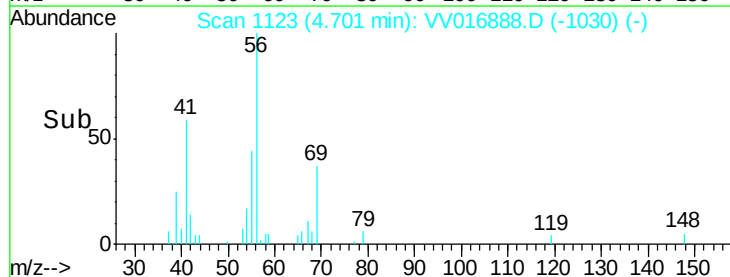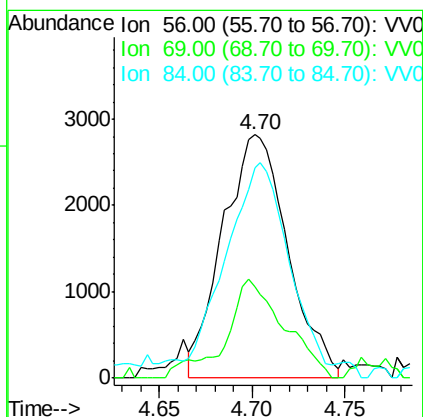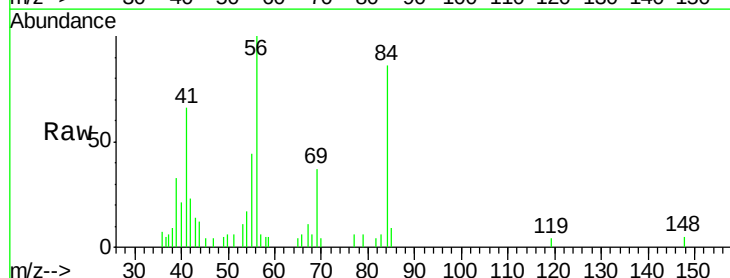

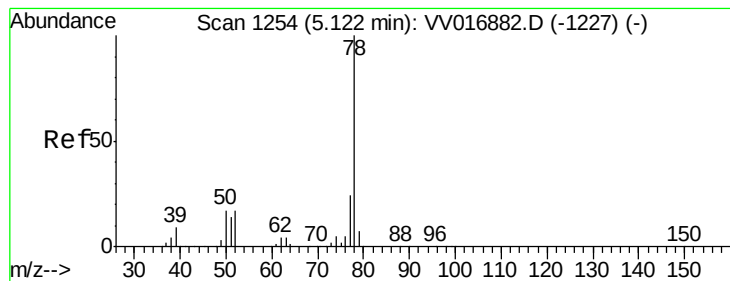

#33

Benzene

Concen: 195.933 ug/L

RT: 5.12 min Scan# 1254

Delta R.T. 0.00 min

Lab File: VV016888.D

Acq: 12 Jun 2020 18:59


Instrument :

MSVOA_V




ClientSampleId :

F9E49

Tgt Ion: 78 Resp: 1978559

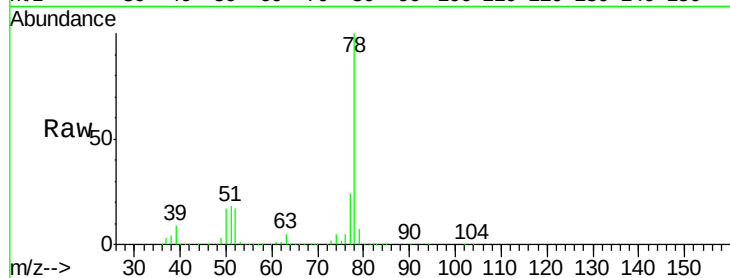

Abundance Ion 78.00 (77.70 to 78.70): VV0

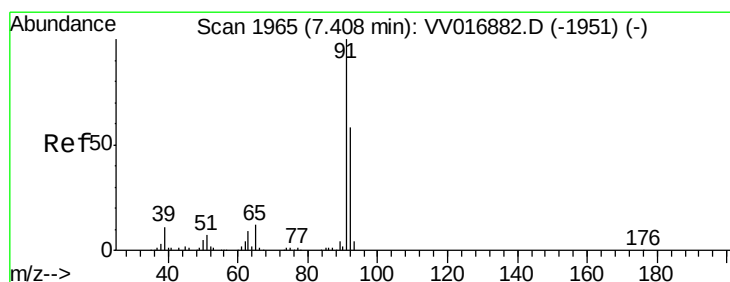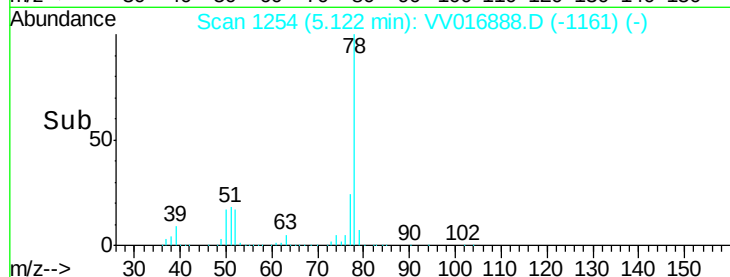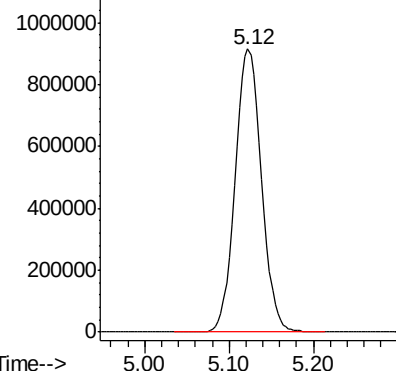

#42

Toluene

Concen: 5.743 ug/L

RT: 7.41 min Scan# 1966

Delta R.T. 0.00 min

Lab File: VV016888.D


Acq: 12 Jun 2020 18:59

Tgt Ion: 91 Resp: 61138



Ion Ratio Lower Upper


91 100

92 53.2 40.4 75.0

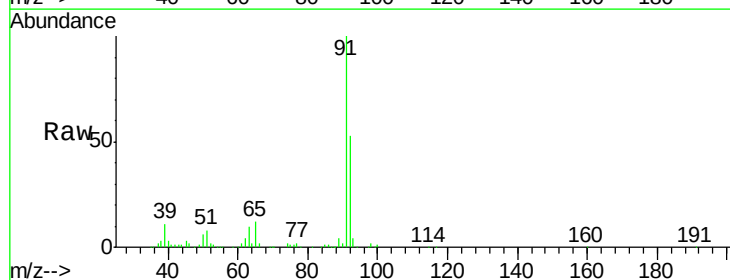

Abundance Ion 91.00 (90.70 to 91.70): VV0

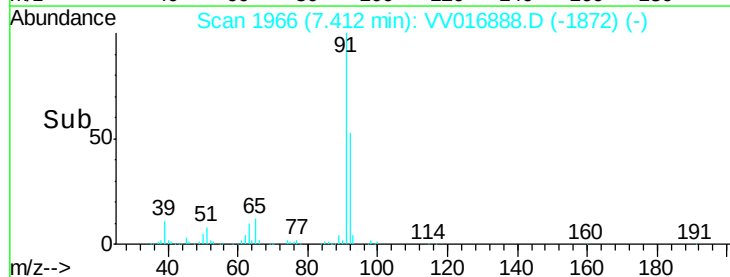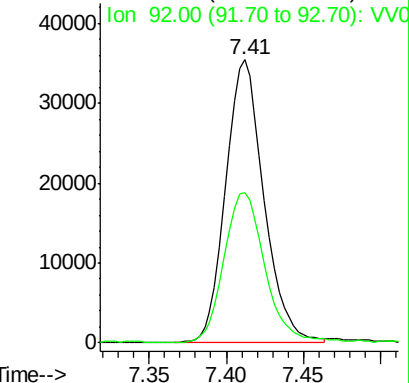

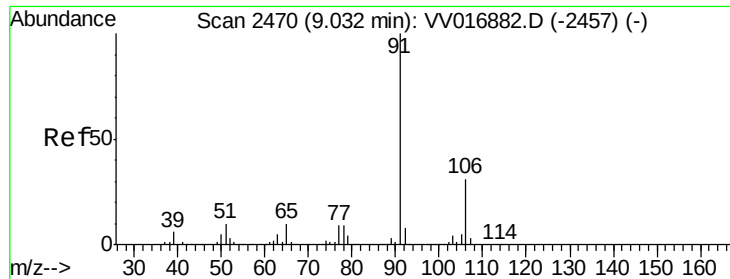

#52

Ethylbenzene

Concen: 10.599 ug/L

RT: 9.04 min Scan# 2471

Delta R.T. 0.00 min

Lab File: VV016888.D

Acq: 12 Jun 2020 18:59

Instrument :

MSVOA_V

ClientSampleId :


F9E49

Tot Ion: 91 Resp: 124974

Ion Ratio Lower Upper




91 100

106 32.0 21.1 39.1

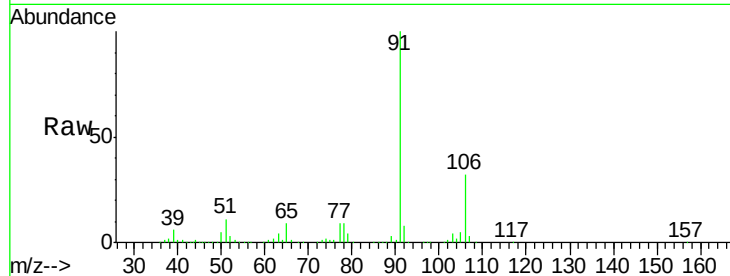

Abundance Ion 91.00 (90.70 to 91.70): VV016888.D (-2377) (-)

Ion 106.00 (105.70 to 106.70): VV016888.D (-2377) (-)

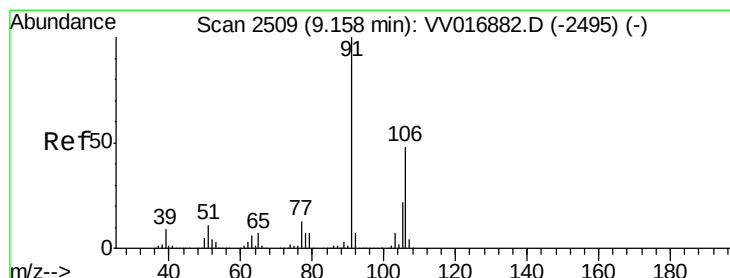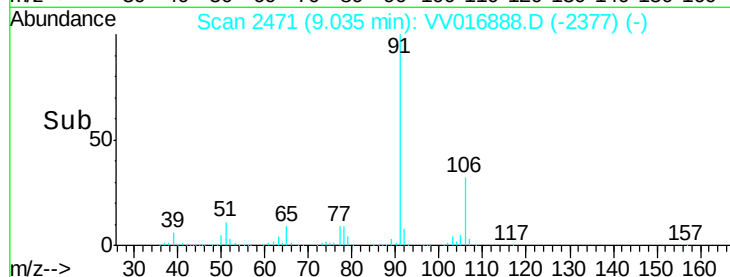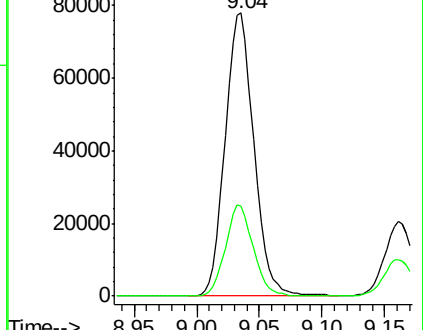

#53

m,p-Xylene

Concen: 3.883 ug/L

RT: 9.16 min Scan# 2510

Delta R.T. 0.00 min

Lab File: VV016888.D


Acq: 12 Jun 2020 18:59

Tgt Ion: 106 Resp: 17048

Ion Ratio Lower Upper



106 100


91 205.8 144.6 268.6

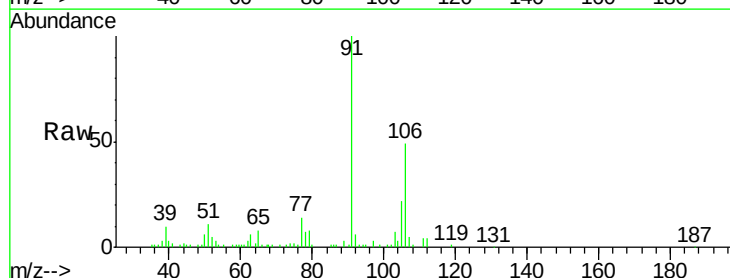

Abundance Ion 106.00 (105.70 to 106.70): VV016888.D (-2416) (-)

Ion 91.00 (90.70 to 91.70): VV016888.D (-2416) (-)

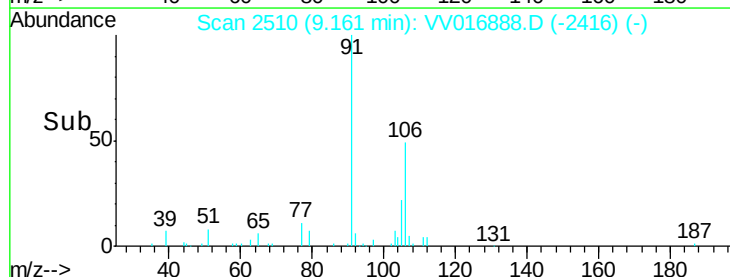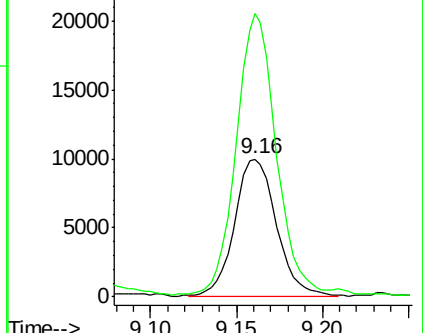

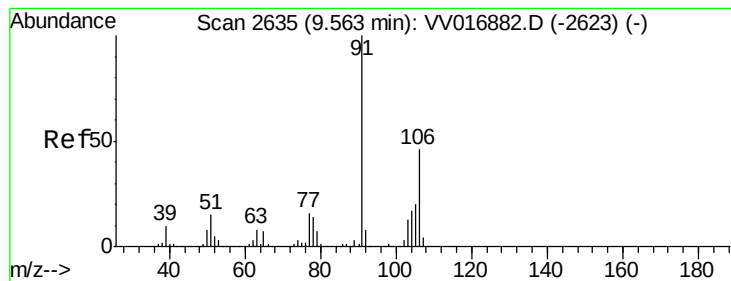

#54
 o-xylene
 Concen: 3.755 ug/L
 RT: 9.57 min Scan# 2636
 Delta R.T. 0.00 min
 Lab File: VV016888.D
 Acq: 12 Jun 2020 18:59

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E49

Tot Ion:106 Resp: 16258
 Ion Ratio Lower Upper
 106 100
 91 204.8 155.9 289.5

