

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016890.D
 Acq On : 12 Jun 2020 19:46
 Operator : SY/MD
 Sample : L2914-02 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D87

Quant Time: Jun 13 03:44:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 13 03:02:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	357702	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	343496	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	175365	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	91463	36.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.48%
7) Chloroethane-d5	1.56	69	70299	46.42	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.84%
11) 1,1-Dichloroethene-d2	2.12	63	135851	32.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.10%
21) 2-Butanone-d5	3.89	46	165768	88.74	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.74%
24) Chloroform-d	4.37	84	224790	43.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.60%
26) 1,2-Dichloroethane-d4	5.05	65	165573	47.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.86%
32) Benzene-d6	5.07	84	431820	43.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.22%
36) 1,2-Dichloropropane-d6	6.09	67	130355	42.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.46%
41) Toluene-d8	7.34	98	394241	43.39	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.78%
43) trans-1,3-Dichloropropene-	7.64	79	66076	41.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.20%
47) 2-Hexanone-d5	8.11	63	102527	76.19	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.19%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	176341	43.16	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.32%
64) 1,2-Dichlorobenzene-d4	11.65	152	174428	46.61	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.22%

Target Compounds


					Ovalue
29) Cyclohexane	4.70	56	13509	3.165 ug/L	96
33) Benzene	5.12	78	3307068	325.401 ug/L	100
42) Toluene	7.41	91	172996	16.147 ug/L	99
52) Ethylbenzene	9.03	91	257661	21.713 ug/L	98
53) m,p-Xylene	9.16	106	17832	4.036 ug/L	95
54) o-xylene	9.56	106	35009	8.034 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016890.D
Acq On : 12 Jun 2020 19:46
Operator : SY/MD
Sample : L2914-02 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D87

Quant Time: Jun 13 03:44:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 13 03:02:20 2020
Response via : Initial Calibration




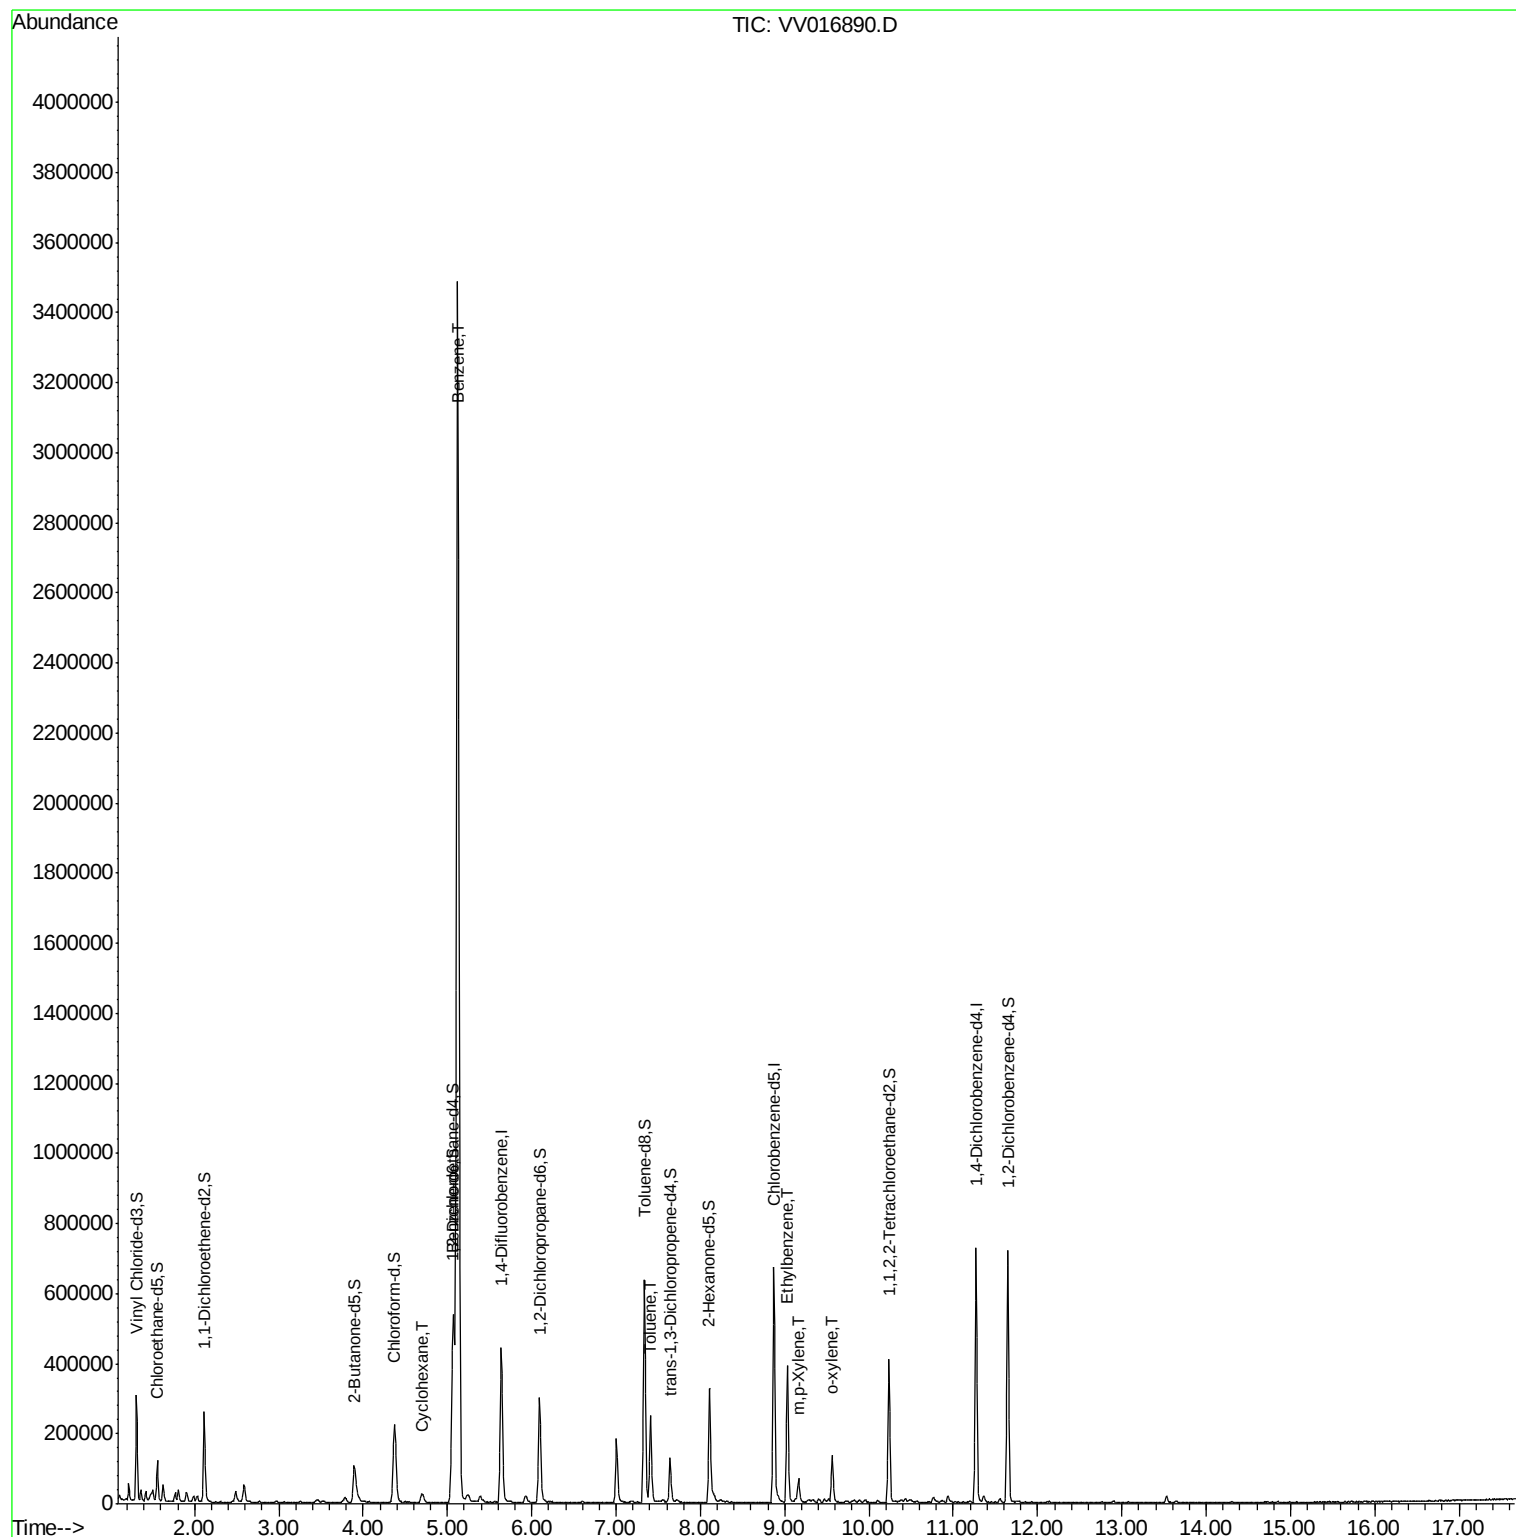


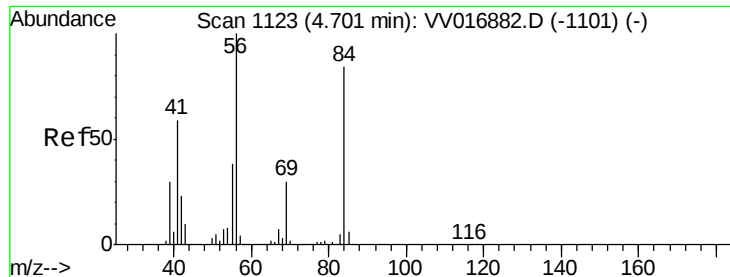




#29
Cyclohexane
Concen: 3.165 ug/L
RT: 4.70 min Scan# 1122
Delta R.T. -0.00 min
Lab File: VV016890.D
Acq: 12 Jun 2020 19:46


Instrument :
MSVOA_V
ClientSampleId :
F9D87

Tot Ion: 56 Resp: 13509
Ion Ratio Lower Upper
56 100
69 30.7 25.0 37.4
84 82.1 69.5 104.3

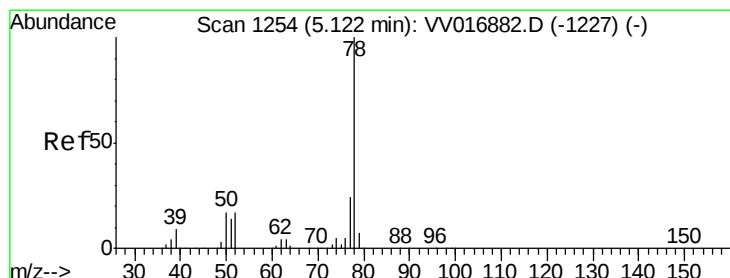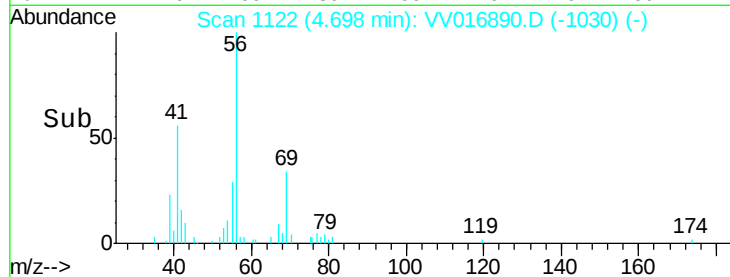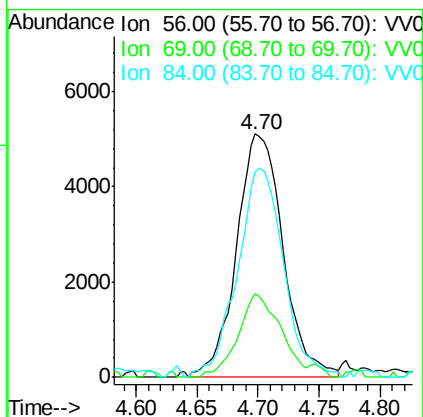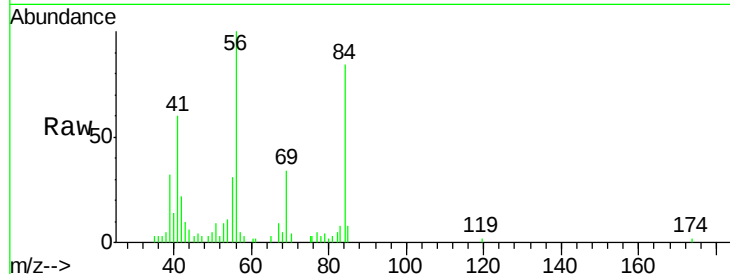

#33
Benzene
Concen: 325.401 ug/L
RT: 5.12 min Scan# 1254
Delta R.T. -0.00 min
Lab File: VV016890.D
Acq: 12 Jun 2020 19:46
Tgt Ion: 78 Resp: 3307068

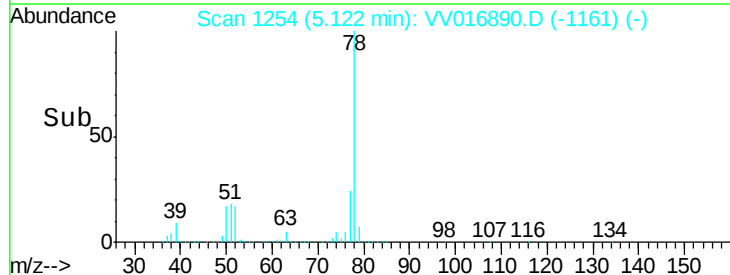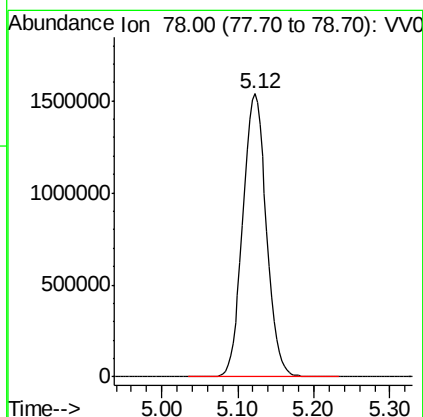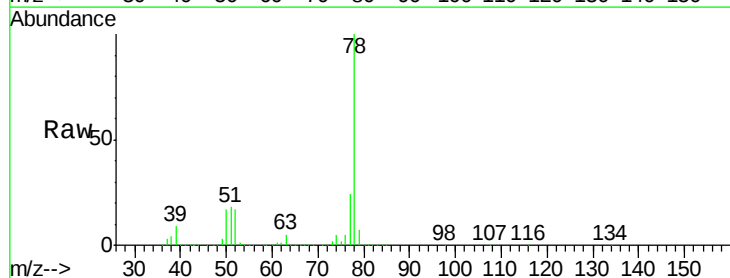

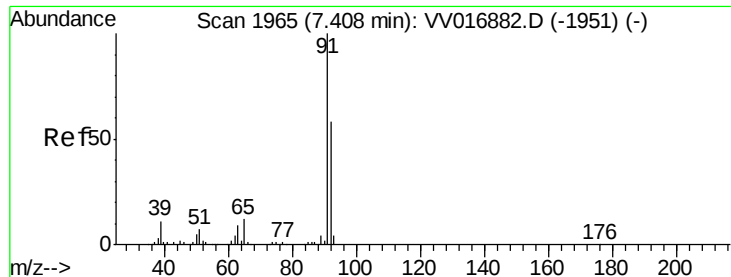

#42

Toluene

Concen: 16.147 ug/L

RT: 7.41 min Scan# 1965

Delta R.T. -0.00 min

Lab File: VV016890.D

Acq: 12 Jun 2020 19:46

Instrument :

MSVOA_V

ClientSampleId :


F9D87

Tot Ion: 91 Resp: 172996

Ion Ratio Lower Upper




91 100

92 58.6 40.4 75.0

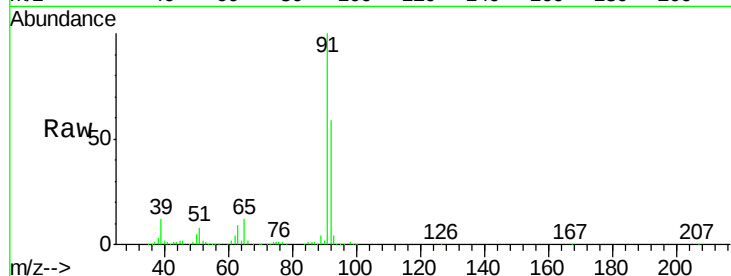

Abundance Ion 91.00 (90.70 to 91.70): VV0

Ion 92.00 (91.70 to 92.70): VV0

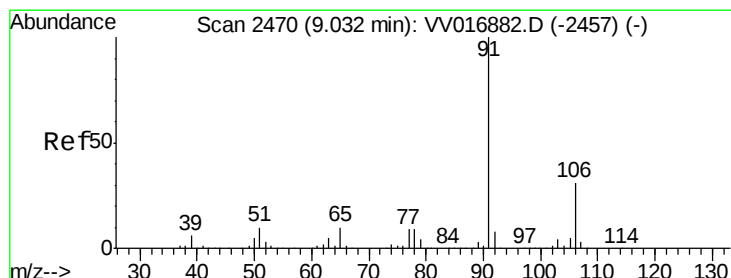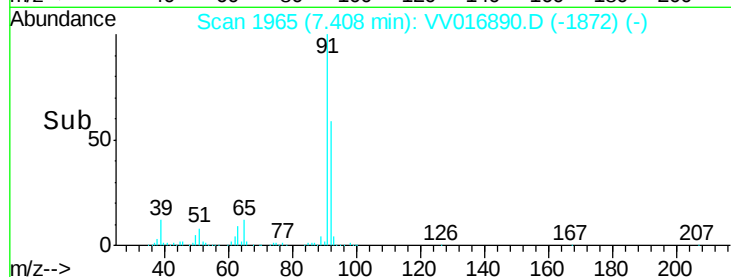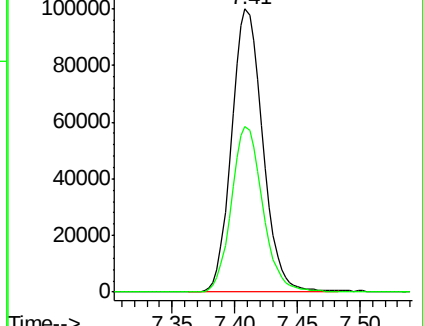

#52

Ethylbenzene

Concen: 21.713 ug/L

RT: 9.03 min Scan# 2470

Delta R.T. -0.00 min

Lab File: VV016890.D


Acq: 12 Jun 2020 19:46

Tgt Ion: 91 Resp: 257661

Ion Ratio Lower Upper



91 100


106 31.3 21.1 39.1

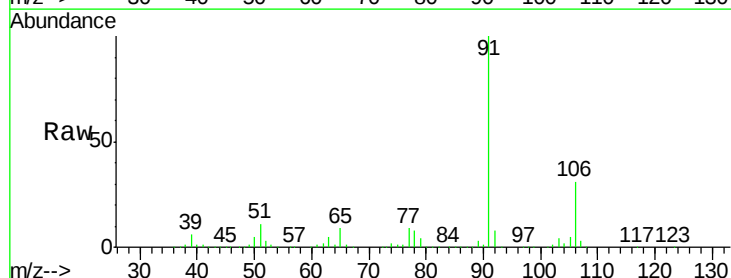

Abundance Ion 91.00 (90.70 to 91.70): VV0

Ion 106.00 (105.70 to 106.70): V

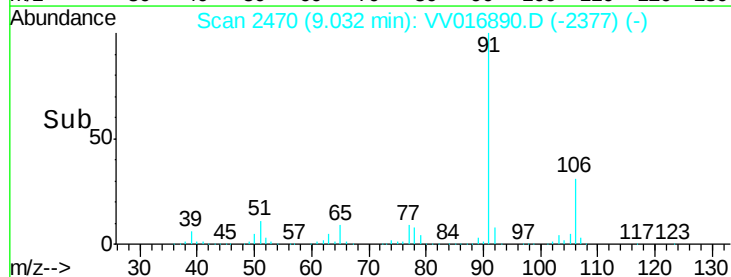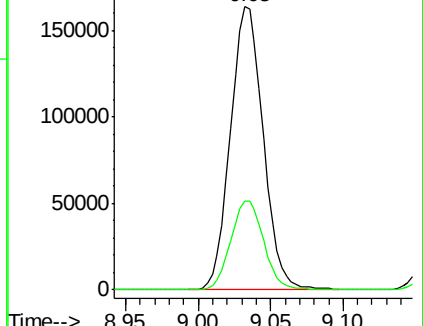

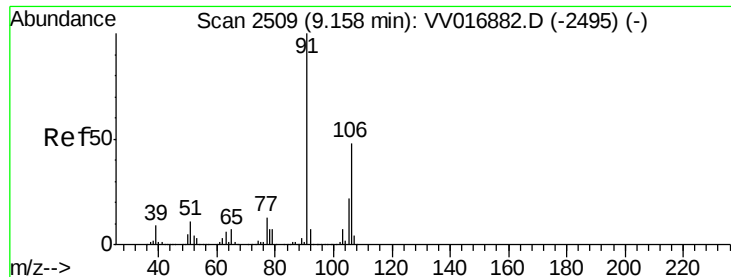

#53

m,p-Xylene

Concen: 4.036 ug/L

RT: 9.16 min Scan# 2511

Delta R.T. 0.01 min

Lab File: VV016890.D

Acq: 12 Jun 2020 19:46

Instrument :

MSVOA_V

ClientSampleId :


F9D87

Tot Ion:106 Resp: 17832

Ion Ratio Lower Upper




106 100

91 214.0 144.6 268.6

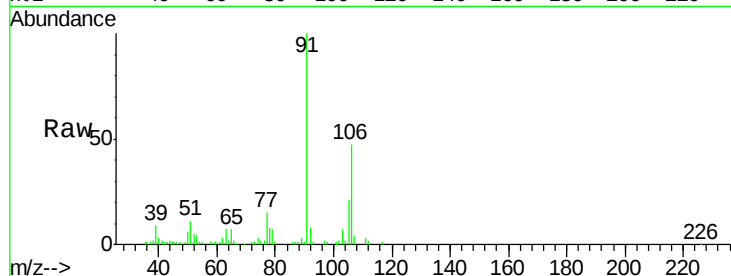

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VV0

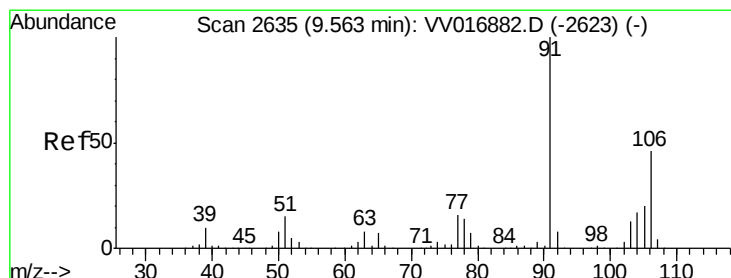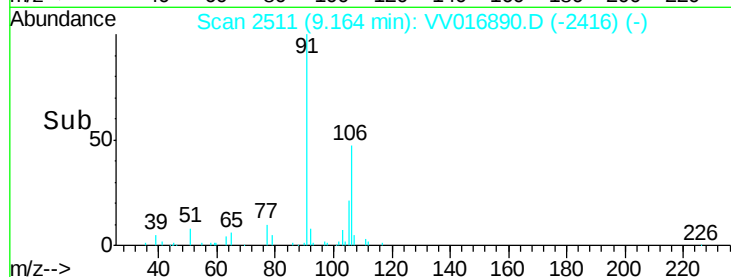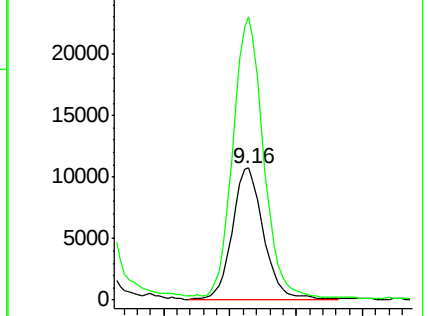

#54

o-xylene

Concen: 8.034 ug/L

RT: 9.56 min Scan# 2635

Delta R.T. -0.00 min

Lab File: VV016890.D


Acq: 12 Jun 2020 19:46

Tgt Ion:106 Resp: 35009

Ion Ratio Lower Upper

106 100

91 207.2 155.9 289.5

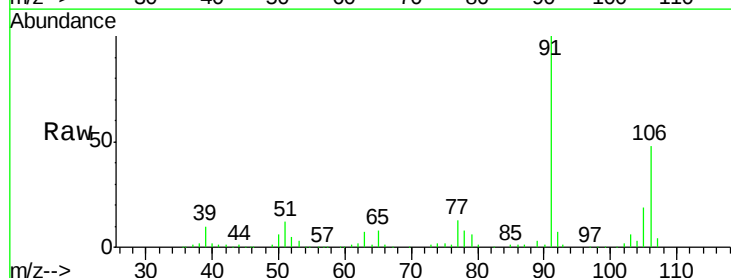

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VV0

