

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016873.D
 Acq On : 12 Jun 2020 12:32
 Operator : SY/MD
 Sample : VV0612WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	193395	186282	12.67%	1.642%
2	1.576	144	151	162	rVB	132058	151781	10.32%	1.338%
3	2.119	311	320	334	rBV	299333	440273	29.94%	3.880%
4	2.563	455	458	462	rBV5	1937	2119	0.14%	0.019%
5	2.743	509	514	516	rBV4	1380	1222	0.08%	0.011%
6	2.968	580	584	585	rBV4	2031	1287	0.09%	0.011%
7	3.039	603	606	611	rVB6	1533	1288	0.09%	0.011%
8	3.087	617	621	623	rBV4	994	927	0.06%	0.008%
9	3.341	699	700	703	rVB3	1701	832	0.06%	0.007%
10	3.367	705	708	711	rBV3	1419	841	0.06%	0.007%
11	3.383	711	713	716	rVB4	1601	805	0.05%	0.007%
12	3.399	716	718	720	rBV3	1042	623	0.04%	0.005%
13	3.499	745	749	751	rBV5	1439	1041	0.07%	0.009%
14	3.585	773	776	778	rBV3	1933	1216	0.08%	0.011%
15	3.662	797	800	804	rBV5	1556	1137	0.08%	0.010%
16	3.695	808	810	815	rVV6	1295	992	0.07%	0.009%
17	3.810	843	846	847	rBV3	1185	622	0.04%	0.005%
18	3.894	860	872	893	rBV	123951	322278	21.91%	2.840%
19	4.254	980	984	988	rBV6	2039	2193	0.15%	0.019%
20	4.373	1007	1021	1044	rVB	244708	585371	39.80%	5.159%
21	4.634	1095	1102	1104	rBV7	2315	2399	0.16%	0.021%
22	4.798	1150	1153	1154	rBV3	1376	597	0.04%	0.005%
23	5.068	1221	1237	1265	rBV2	572221	1470720	100.00%	12.962%
24	5.357	1325	1327	1329	rBV3	1358	749	0.05%	0.007%
25	5.396	1336	1339	1340	rBV3	1519	840	0.06%	0.007%
26	5.424	1343	1348	1349	rBV4	2201	1797	0.12%	0.016%
27	5.637	1401	1414	1437	rBV	462837	928628	63.14%	8.185%
28	6.090	1544	1555	1575	rVB	328665	654770	44.52%	5.771%
29	6.354	1634	1637	1639	rVB4	1473	780	0.05%	0.007%
30	6.531	1689	1692	1696	rVB7	1561	998	0.07%	0.009%
31	6.653	1727	1730	1733	rBV5	1632	1038	0.07%	0.009%
32	6.785	1763	1771	1772	rBV7	1953	1669	0.11%	0.015%
33	6.820	1778	1782	1785	rBV4	1852	1671	0.11%	0.015%
34	6.842	1785	1789	1795	rVB8	2139	2071	0.14%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016873.D
 Acq On : 12 Jun 2020 12:32
 Operator : SY/MD
 Sample : VV0612WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.910	1806	1810	1816	rBV6	2485	2404	0.16%	0.021%
36	6.961	1822	1826	1827	rBV4	1650	1164	0.08%	0.010%
37	7.006	1830	1840	1855	rVV	192557	335844	22.84%	2.960%
38	7.161	1886	1888	1890	rBV3	1971	1318	0.09%	0.012%
39	7.244	1912	1914	1916	rBV3	1250	652	0.04%	0.006%
40	7.334	1930	1942	1957	rBV	684269	1174619	79.87%	10.353%
41	7.640	2026	2037	2056	rBV	140167	237214	16.13%	2.091%
42	7.926	2123	2126	2129	rBV4	1330	1011	0.07%	0.009%
43	7.984	2140	2144	2145	rBV3	1520	997	0.07%	0.009%
44	8.106	2171	2182	2212	rVV2	338762	664925	45.21%	5.860%
45	8.572	2323	2327	2329	rBV5	2111	1589	0.11%	0.014%
46	8.871	2409	2420	2439	rBV	710761	1132998	77.04%	9.986%
47	9.032	2466	2470	2473	rBV5	2163	2118	0.14%	0.019%
48	9.209	2520	2525	2527	rBV5	1822	1521	0.10%	0.013%
49	9.276	2541	2546	2547	rBV4	1852	1465	0.10%	0.013%
50	9.338	2563	2565	2571	rVB6	1467	1156	0.08%	0.010%
51	9.450	2598	2600	2603	rVB4	1481	634	0.04%	0.006%
52	9.778	2698	2702	2706	rBV7	1964	1662	0.11%	0.015%
53	9.823	2714	2716	2722	rVB5	2099	1772	0.12%	0.016%
54	9.916	2741	2745	2747	rBV4	1649	1381	0.09%	0.012%
55	10.000	2768	2771	2773	rBV2	1264	633	0.04%	0.006%
56	10.016	2773	2776	2777	rBV3	1061	598	0.04%	0.005%
57	10.183	2826	2828	2832	rVB5	1751	856	0.06%	0.008%
58	10.238	2832	2845	2859	rBV	422069	657747	44.72%	5.797%
59	10.382	2888	2890	2894	rBV5	1601	1386	0.09%	0.012%
60	10.505	2926	2928	2930	rVV3	1740	1061	0.07%	0.009%
61	10.530	2934	2936	2939	rVV3	1776	992	0.07%	0.009%
62	10.569	2940	2948	2952	rVB10	3917	5592	0.38%	0.049%
63	10.595	2952	2956	2958	rBV3	2057	1594	0.11%	0.014%
64	10.688	2981	2985	2988	rVV6	1850	1215	0.08%	0.011%
65	10.865	3034	3040	3043	rBV8	2325	2567	0.17%	0.023%
66	10.881	3043	3045	3046	rBV2	1436	660	0.04%	0.006%
67	11.067	3100	3103	3106	rBV4	1275	1056	0.07%	0.009%
68	11.128	3120	3122	3126	rVB4	1964	1257	0.09%	0.011%
69	11.270	3155	3166	3186	rBV	740505	1125583	76.53%	9.920%
70	11.450	3218	3222	3224	rBV3	1325	1063	0.07%	0.009%
71	11.646	3271	3283	3306	rBV	756774	1163893	79.14%	10.258%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016873.D
 Acq On : 12 Jun 2020 12:32
 Operator : SY/MD
 Sample : VV0612WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.971	3381	3384	3390	rVB7	1726	1787	0.12%	0.016%
73	12.016	3395	3398	3401	rBV4	1729	1138	0.08%	0.010%
74	12.148	3437	3439	3443	rBV4	1715	1100	0.07%	0.010%
75	12.337	3494	3498	3501	rVB5	1390	982	0.07%	0.009%
76	12.366	3505	3507	3510	rBV3	1485	802	0.05%	0.007%
77	12.469	3537	3539	3545	rVB6	2005	1530	0.10%	0.013%
78	12.562	3564	3568	3572	rBV7	1856	1873	0.13%	0.017%
79	12.582	3572	3574	3577	rVV3	1445	778	0.05%	0.007%
80	12.726	3617	3619	3621	rBV3	1356	802	0.05%	0.007%
81	12.906	3672	3675	3676	rBV3	1565	871	0.06%	0.008%
82	12.958	3687	3691	3696	rVB6	1443	1333	0.09%	0.012%
83	13.051	3717	3720	3722	rBV4	1049	606	0.04%	0.005%
84	13.180	3756	3760	3762	rBV4	1535	1302	0.09%	0.011%
85	13.254	3781	3783	3785	rBV3	1242	669	0.05%	0.006%
86	13.289	3788	3794	3802	rVB10	4436	7136	0.49%	0.063%
87	13.469	3847	3850	3851	rBV3	1229	687	0.05%	0.006%
88	13.524	3863	3867	3868	rBV4	4891	3415	0.23%	0.030%
89	13.614	3893	3895	3897	rBV3	2362	1194	0.08%	0.011%
90	13.710	3923	3925	3928	rBV5	964	605	0.04%	0.005%
91	13.739	3933	3934	3937	rBV3	1205	761	0.05%	0.007%
92	13.762	3938	3941	3942	rBV2	4055	2255	0.15%	0.020%
93	13.890	3980	3981	3984	rBV3	1196	601	0.04%	0.005%
94	13.974	4005	4007	4011	rBV4	1149	1023	0.07%	0.009%
95	14.013	4017	4019	4022	rBV5	993	622	0.04%	0.005%
96	14.202	4071	4078	4079	rBV6	1424	1516	0.10%	0.013%
97	14.431	4145	4149	4150	rBV4	2032	1434	0.10%	0.013%
98	14.546	4182	4185	4186	rBV3	1314	779	0.05%	0.007%
99	14.759	4249	4251	4254	rVB4	1688	939	0.06%	0.008%
100	15.083	4350	4352	4357	rVB5	1981	1536	0.10%	0.014%


Sum of corrected areas: 11346130

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016873.D
Acq On : 12 Jun 2020 12:32
Operator : SY/MD
Sample : VV0612WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

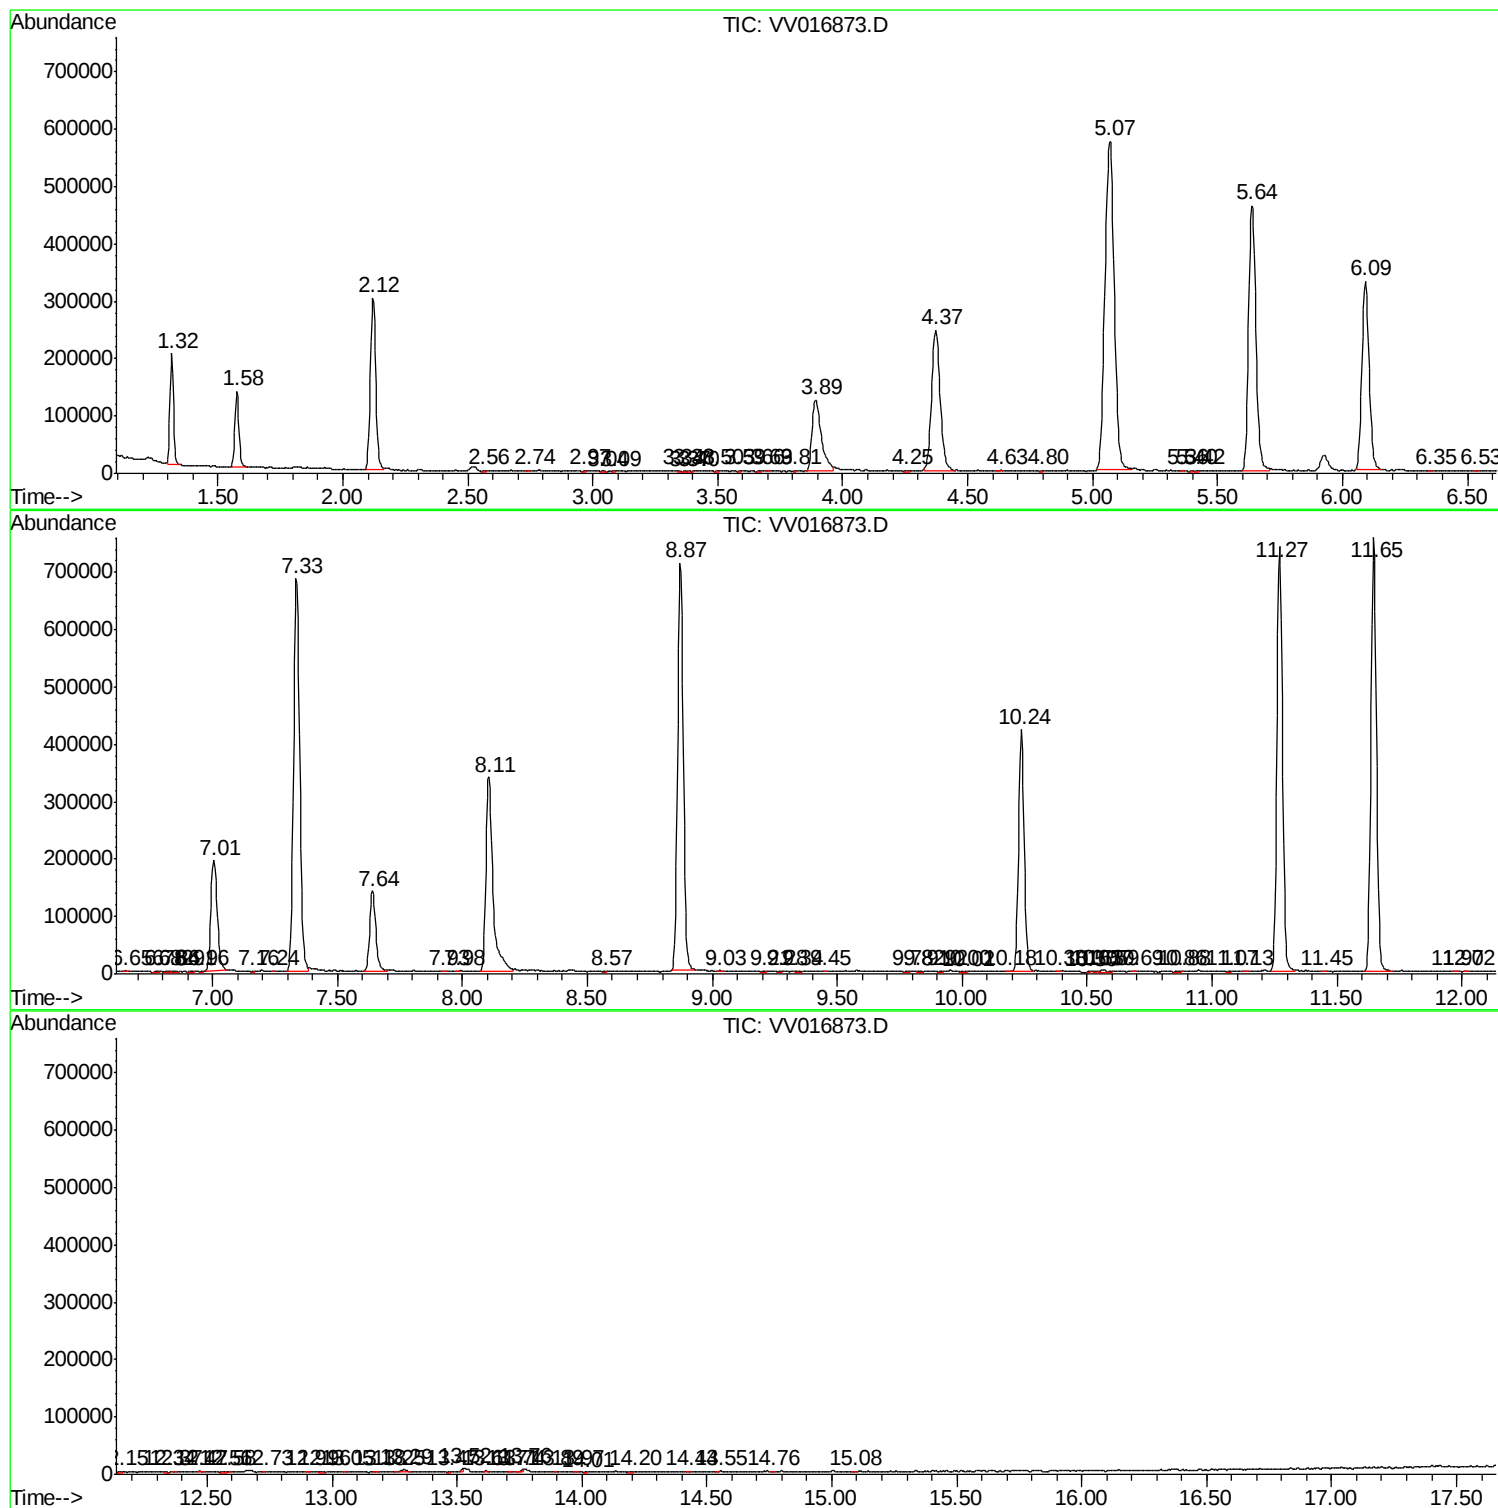

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016873.D
Acq On : 12 Jun 2020 12:32
Operator : SY/MD
Sample : VV0612WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061220\
Data File : VV016873.D
Acq On : 12 Jun 2020 12:32
Operator : SY/MD
Sample : VV0612WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK83

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc