

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016876.D
 Acq On : 12 Jun 2020 14:02
 Operator : SY/MD
 Sample : L2947-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXE4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	79	rVB	179033	173683	12.46%	1.652%
2	1.560	139	146	156	rVB	120263	139802	10.03%	1.330%
3	2.116	310	319	337	rVB	275077	402658	28.88%	3.830%
4	2.293	365	374	388	rBV2	13381	36875	2.64%	0.351%
5	2.476	429	431	434	rBV4	1618	691	0.05%	0.007%
6	3.261	673	675	678	rVB4	1823	848	0.06%	0.008%
7	3.277	678	680	683	rBV5	1759	881	0.06%	0.008%
8	3.363	702	707	710	rBV7	1658	1472	0.11%	0.014%
9	3.463	735	738	741	rBV5	1938	1401	0.10%	0.013%
10	3.495	746	748	752	rBV4	1910	1672	0.12%	0.016%
11	3.598	776	780	782	rBV5	1747	1102	0.08%	0.010%
12	3.634	789	791	795	rBV4	1236	1093	0.08%	0.010%
13	3.701	810	812	816	rVB4	1923	1109	0.08%	0.011%
14	3.736	816	823	824	rBV6	1855	1770	0.13%	0.017%
15	3.756	827	829	832	rVB4	1461	806	0.06%	0.008%
16	3.894	863	872	897	rVV	103080	275994	19.79%	2.625%
17	4.180	958	961	962	rBV3	1448	542	0.04%	0.005%
18	4.373	1008	1021	1047	rVB	224086	554297	39.75%	5.273%
19	4.566	1078	1081	1089	rBV9	2284	2234	0.16%	0.021%
20	4.778	1145	1147	1150	rBV3	1682	1035	0.07%	0.010%
21	4.833	1162	1164	1167	rVB4	2167	861	0.06%	0.008%
22	4.923	1188	1192	1194	rBV3	1331	905	0.06%	0.009%
23	4.939	1194	1197	1201	rVV5	1986	1054	0.08%	0.010%
24	5.071	1216	1238	1263	rBV2	539861	1394437	100.00%	13.265%
25	5.293	1305	1307	1312	rBV5	1525	1193	0.09%	0.011%
26	5.418	1344	1346	1350	rBV5	1504	1004	0.07%	0.010%
27	5.640	1403	1415	1437	rVV	411952	823320	59.04%	7.832%
28	6.093	1544	1556	1585	rVB	309559	627612	45.01%	5.970%
29	6.485	1674	1678	1680	rBV4	2021	1339	0.10%	0.013%
30	6.524	1687	1690	1691	rBV2	1426	871	0.06%	0.008%
31	6.691	1739	1742	1744	rBV3	1826	1108	0.08%	0.011%
32	6.781	1768	1770	1773	rBV4	1388	815	0.06%	0.008%
33	6.823	1781	1783	1787	rVB5	2071	1412	0.10%	0.013%
34	6.875	1797	1799	1804	rBV6	1332	1163	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016876.D
 Acq On : 12 Jun 2020 14:02
 Operator : SY/MD
 Sample : L2947-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXE4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.926	1811	1815	1816	rBV3	2117	1229	0.09%	0.012%
36	7.006	1826	1840	1857	rBV	182145	323773	23.22%	3.080%
37	7.106	1869	1871	1873	rBV3	1829	1107	0.08%	0.011%
38	7.338	1930	1943	1961	rBV	647356	1110156	79.61%	10.560%
39	7.640	2027	2037	2057	rBV	129786	222453	15.95%	2.116%
40	7.775	2077	2079	2081	rBV3	1647	877	0.06%	0.008%
41	7.839	2098	2099	2101	rVB2	1848	568	0.04%	0.005%
42	7.855	2101	2104	2106	rBV4	1920	1199	0.09%	0.011%
43	8.045	2160	2163	2168	rVB7	2352	1639	0.12%	0.016%
44	8.071	2168	2171	2173	rBV4	1789	1306	0.09%	0.012%
45	8.109	2173	2183	2220	rVV2	290979	621786	44.59%	5.915%
46	8.643	2348	2349	2353	rBV4	1335	848	0.06%	0.008%
47	8.704	2364	2368	2370	rBV4	1452	1282	0.09%	0.012%
48	8.759	2382	2385	2387	rVB3	1639	967	0.07%	0.009%
49	8.874	2410	2421	2440	rVB	632647	1009360	72.38%	9.601%
50	9.083	2483	2486	2488	rBV4	1866	1187	0.09%	0.011%
51	9.096	2488	2490	2494	rVV3	2645	1652	0.12%	0.016%
52	9.386	2577	2580	2582	rBV3	2491	1370	0.10%	0.013%
53	9.418	2586	2590	2594	rBV5	1598	1651	0.12%	0.016%
54	9.508	2616	2618	2620	rBV3	1378	845	0.06%	0.008%
55	9.572	2629	2638	2641	rBV3	4764	6157	0.44%	0.059%
56	9.714	2680	2682	2685	rVB4	1665	706	0.05%	0.007%
57	9.733	2686	2688	2691	rVB4	1013	528	0.04%	0.005%
58	9.987	2764	2767	2769	rBV4	1346	758	0.05%	0.007%
59	10.016	2773	2776	2779	rBV5	1649	1315	0.09%	0.013%
60	10.061	2788	2790	2794	rVB3	1443	996	0.07%	0.009%
61	10.238	2830	2845	2860	rBV	368330	588937	42.23%	5.602%
62	10.344	2875	2878	2879	rBV3	1393	817	0.06%	0.008%
63	10.395	2889	2894	2896	rBV5	2558	2426	0.17%	0.023%
64	10.444	2907	2909	2910	rBV2	1438	632	0.05%	0.006%
65	10.485	2918	2922	2926	rBV6	1611	1576	0.11%	0.015%
66	10.601	2955	2958	2964	rVB7	2297	2161	0.15%	0.021%
67	10.630	2965	2967	2971	rVV4	992	612	0.04%	0.006%
68	10.736	2998	3000	3001	rBV2	1170	591	0.04%	0.006%
69	10.788	3012	3016	3020	rBV6	2104	2320	0.17%	0.022%
70	10.807	3020	3022	3029	rVB7	1920	1730	0.12%	0.016%
71	11.032	3091	3092	3097	rBV4	929	700	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016876.D
 Acq On : 12 Jun 2020 14:02
 Operator : SY/MD
 Sample : L2947-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXE4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3184	rBV	662747	1009220	72.37%	9.600%
73	11.534	3246	3248	3252	rVB4	1083	700	0.05%	0.007%
74	11.646	3272	3283	3303	rBV	704080	1098350	78.77%	10.448%
75	11.884	3355	3357	3360	rVB4	2312	1347	0.10%	0.013%
76	11.903	3360	3363	3366	rBV5	2009	1531	0.11%	0.015%
77	11.980	3385	3387	3392	rBV4	1318	932	0.07%	0.009%
78	12.009	3394	3396	3399	rBV2	1542	666	0.05%	0.006%
79	12.109	3424	3427	3428	rBV3	1546	693	0.05%	0.007%
80	12.135	3433	3435	3439	rBV4	1359	895	0.06%	0.009%
81	12.254	3469	3472	3474	rBV4	1374	1067	0.08%	0.010%
82	12.366	3503	3507	3510	rVB4	1618	1267	0.09%	0.012%
83	12.382	3510	3512	3514	rBV3	1361	746	0.05%	0.007%
84	12.614	3578	3584	3589	rBV8	2224	3096	0.22%	0.029%
85	12.762	3628	3630	3634	rBV4	1483	996	0.07%	0.009%
86	12.849	3654	3657	3659	rVB3	1816	1077	0.08%	0.010%
87	12.868	3659	3663	3665	rBV5	1667	1222	0.09%	0.012%
88	12.977	3695	3697	3701	rVB4	1440	801	0.06%	0.008%
89	13.109	3733	3738	3741	rBV6	1408	1393	0.10%	0.013%
90	13.164	3751	3755	3758	rBV5	1472	983	0.07%	0.009%
91	13.225	3771	3774	3775	rBV3	1627	797	0.06%	0.008%
92	13.341	3808	3810	3812	rBV3	1382	891	0.06%	0.008%
93	13.630	3897	3900	3902	rBV3	1550	770	0.06%	0.007%
94	13.701	3921	3922	3926	rVB4	1486	856	0.06%	0.008%
95	13.726	3926	3930	3933	rBV6	2550	1846	0.13%	0.018%
96	13.916	3987	3989	3993	rBV4	1121	700	0.05%	0.007%
97	13.939	3993	3996	3998	rBV4	1279	1034	0.07%	0.010%
98	13.996	4012	4014	4017	rBV4	1286	979	0.07%	0.009%
99	14.270	4097	4099	4101	rBV3	1333	701	0.05%	0.007%
100	14.540	4180	4183	4187	rBV5	2127	1697	0.12%	0.016%


Sum of corrected areas: 10512529

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016876.D
Acq On : 12 Jun 2020 14:02
Operator : SY/MD
Sample : L2947-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXE4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

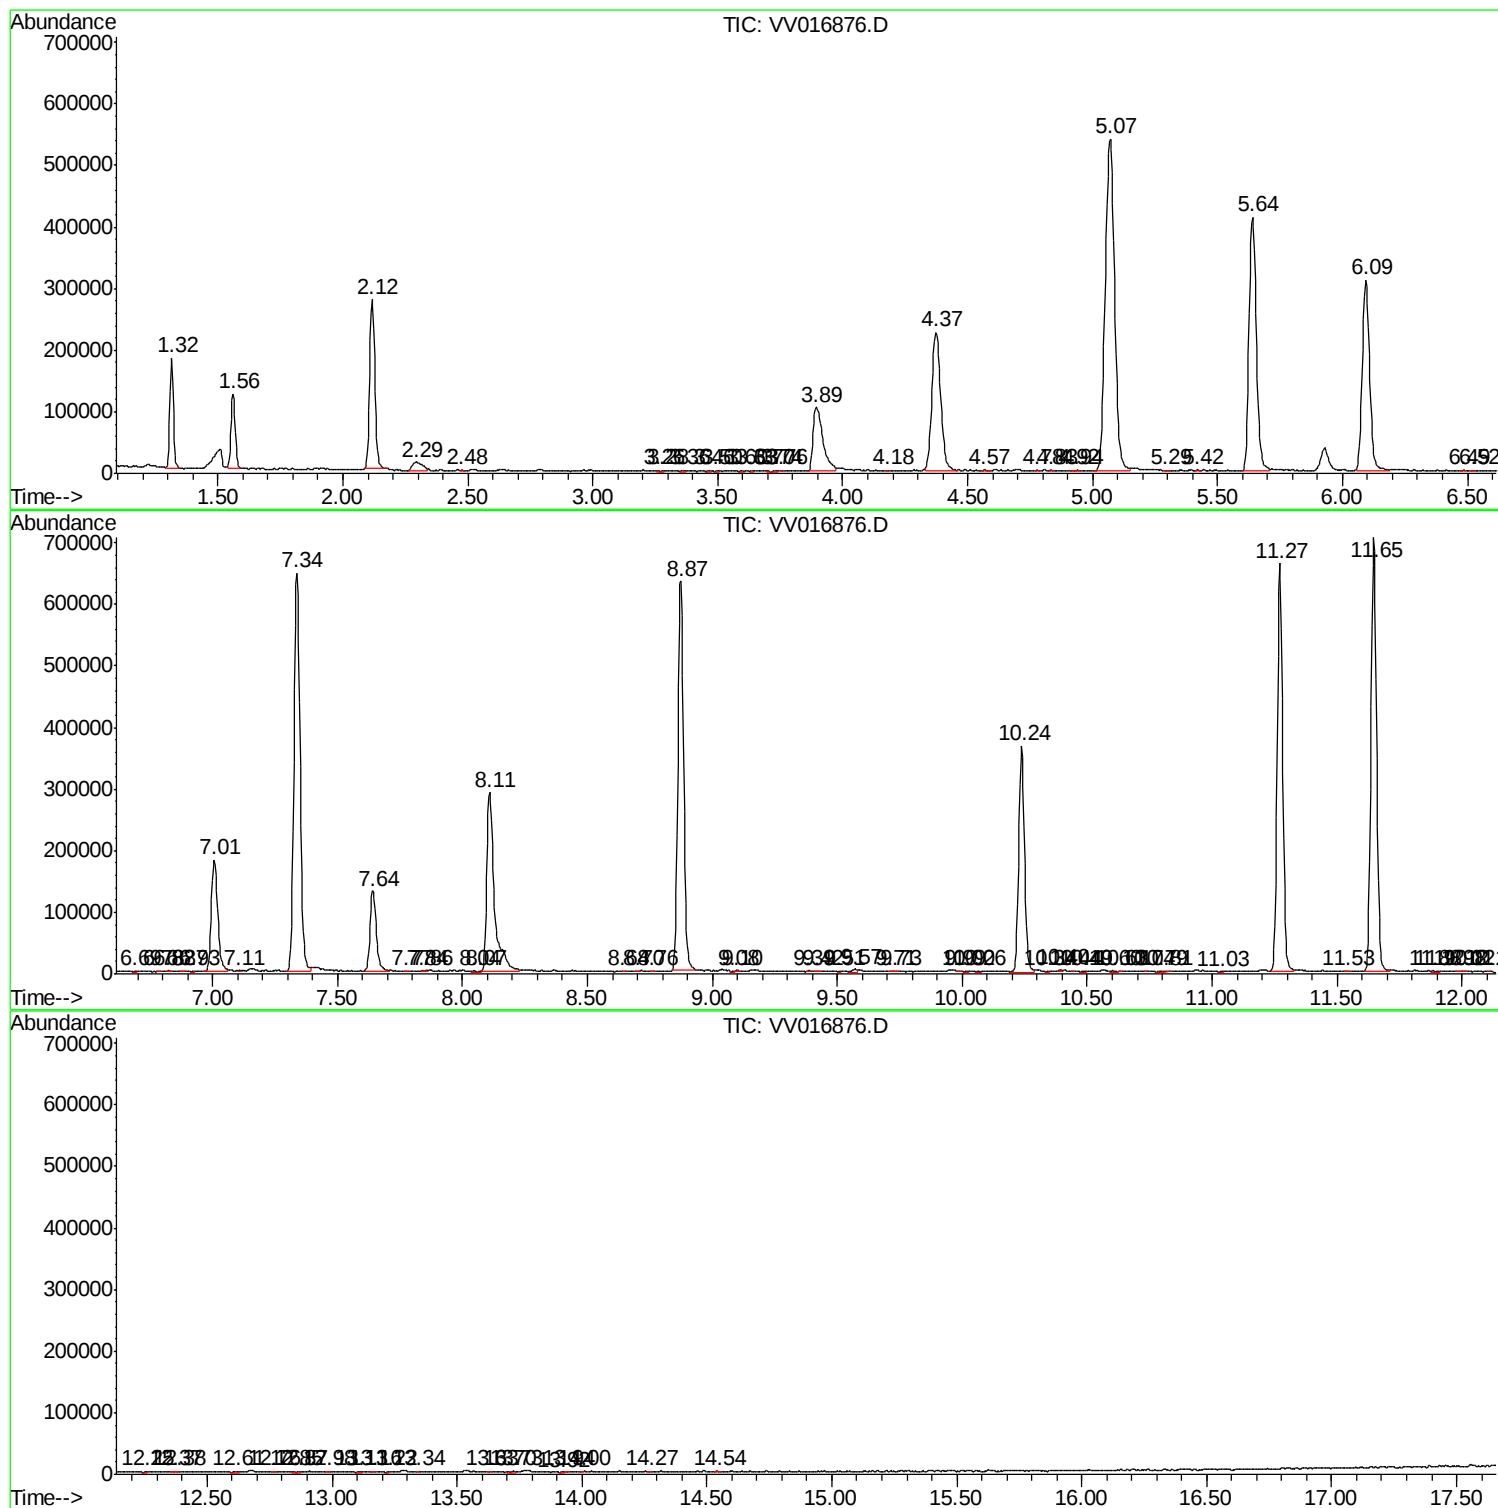

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016876.D
Acq On : 12 Jun 2020 14:02
Operator : SY/MD
Sample : L2947-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXE4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016876.D
Acq On : 12 Jun 2020 14:02
Operator : SY/MD
Sample : L2947-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXE4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc