

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016877.D
 Acq On : 12 Jun 2020 14:26
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	80	rVB	112378	113385	12.90%	1.997%
2	1.560	140	146	155	rVB	78184	90492	10.30%	1.594%
3	2.116	310	319	333	rVB	176485	257461	29.29%	4.534%
4	2.563	454	458	460	rBV5	2161	1542	0.18%	0.027%
5	2.859	548	550	554	rVB3	1253	684	0.08%	0.012%
6	3.023	597	601	604	rBV5	1943	1686	0.19%	0.030%
7	3.113	625	629	632	rBV3	1599	1649	0.19%	0.029%
8	3.264	671	676	679	rBV7	1932	1603	0.18%	0.028%
9	3.319	692	693	694	rBV	786	291	0.03%	0.005%
10	3.434	725	729	731	rBV4	1868	1493	0.17%	0.026%
11	3.589	775	777	781	rBV5	1480	841	0.10%	0.015%
12	3.627	787	789	794	rBB6	1372	986	0.11%	0.017%
13	3.701	809	812	814	rBV3	1475	1078	0.12%	0.019%
14	3.746	825	826	832	rVB6	1213	714	0.08%	0.013%
15	3.772	832	834	837	rBV3	1316	673	0.08%	0.012%
16	3.830	849	852	860	rVB10	1585	1365	0.16%	0.024%
17	3.865	860	863	864	rBV3	1984	1028	0.12%	0.018%
18	3.897	864	873	900	rVV	70498	200746	22.84%	3.535%
19	4.155	949	953	958	rBV7	2336	2395	0.27%	0.042%
20	4.222	972	974	981	rBV7	1599	1801	0.20%	0.032%
21	4.373	1008	1021	1043	rVB2	144897	351352	39.98%	6.187%
22	4.663	1110	1111	1112	rBV	1292	409	0.05%	0.007%
23	4.775	1145	1146	1149	rBV3	1301	612	0.07%	0.011%
24	5.068	1222	1237	1265	rBV2	344468	878898	100.00%	15.478%
25	5.454	1355	1357	1359	rBV3	1177	580	0.07%	0.010%
26	5.573	1390	1394	1396	rBV4	1287	1044	0.12%	0.018%
27	5.640	1405	1415	1434	rVB	111768	217941	24.80%	3.838%
28	5.846	1477	1479	1484	rVB4	1617	1059	0.12%	0.019%
29	5.872	1484	1487	1489	rBV3	2324	1459	0.17%	0.026%
30	5.929	1497	1505	1518	rVB2	22248	44024	5.01%	0.775%
31	6.093	1544	1556	1576	rVB	195851	392142	44.62%	6.906%
32	6.367	1639	1641	1645	rBV5	2055	1665	0.19%	0.029%
33	6.457	1667	1669	1671	rBV3	1678	622	0.07%	0.011%
34	6.544	1694	1696	1700	rBV4	1828	1408	0.16%	0.025%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016877.D
 Acq On : 12 Jun 2020 14:26
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.659	1730	1732	1737	rVB6	2006	1684	0.19%	0.030%
36	6.695	1737	1743	1744	rBV5	1521	1549	0.18%	0.027%
37	6.836	1785	1787	1790	rBV3	1206	682	0.08%	0.012%
38	6.904	1805	1808	1810	rBV4	736	490	0.06%	0.009%
39	6.917	1810	1812	1813	rBV2	1520	660	0.08%	0.012%
40	7.007	1830	1840	1859	rBV	111655	199012	22.64%	3.505%
41	7.113	1871	1873	1875	rBV3	1393	872	0.10%	0.015%
42	7.338	1931	1943	1963	rBV	401042	700548	79.71%	12.337%
43	7.643	2029	2038	2051	rBV	80527	134178	15.27%	2.363%
44	7.875	2108	2110	2112	rBV3	1063	628	0.07%	0.011%
45	8.000	2146	2149	2152	rBV4	2089	1490	0.17%	0.026%
46	8.109	2174	2183	2214	rBV2	182772	378441	43.06%	6.664%
47	8.444	2285	2287	2291	rBV4	1148	663	0.08%	0.012%
48	8.486	2297	2300	2302	rVB4	1670	990	0.11%	0.017%
49	8.714	2369	2371	2374	rVB4	935	457	0.05%	0.008%
50	8.875	2411	2421	2435	rBV	180051	285334	32.46%	5.025%
51	8.968	2448	2450	2457	rBV8	1575	1220	0.14%	0.021%
52	9.032	2468	2470	2473	rBV3	1289	898	0.10%	0.016%
53	9.283	2545	2548	2552	rBV5	1075	1109	0.13%	0.020%
54	9.418	2587	2590	2592	rBV4	1213	798	0.09%	0.014%
55	9.560	2632	2634	2638	rBV4	1789	1602	0.18%	0.028%
56	9.672	2667	2669	2671	rBV3	1387	636	0.07%	0.011%
57	9.781	2701	2703	2705	rBV3	1389	814	0.09%	0.014%
58	9.855	2724	2726	2727	rBV2	1313	367	0.04%	0.006%
59	10.039	2781	2783	2785	rBV3	1496	770	0.09%	0.014%
60	10.080	2793	2796	2799	rBV4	1643	1129	0.13%	0.020%
61	10.109	2803	2805	2809	rVB4	1672	1024	0.12%	0.018%
62	10.138	2811	2814	2819	rBV6	1308	1465	0.17%	0.026%
63	10.199	2831	2833	2834	rBV2	1650	776	0.09%	0.014%
64	10.238	2834	2845	2858	rVV	244753	379214	43.15%	6.678%
65	10.312	2866	2868	2871	rVB5	1475	528	0.06%	0.009%
66	10.334	2873	2875	2877	rVB3	1505	571	0.06%	0.010%
67	10.399	2891	2895	2896	rBV4	1561	1143	0.13%	0.020%
68	10.653	2972	2974	2978	rBV3	2096	1478	0.17%	0.026%
69	10.743	2999	3002	3005	rBV5	1406	1012	0.12%	0.018%
70	10.810	3021	3023	3025	rBV2	1792	775	0.09%	0.014%
71	10.852	3034	3036	3037	rBV2	1344	478	0.05%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016877.D
 Acq On : 12 Jun 2020 14:26
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.961	3066	3070	3073	rBV6	1721	1408	0.16%	0.025%
73	11.106	3112	3115	3118	rBV5	1697	1152	0.13%	0.020%
74	11.174	3132	3136	3138	rBV4	2142	1439	0.16%	0.025%
75	11.225	3150	3152	3154	rBV3	1548	665	0.08%	0.012%
76	11.273	3155	3167	3185	rVV	171977	278220	31.66%	4.900%
77	11.469	3223	3228	3229	rBV6	1771	1208	0.14%	0.021%
78	11.646	3271	3283	3298	rBV	441483	692317	78.77%	12.192%
79	11.781	3323	3325	3328	rBV3	2144	1277	0.15%	0.022%
80	11.952	3375	3378	3380	rBV3	1232	747	0.08%	0.013%
81	12.058	3408	3411	3413	rBV4	1764	1085	0.12%	0.019%
82	12.080	3417	3418	3425	rVB5	1552	1076	0.12%	0.019%
83	12.167	3443	3445	3447	rVB3	1179	358	0.04%	0.006%
84	12.399	3515	3517	3524	rVB6	1863	1581	0.18%	0.028%
85	12.428	3524	3526	3529	rBV4	1204	642	0.07%	0.011%
86	12.656	3595	3597	3598	rBV3	1401	622	0.07%	0.011%
87	12.736	3619	3622	3623	rBV3	1423	933	0.11%	0.016%
88	12.820	3644	3648	3651	rBV6	1760	1822	0.21%	0.032%
89	13.016	3708	3709	3711	rBV2	1210	405	0.05%	0.007%
90	13.186	3759	3762	3763	rBV3	1244	622	0.07%	0.011%
91	13.321	3802	3804	3806	rBV3	1356	456	0.05%	0.008%
92	13.675	3911	3914	3918	rBV3	2117	1558	0.18%	0.027%
93	13.752	3936	3938	3942	rBV4	1248	880	0.10%	0.015%
94	13.839	3963	3965	3968	rBV3	1593	885	0.10%	0.016%
95	13.910	3984	3987	3989	rBV3	1363	1036	0.12%	0.018%
96	14.103	4045	4047	4048	rBV2	1973	839	0.10%	0.015%
97	14.270	4096	4099	4101	rBV3	1519	1068	0.12%	0.019%
98	14.456	4155	4157	4163	rBV7	1789	1548	0.18%	0.027%
99	15.238	4398	4400	4401	rBV2	1914	878	0.10%	0.015%
100	16.038	4647	4649	4652	rBV5	1883	1182	0.13%	0.021%


Sum of corrected areas: 5678522

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016877.D
Acq On : 12 Jun 2020 14:26
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

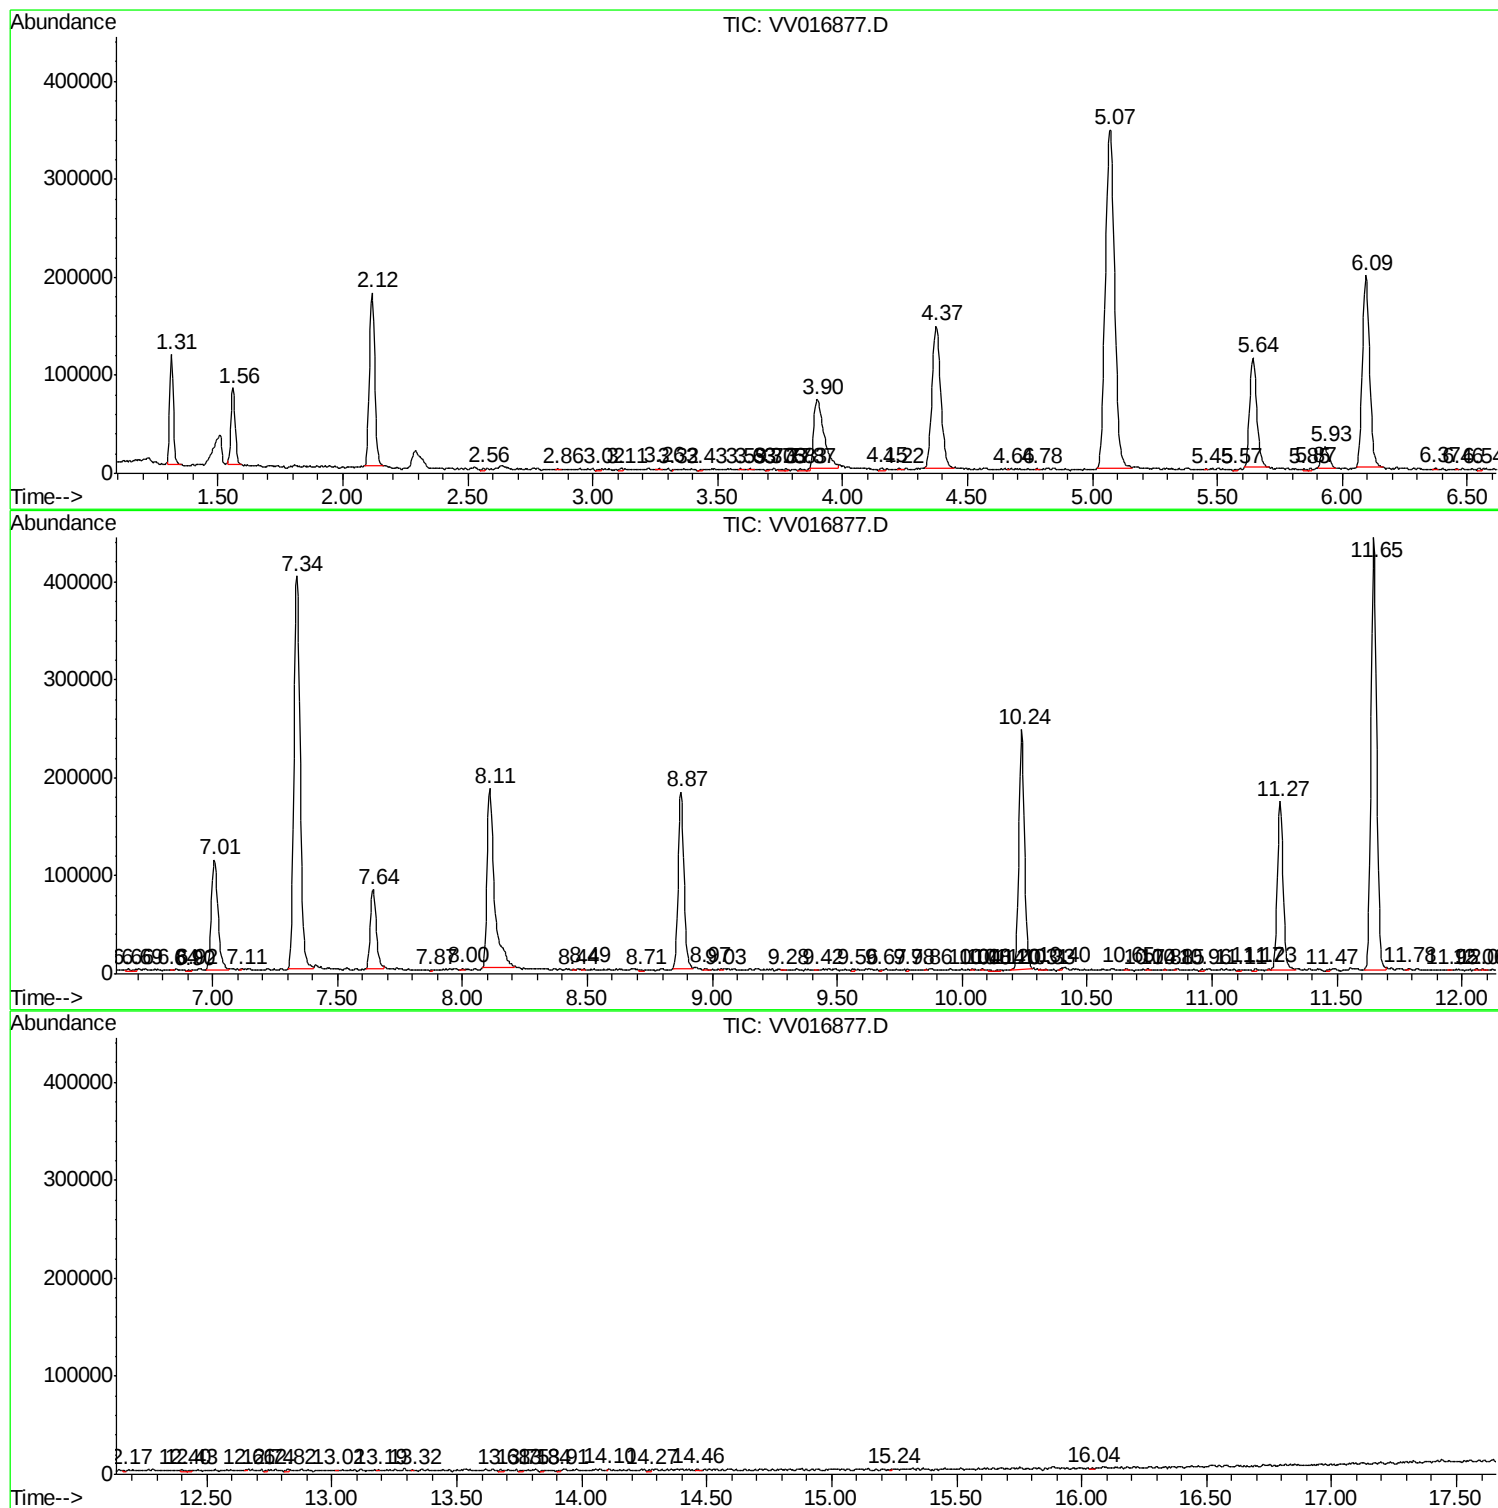

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016877.D
Acq On : 12 Jun 2020 14:26
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016877.D
Acq On : 12 Jun 2020 14:26
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc