

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016891.D
 Acq On : 12 Jun 2020 20:10
 Operator : SY/MD
 Sample : L2914-03 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	166292	174841	12.21%	1.619%
2	1.563	143	147	156	rVB	125637	129371	9.03%	1.198%
3	2.116	310	319	339	rVB	265956	399607	27.90%	3.700%
4	2.486	425	434	436	rBV8	4608	5441	0.38%	0.050%
5	2.586	458	465	468	rBV8	4132	5768	0.40%	0.053%
6	2.862	549	551	555	rBV5	1465	1398	0.10%	0.013%
7	2.891	558	560	564	rBV5	1267	810	0.06%	0.008%
8	3.087	619	621	624	rVB3	1369	623	0.04%	0.006%
9	3.123	630	632	634	rBV2	1139	652	0.05%	0.006%
10	3.142	636	638	641	rVB3	1711	799	0.06%	0.007%
11	3.158	641	643	646	rBV4	1201	930	0.06%	0.009%
12	3.267	675	677	680	rBV3	1021	640	0.04%	0.006%
13	3.441	728	731	732	rBV3	1978	1084	0.08%	0.010%
14	3.563	765	769	771	rBV4	1239	963	0.07%	0.009%
15	3.637	790	792	794	rBV3	1329	655	0.05%	0.006%
16	3.698	808	811	814	rBV5	1196	753	0.05%	0.007%
17	3.769	830	833	836	rBV4	1839	1569	0.11%	0.015%
18	3.814	845	847	853	rVB6	1974	1406	0.10%	0.013%
19	3.897	863	873	899	rBV	108341	297984	20.80%	2.759%
20	4.200	964	967	971	rVB6	2378	1658	0.12%	0.015%
21	4.312	998	1002	1004	rBV4	2155	1636	0.11%	0.015%
22	4.373	1007	1021	1043	rVV	227276	553063	38.61%	5.121%
23	4.483	1052	1055	1058	rBV5	1634	1018	0.07%	0.009%
24	4.508	1061	1063	1065	rBV3	1825	849	0.06%	0.008%
25	4.595	1086	1090	1092	rVB4	1250	893	0.06%	0.008%
26	4.621	1096	1098	1101	rBV3	1056	720	0.05%	0.007%
27	4.672	1112	1114	1115	rBV2	1531	577	0.04%	0.005%
28	4.814	1155	1158	1161	rBV5	1376	677	0.05%	0.006%
29	4.830	1161	1163	1166	rVB5	1716	879	0.06%	0.008%
30	4.913	1188	1189	1196	rVB7	1173	888	0.06%	0.008%
31	4.939	1196	1197	1200	rVB3	1588	608	0.04%	0.006%
32	4.968	1200	1206	1208	rBV6	1568	1270	0.09%	0.012%
33	5.071	1219	1238	1248	rBV2	550189	1432386	100.00%	13.263%
34	5.524	1377	1379	1382	rBV3	2017	1484	0.10%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016891.D
 Acq On : 12 Jun 2020 20:10
 Operator : SY/MD
 Sample : L2914-03 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.640	1402	1415	1435	rBV	453703	898789	62.75%	8.322%
36	5.926	1496	1504	1523	rVB3	24805	51022	3.56%	0.472%
37	6.093	1544	1556	1579	rVB2	311944	625053	43.64%	5.788%
38	6.441	1657	1664	1667	rVB7	2655	2836	0.20%	0.026%
39	6.470	1671	1673	1674	rBV2	1318	667	0.05%	0.006%
40	6.515	1683	1687	1690	rVB4	1358	1115	0.08%	0.010%
41	6.544	1693	1696	1699	rVB4	1452	1010	0.07%	0.009%
42	6.875	1793	1799	1800	rBV5	1085	1058	0.07%	0.010%
43	6.926	1812	1815	1817	rBV3	1142	715	0.05%	0.007%
44	7.007	1828	1840	1856	rBV	186298	332140	23.19%	3.075%
45	7.245	1909	1914	1916	rBV6	1666	1578	0.11%	0.015%
46	7.283	1924	1926	1930	rBV4	1561	1361	0.10%	0.013%
47	7.338	1930	1943	1958	rBV	644057	1103561	77.04%	10.219%
48	7.640	2028	2037	2056	rVB	132916	220461	15.39%	2.041%
49	7.810	2088	2090	2093	rBV2	1182	902	0.06%	0.008%
50	7.917	2120	2123	2128	rVB6	1690	1045	0.07%	0.010%
51	8.036	2158	2160	2164	rBV4	1565	1256	0.09%	0.012%
52	8.109	2173	2183	2215	rBV	314371	627916	43.84%	5.814%
53	8.614	2337	2340	2342	rBV2	1709	1068	0.07%	0.010%
54	8.871	2409	2420	2445	rBV	676501	1090501	76.13%	10.098%
55	9.035	2463	2471	2487	rVB	38464	62103	4.34%	0.575%
56	9.219	2526	2528	2534	rVB6	1602	1516	0.11%	0.014%
57	9.457	2598	2602	2603	rBV3	2078	1421	0.10%	0.013%
58	9.566	2629	2636	2647	rVB4	9913	16347	1.14%	0.151%
59	9.653	2660	2663	2666	rBV5	1018	813	0.06%	0.008%
60	9.730	2685	2687	2688	rBV2	1779	915	0.06%	0.008%
61	9.926	2744	2748	2750	rBV5	1725	1301	0.09%	0.012%
62	10.093	2796	2800	2801	rBV3	2381	1286	0.09%	0.012%
63	10.167	2819	2823	2825	rBV4	1439	1034	0.07%	0.010%
64	10.238	2835	2845	2860	rVB	400389	610511	42.62%	5.653%
65	10.521	2932	2933	2938	rBV3	1563	841	0.06%	0.008%
66	10.543	2938	2940	2943	rBV4	1612	902	0.06%	0.008%
67	10.675	2979	2981	2983	rBV4	1510	827	0.06%	0.008%
68	10.756	3003	3006	3007	rBV3	1834	895	0.06%	0.008%
69	10.849	3029	3035	3036	rBV5	1927	1726	0.12%	0.016%
70	11.045	3094	3096	3099	rVB3	1557	927	0.06%	0.009%
71	11.064	3099	3102	3105	rBV6	1411	1086	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016891.D
 Acq On : 12 Jun 2020 20:10
 Operator : SY/MD
 Sample : L2914-03 25X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3182	rBV	666939	1018152	71.08%	9.428%
73	11.476	3228	3230	3232	rBV4	1181	630	0.04%	0.006%
74	11.646	3272	3283	3300	rBV	673016	1058681	73.91%	9.803%
75	11.740	3310	3312	3314	rBV3	1665	918	0.06%	0.009%
76	11.884	3354	3357	3360	rBV3	1856	1282	0.09%	0.012%
77	12.013	3394	3397	3399	rBV3	1431	812	0.06%	0.008%
78	12.103	3421	3425	3428	rBV4	2005	2111	0.15%	0.020%
79	12.183	3446	3450	3453	rVB5	1343	1064	0.07%	0.010%
80	12.370	3503	3508	3510	rBV5	1078	1052	0.07%	0.010%
81	12.469	3535	3539	3540	rBV2	1681	980	0.07%	0.009%
82	12.556	3563	3566	3572	rBV8	1841	1676	0.12%	0.016%
83	12.588	3572	3576	3578	rBV3	933	671	0.05%	0.006%
84	12.791	3635	3639	3641	rBV5	1161	883	0.06%	0.008%
85	12.907	3672	3675	3677	rBV4	2725	1710	0.12%	0.016%
86	12.984	3694	3699	3703	rBV5	1193	1254	0.09%	0.012%
87	13.003	3703	3705	3707	rVV3	1322	747	0.05%	0.007%
88	13.019	3707	3710	3716	rVB8	2167	1849	0.13%	0.017%
89	13.045	3716	3718	3723	rBV6	1025	629	0.04%	0.006%
90	13.627	3895	3899	3901	rBV4	921	812	0.06%	0.008%
91	13.781	3944	3947	3949	rBV3	2110	1024	0.07%	0.009%
92	13.923	3987	3991	3994	rBV5	2004	1511	0.11%	0.014%
93	14.003	4012	4016	4020	rVB6	1859	1506	0.11%	0.014%
94	14.029	4020	4024	4027	rBV4	1869	1505	0.11%	0.014%
95	14.125	4050	4054	4055	rBV3	1159	682	0.05%	0.006%
96	14.199	4074	4077	4080	rBV4	1242	964	0.07%	0.009%
97	14.283	4101	4103	4106	rBV4	1266	841	0.06%	0.008%
98	14.376	4130	4132	4136	rVB4	1711	1129	0.08%	0.010%
99	14.402	4136	4140	4141	rBV4	1613	1042	0.07%	0.010%
100	15.170	4378	4379	4383	rBV4	1514	1051	0.07%	0.010%


Sum of corrected areas: 10799573

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016891.D
Acq On : 12 Jun 2020 20:10
Operator : SY/MD
Sample : L2914-03 25X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

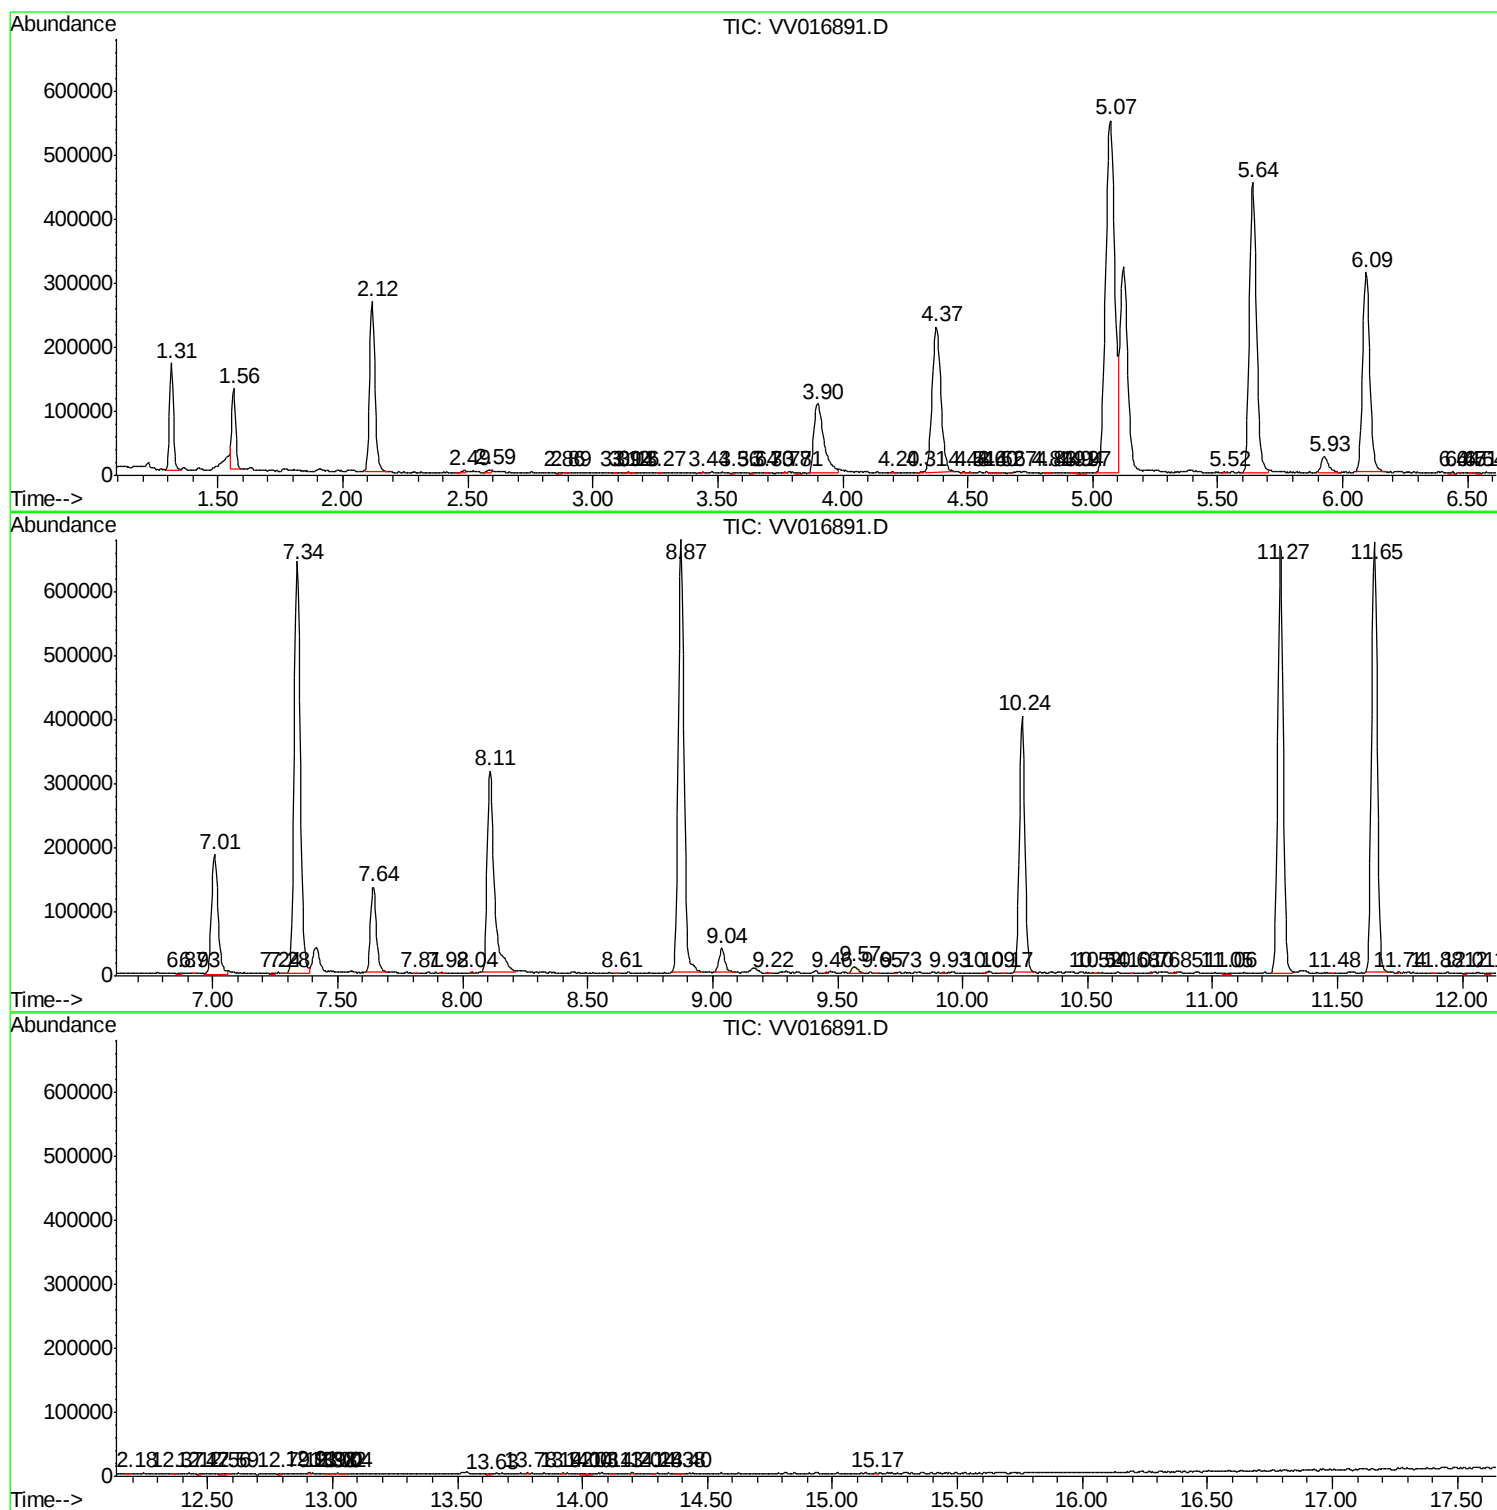

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016891.D
Acq On : 12 Jun 2020 20:10
Operator : SY/MD
Sample : L2914-03 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016891.D
Acq On : 12 Jun 2020 20:10
Operator : SY/MD
Sample : L2914-03 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D96

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc