

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016901.D
 Acq On : 13 Jun 2020 00:55
 Operator : SY/MD
 Sample : VV0612WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	83	rVB	165132	167998	12.67%	1.646%
2	1.553	138	144	158	rVB	116689	140514	10.60%	1.377%
3	2.113	309	318	335	rVB	263898	394691	29.76%	3.867%
4	2.203	342	346	348	rBV5	1635	1467	0.11%	0.014%
5	2.582	461	464	467	rBV4	1122	733	0.06%	0.007%
6	2.618	472	475	477	rBV3	1613	1105	0.08%	0.011%
7	2.753	513	517	519	rBV4	1575	1156	0.09%	0.011%
8	2.929	567	572	573	rBV5	2011	1233	0.09%	0.012%
9	2.994	589	592	594	rBV4	1388	890	0.07%	0.009%
10	3.142	635	638	640	rBV4	1641	1010	0.08%	0.010%
11	3.171	643	647	649	rVB4	1823	1341	0.10%	0.013%
12	3.199	651	656	660	rBV8	2110	2197	0.17%	0.022%
13	3.222	660	663	666	rBV4	1775	950	0.07%	0.009%
14	3.553	764	766	768	rBV3	1483	917	0.07%	0.009%
15	3.585	773	776	779	rBV4	1465	1172	0.09%	0.011%
16	3.675	801	804	807	rVB3	1585	975	0.07%	0.010%
17	3.894	860	872	897	rBV2	104857	281627	21.24%	2.759%
18	4.158	951	954	958	rBV4	1062	844	0.06%	0.008%
19	4.373	1005	1021	1043	rBV	217036	530076	39.97%	5.193%
20	4.621	1091	1098	1100	rBV8	1578	1767	0.13%	0.017%
21	4.817	1156	1159	1161	rBV4	1435	908	0.07%	0.009%
22	4.910	1185	1188	1190	rBV4	1296	801	0.06%	0.008%
23	4.942	1196	1198	1201	rBV4	1781	968	0.07%	0.009%
24	4.974	1206	1208	1212	rVB4	1514	790	0.06%	0.008%
25	4.997	1212	1215	1217	rBV3	1323	818	0.06%	0.008%
26	5.068	1220	1237	1262	rBV2	513267	1326219	100.00%	12.992%
27	5.270	1298	1300	1305	rBV6	1530	1244	0.09%	0.012%
28	5.331	1314	1319	1321	rBV5	2149	2038	0.15%	0.020%
29	5.383	1333	1335	1337	rBV3	1371	747	0.06%	0.007%
30	5.486	1364	1367	1369	rBV4	2225	1419	0.11%	0.014%
31	5.637	1399	1414	1438	rBV	404687	812475	61.26%	7.959%
32	5.926	1493	1504	1516	rBV2	24850	51288	3.87%	0.502%
33	6.093	1543	1556	1580	rBV	290121	593012	44.71%	5.809%
34	6.408	1651	1654	1657	rBV4	1998	1146	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016901.D
 Acq On : 13 Jun 2020 00:55
 Operator : SY/MD
 Sample : VV0612WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.585	1704	1709	1714	rBV8	2071	2068	0.16%	0.020%
36	6.662	1731	1733	1736	rVB2	1628	833	0.06%	0.008%
37	6.682	1736	1739	1742	rBV4	1375	1019	0.08%	0.010%
38	6.736	1751	1756	1759	rBV5	1368	1371	0.10%	0.013%
39	6.875	1797	1799	1805	rVB7	1472	971	0.07%	0.010%
40	7.006	1828	1840	1859	rBV	166584	301023	22.70%	2.949%
41	7.170	1888	1891	1893	rBV3	1264	825	0.06%	0.008%
42	7.338	1928	1943	1962	rBV	610178	1045633	78.84%	10.243%
43	7.559	2008	2012	2015	rBV5	1994	1499	0.11%	0.015%
44	7.640	2026	2037	2056	rBV	122273	210449	15.87%	2.062%
45	7.942	2128	2131	2133	rBV3	1806	1164	0.09%	0.011%
46	8.106	2172	2182	2215	rBV2	307502	616994	46.52%	6.044%
47	8.383	2265	2268	2274	rVB7	1566	1487	0.11%	0.015%
48	8.733	2375	2377	2379	rBV3	1267	753	0.06%	0.007%
49	8.778	2387	2391	2395	rBV6	1581	906	0.07%	0.009%
50	8.871	2408	2420	2437	rBV	606640	982451	74.08%	9.625%
51	9.125	2495	2499	2503	rBV7	1710	1467	0.11%	0.014%
52	9.260	2538	2541	2544	rVB3	1403	905	0.07%	0.009%
53	9.373	2574	2576	2581	rVB6	1755	1396	0.11%	0.014%
54	9.450	2597	2600	2603	rBV5	1195	1046	0.08%	0.010%
55	9.473	2605	2607	2611	rVV4	822	704	0.05%	0.007%
56	9.553	2628	2632	2634	rBV5	1708	1582	0.12%	0.015%
57	9.765	2696	2698	2702	rBV4	1466	970	0.07%	0.010%
58	9.788	2702	2705	2708	rBV3	1018	748	0.06%	0.007%
59	9.839	2718	2721	2722	rBV3	1955	1265	0.10%	0.012%
60	10.006	2770	2773	2775	rBV3	1027	701	0.05%	0.007%
61	10.100	2799	2802	2805	rVB4	1509	1007	0.08%	0.010%
62	10.238	2834	2845	2859	rVB	385959	592226	44.66%	5.802%
63	10.527	2931	2935	2940	rBV7	1372	1397	0.11%	0.014%
64	10.759	3005	3007	3009	rBV2	1499	945	0.07%	0.009%
65	10.800	3016	3020	3021	rBV4	1933	1497	0.11%	0.015%
66	10.878	3042	3044	3049	rVB5	1512	1079	0.08%	0.011%
67	10.903	3049	3052	3055	rBV5	889	712	0.05%	0.007%
68	10.964	3069	3071	3077	rBV7	1474	1531	0.12%	0.015%
69	11.032	3088	3092	3094	rBV3	1458	965	0.07%	0.009%
70	11.186	3133	3140	3143	rBV8	2637	3012	0.23%	0.030%
71	11.270	3155	3166	3185	rBV	647992	985142	74.28%	9.651%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016901.D
 Acq On : 13 Jun 2020 00:55
 Operator : SY/MD
 Sample : VV0612WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.489	3229	3234	3237	rBV6	1867	1908	0.14%	0.019%
73	11.508	3237	3240	3244	rVV4	1308	1210	0.09%	0.012%
74	11.646	3271	3283	3300	rBV	688933	1072660	80.88%	10.508%
75	11.881	3354	3356	3358	rBV3	1595	813	0.06%	0.008%
76	11.958	3377	3380	3382	rBV3	1787	1017	0.08%	0.010%
77	12.019	3396	3399	3404	rBV7	1579	1699	0.13%	0.017%
78	12.061	3410	3412	3417	rBV5	1376	695	0.05%	0.007%
79	12.087	3417	3420	3422	rBV3	1220	865	0.07%	0.008%
80	12.128	3430	3433	3434	rBV3	1497	863	0.07%	0.008%
81	12.161	3438	3443	3447	rVV8	1971	1969	0.15%	0.019%
82	12.186	3447	3451	3454	rVB4	1241	1059	0.08%	0.010%
83	12.508	3549	3551	3554	rBV3	1288	804	0.06%	0.008%
84	12.739	3620	3623	3625	rBV3	1457	851	0.06%	0.008%
85	12.913	3674	3677	3680	rBV4	1092	940	0.07%	0.009%
86	13.077	3724	3728	3729	rBV3	1111	721	0.05%	0.007%
87	13.119	3737	3741	3744	rBV6	1674	1557	0.12%	0.015%
88	13.180	3756	3760	3762	rBV5	2195	1510	0.11%	0.015%
89	13.276	3787	3790	3792	rBV3	1738	1257	0.09%	0.012%
90	13.530	3857	3869	3873	rBV3	3423	6041	0.46%	0.059%
91	13.604	3889	3892	3895	rVB4	1611	792	0.06%	0.008%
92	13.624	3895	3898	3899	rBV3	1295	886	0.07%	0.009%
93	13.691	3914	3919	3926	rBV8	1781	3070	0.23%	0.030%
94	13.797	3950	3952	3954	rBV3	1781	1049	0.08%	0.010%
95	14.543	4182	4184	4187	rBV4	1002	812	0.06%	0.008%
96	14.694	4228	4231	4233	rBV4	1456	802	0.06%	0.008%
97	14.736	4241	4244	4248	rBV5	1825	1389	0.10%	0.014%
98	14.926	4301	4303	4305	rBV3	1478	904	0.07%	0.009%
99	15.061	4343	4345	4350	rBV6	1776	1262	0.10%	0.012%
100	15.656	4527	4530	4533	rBV3	2692	2096	0.16%	0.021%


Sum of corrected areas: 10207780

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016901.D
Acq On : 13 Jun 2020 00:55
Operator : SY/MD
Sample : VV0612WBL03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

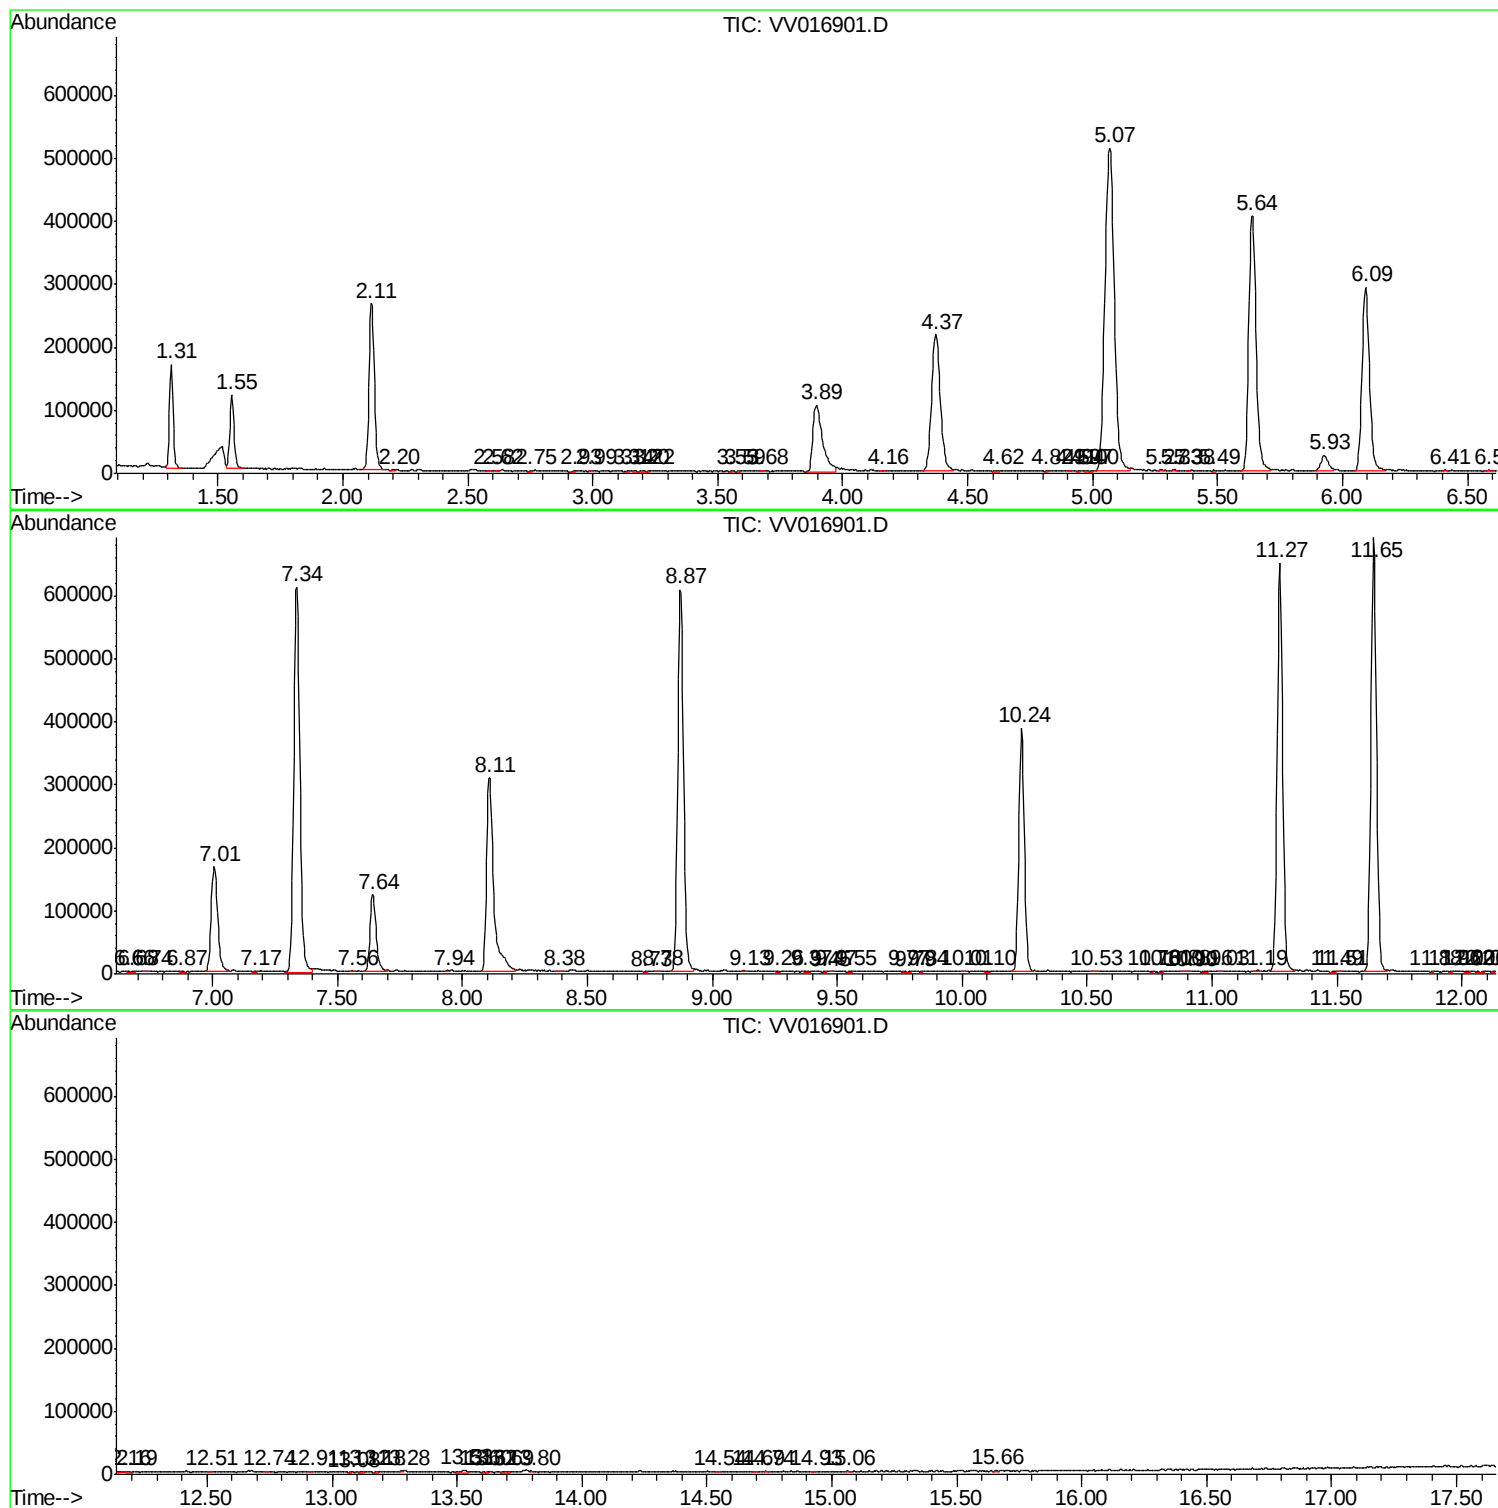

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016901.D
Acq On : 13 Jun 2020 00:55
Operator : SY/MD
Sample : VV0612WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016901.D
Acq On : 13 Jun 2020 00:55
Operator : SY/MD
Sample : VV0612WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK85

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc