

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016903.D
 Acq On : 13 Jun 2020 01:43
 Operator : SY/MD
 Sample : L2913-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	173312	172539	11.79%	1.570%
2	1.569	144	149	161	rVB	120831	135468	9.25%	1.233%
3	2.119	311	320	340	rVB	281795	426780	29.16%	3.883%
4	2.332	383	386	387	rBV3	1314	888	0.06%	0.008%
5	2.569	457	460	462	rBV3	1462	704	0.05%	0.006%
6	2.881	555	557	559	rBV3	1552	909	0.06%	0.008%
7	3.077	616	618	620	rBV2	1659	842	0.06%	0.008%
8	3.148	638	640	644	rBV3	1183	669	0.05%	0.006%
9	3.196	652	655	659	rVB6	1395	1261	0.09%	0.011%
10	3.270	676	678	680	rVB3	1382	697	0.05%	0.006%
11	3.283	680	682	687	rBV4	1482	1193	0.08%	0.011%
12	3.312	687	691	693	rBV4	1449	1049	0.07%	0.010%
13	3.399	714	718	719	rBV3	851	706	0.05%	0.006%
14	3.425	724	726	731	rVB4	874	720	0.05%	0.007%
15	3.505	745	751	752	rBV5	1616	1094	0.07%	0.010%
16	3.528	756	758	761	rVB3	1759	990	0.07%	0.009%
17	3.605	778	782	785	rBV5	1415	1302	0.09%	0.012%
18	3.820	847	849	853	rBV3	1379	1268	0.09%	0.012%
19	3.901	863	874	906	rBV	111850	318754	21.78%	2.900%
20	4.229	973	976	977	rBV3	1507	1047	0.07%	0.010%
21	4.373	1007	1021	1045	rBV	239138	576431	39.38%	5.245%
22	4.576	1079	1084	1088	rBV7	2341	2750	0.19%	0.025%
23	4.811	1155	1157	1159	rBV2	1154	682	0.05%	0.006%
24	4.865	1171	1174	1176	rBV2	1238	876	0.06%	0.008%
25	4.907	1184	1187	1189	rBV4	1742	925	0.06%	0.008%
26	5.071	1219	1238	1262	rBV2	570604	1463734	100.00%	13.318%
27	5.482	1364	1366	1368	rBV3	1458	776	0.05%	0.007%
28	5.573	1392	1394	1399	rVB4	2565	1761	0.12%	0.016%
29	5.640	1399	1415	1443	rBV	455095	915091	62.52%	8.326%
30	5.926	1497	1504	1519	rVB3	26937	55016	3.76%	0.501%
31	6.093	1542	1556	1577	rBV	330300	661853	45.22%	6.022%
32	6.322	1623	1627	1629	rBV4	1159	911	0.06%	0.008%
33	6.405	1649	1653	1656	rBV4	1188	1192	0.08%	0.011%
34	6.762	1759	1764	1765	rBV3	1338	856	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016903.D
 Acq On : 13 Jun 2020 01:43
 Operator : SY/MD
 Sample : L2913-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.836	1784	1787	1788	rBV3	1361	671	0.05%	0.006%
36	6.923	1807	1814	1815	rBV5	1345	1108	0.08%	0.010%
37	7.007	1830	1840	1861	rBV	185630	325387	22.23%	2.961%
38	7.161	1883	1888	1892	rBV8	1634	1942	0.13%	0.018%
39	7.270	1921	1922	1927	rBV4	1087	832	0.06%	0.008%
40	7.338	1927	1943	1966	rBV	682217	1167490	79.76%	10.623%
41	7.640	2028	2037	2052	rBV	130892	224423	15.33%	2.042%
42	7.865	2101	2107	2110	rBV8	1332	1109	0.08%	0.010%
43	7.891	2110	2115	2117	rVB5	1782	1382	0.09%	0.013%
44	7.910	2117	2121	2123	rBV4	1483	1118	0.08%	0.010%
45	7.990	2144	2146	2148	rBV3	1651	932	0.06%	0.008%
46	8.013	2151	2153	2156	rVV4	1693	754	0.05%	0.007%
47	8.109	2173	2183	2213	rBV2	314582	634767	43.37%	5.776%
48	8.344	2253	2256	2260	rBV5	2078	1497	0.10%	0.014%
49	8.418	2275	2279	2280	rBV3	1779	1029	0.07%	0.009%
50	8.598	2333	2335	2339	rBV5	1269	1268	0.09%	0.012%
51	8.695	2361	2365	2369	rBV5	1423	1094	0.07%	0.010%
52	8.807	2398	2400	2403	rVB3	1694	859	0.06%	0.008%
53	8.875	2408	2421	2444	rBV	679761	1099221	75.10%	10.002%
54	9.225	2526	2530	2534	rBV6	1639	1417	0.10%	0.013%
55	9.415	2585	2589	2593	rBV5	2475	2657	0.18%	0.024%
56	9.508	2613	2618	2619	rBV4	1961	1438	0.10%	0.013%
57	9.521	2619	2622	2624	rVV4	1424	669	0.05%	0.006%
58	9.772	2695	2700	2702	rBV7	1404	1134	0.08%	0.010%
59	9.833	2716	2719	2722	rBV4	1092	755	0.05%	0.007%
60	10.193	2829	2831	2834	rBV4	1124	720	0.05%	0.007%
61	10.238	2834	2845	2863	rVV	395457	627991	42.90%	5.714%
62	10.492	2922	2924	2930	rVB7	1311	979	0.07%	0.009%
63	10.579	2947	2951	2956	rVB8	1709	1491	0.10%	0.014%
64	10.604	2956	2959	2962	rBV4	1941	1554	0.11%	0.014%
65	11.022	3086	3089	3091	rVB4	1299	695	0.05%	0.006%
66	11.055	3096	3099	3100	rBV3	1341	706	0.05%	0.006%
67	11.093	3109	3111	3118	rBV7	1895	1519	0.10%	0.014%
68	11.209	3144	3147	3150	rBV4	2222	1882	0.13%	0.017%
69	11.270	3154	3166	3183	rBV	647946	1010533	69.04%	9.195%
70	11.498	3233	3237	3242	rVB7	1600	1743	0.12%	0.016%
71	11.572	3257	3260	3262	rBV4	1661	1165	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016903.D
 Acq On : 13 Jun 2020 01:43
 Operator : SY/MD
 Sample : L2913-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3300	rBV	695549	1082048	73.92%	9.845%
73	11.887	3354	3358	3360	rBV5	1076	740	0.05%	0.007%
74	11.932	3368	3372	3376	rBV5	1693	1572	0.11%	0.014%
75	12.145	3433	3438	3441	rBV4	1576	1439	0.10%	0.013%
76	12.219	3459	3461	3465	rBV5	1097	989	0.07%	0.009%
77	12.479	3538	3542	3544	rBV3	1268	699	0.05%	0.006%
78	12.492	3544	3546	3549	rVV4	1955	983	0.07%	0.009%
79	12.521	3552	3555	3559	rBV5	1240	902	0.06%	0.008%
80	12.627	3585	3588	3591	rVB4	1740	1155	0.08%	0.011%
81	12.643	3591	3593	3595	rBV3	1821	1036	0.07%	0.009%
82	12.669	3597	3601	3602	rBV4	1419	1054	0.07%	0.010%
83	12.698	3607	3610	3611	rBV2	1552	813	0.06%	0.007%
84	12.858	3658	3660	3662	rVB3	2361	995	0.07%	0.009%
85	13.106	3734	3737	3739	rBV4	1019	716	0.05%	0.007%
86	13.190	3760	3763	3767	rBV3	1367	1310	0.09%	0.012%
87	13.228	3772	3775	3781	rBV7	1829	2196	0.15%	0.020%
88	13.383	3820	3823	3827	rBV4	1328	886	0.06%	0.008%
89	13.447	3839	3843	3845	rBV3	1504	918	0.06%	0.008%
90	13.585	3884	3886	3887	rBV2	2246	915	0.06%	0.008%
91	13.649	3904	3906	3909	rBV3	1195	934	0.06%	0.008%
92	13.688	3915	3918	3921	rBV3	1289	1043	0.07%	0.009%
93	13.752	3935	3938	3940	rBV3	2600	1662	0.11%	0.015%
94	14.019	4017	4021	4023	rBV3	1322	984	0.07%	0.009%
95	14.029	4023	4024	4027	rBV3	1381	798	0.05%	0.007%
96	14.778	4255	4257	4259	rBV3	1658	854	0.06%	0.008%
97	14.842	4272	4277	4278	rBV4	1409	1131	0.08%	0.010%
98	15.206	4387	4390	4391	rBV2	1962	950	0.06%	0.009%
99	15.280	4409	4413	4415	rBV5	1266	871	0.06%	0.008%
100	15.489	4474	4478	4481	rBV5	2106	2155	0.15%	0.020%


Sum of corrected areas: 10990413

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016903.D
Acq On : 13 Jun 2020 01:43
Operator : SY/MD
Sample : L2913-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

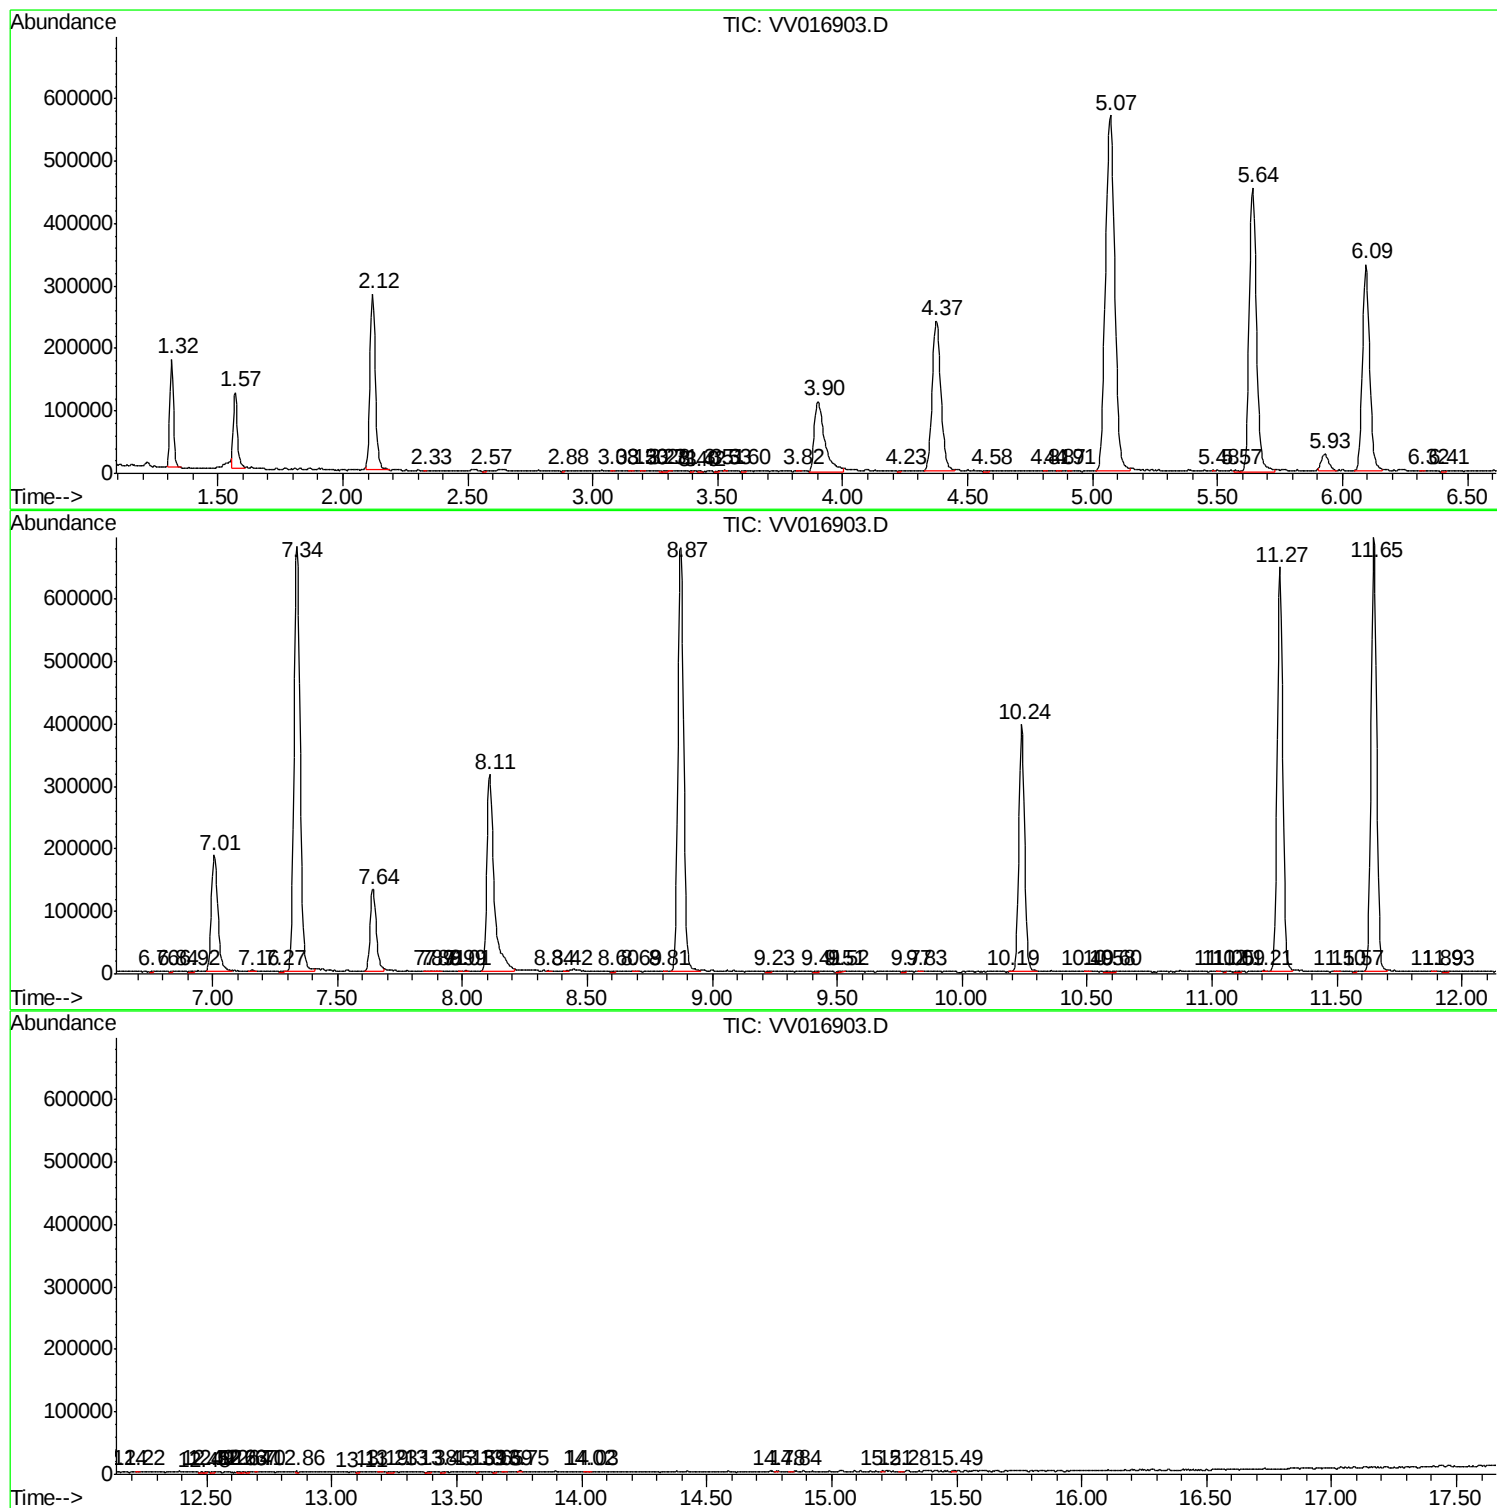

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016903.D
Acq On : 13 Jun 2020 01:43
Operator : SY/MD
Sample : L2913-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016903.D
Acq On : 13 Jun 2020 01:43
Operator : SY/MD
Sample : L2913-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc