

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016904.D
 Acq On : 13 Jun 2020 02:07
 Operator : SY/MD
 Sample : VIBLK52
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	158862	160252	11.25%	1.492%
2	1.569	144	149	166	rVB	109514	131443	9.22%	1.224%
3	2.119	310	320	337	rVB	262513	396710	27.84%	3.694%
4	2.245	357	359	362	rBV3	1072	703	0.05%	0.007%
5	2.479	429	432	433	rBV3	1739	997	0.07%	0.009%
6	2.592	463	467	468	rBV4	1029	659	0.05%	0.006%
7	2.733	509	511	513	rBV3	1140	656	0.05%	0.006%
8	2.897	558	562	564	rBV3	1485	1293	0.09%	0.012%
9	2.946	574	577	578	rBV3	978	486	0.03%	0.005%
10	2.962	578	582	584	rVV3	1017	707	0.05%	0.007%
11	3.036	600	605	608	rBV9	1416	1645	0.12%	0.015%
12	3.081	617	619	622	rBV4	1532	779	0.05%	0.007%
13	3.094	622	623	628	rVB5	1229	768	0.05%	0.007%
14	3.212	657	660	661	rBV3	881	509	0.04%	0.005%
15	3.293	683	685	688	rBV3	1638	1263	0.09%	0.012%
16	3.331	694	697	700	rBV4	1915	905	0.06%	0.008%
17	3.354	700	704	708	rVB5	1323	1098	0.08%	0.010%
18	3.383	711	713	717	rBV5	1243	1026	0.07%	0.010%
19	3.428	723	727	728	rBV3	1667	1176	0.08%	0.011%
20	3.463	736	738	740	rBV3	1110	544	0.04%	0.005%
21	3.592	770	778	781	rBV9	1909	2691	0.19%	0.025%
22	3.737	820	823	824	rBV3	827	463	0.03%	0.004%
23	3.765	828	832	836	rVB7	1688	1420	0.10%	0.013%
24	3.794	836	841	844	rVB6	1846	1870	0.13%	0.017%
25	3.811	844	846	849	rBV3	1135	908	0.06%	0.008%
26	3.856	857	860	863	rBV4	1854	1159	0.08%	0.011%
27	3.901	863	874	906	rBV	110817	322143	22.61%	3.000%
28	4.373	1008	1021	1041	rBV2	230890	555675	39.00%	5.174%
29	4.984	1208	1211	1212	rBV4	1260	772	0.05%	0.007%
30	5.071	1221	1238	1263	rBV2	556674	1424979	100.00%	13.269%
31	5.495	1366	1370	1371	rBV3	1979	1319	0.09%	0.012%
32	5.640	1403	1415	1445	rBV	450877	896834	62.94%	8.351%
33	6.093	1544	1556	1575	rBV	320652	638514	44.81%	5.946%
34	6.502	1681	1683	1686	rBV3	977	654	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016904.D
 Acq On : 13 Jun 2020 02:07
 Operator : SY/MD
 Sample : VIBLK52
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.643	1725	1727	1729	rBV3	849	381	0.03%	0.004%
36	6.798	1771	1775	1779	rBV6	1869	1414	0.10%	0.013%
37	6.817	1779	1781	1782	rBV2	1540	676	0.05%	0.006%
38	6.868	1794	1797	1803	rBV6	1877	2082	0.15%	0.019%
39	7.007	1829	1840	1860	rBV	179102	322778	22.65%	3.006%
40	7.257	1911	1918	1923	rBV10	1965	2800	0.20%	0.026%
41	7.293	1927	1929	1930	rBV2	1344	555	0.04%	0.005%
42	7.338	1930	1943	1959	rBV	655511	1129312	79.25%	10.516%
43	7.640	2028	2037	2056	rBV	129352	223613	15.69%	2.082%
44	7.794	2083	2085	2088	rVB4	1588	970	0.07%	0.009%
45	7.810	2088	2090	2093	rBV3	937	696	0.05%	0.006%
46	8.109	2173	2183	2219	rBV2	308366	628896	44.13%	5.856%
47	8.566	2322	2325	2329	rVB4	1854	1420	0.10%	0.013%
48	8.653	2350	2352	2354	rBV3	1545	676	0.05%	0.006%
49	8.711	2367	2370	2371	rBV3	1244	783	0.05%	0.007%
50	8.875	2407	2421	2437	rBV	673490	1098860	77.11%	10.233%
51	9.508	2615	2618	2619	rBV2	1552	731	0.05%	0.007%
52	9.534	2624	2626	2628	rVB2	1731	685	0.05%	0.006%
53	9.559	2628	2634	2635	rBV5	1527	1539	0.11%	0.014%
54	9.887	2734	2736	2740	rVB3	1392	782	0.05%	0.007%
55	10.106	2802	2804	2806	rBV3	1301	558	0.04%	0.005%
56	10.196	2828	2832	2833	rBV3	870	518	0.04%	0.005%
57	10.238	2833	2845	2862	rVV	400119	625532	43.90%	5.825%
58	10.318	2868	2870	2871	rBV2	1726	662	0.05%	0.006%
59	10.421	2900	2902	2906	rVB3	2207	1312	0.09%	0.012%
60	10.457	2906	2913	2916	rBV8	1944	2759	0.19%	0.026%
61	10.521	2931	2933	2935	rBV3	1242	712	0.05%	0.007%
62	10.569	2942	2948	2951	rBV6	2354	2608	0.18%	0.024%
63	10.585	2951	2953	2954	rBV2	1027	369	0.03%	0.003%
64	10.627	2964	2966	2968	rBV3	1052	375	0.03%	0.003%
65	10.662	2975	2977	2979	rBV3	1263	768	0.05%	0.007%
66	10.762	3005	3008	3011	rBV5	1625	1139	0.08%	0.011%
67	10.875	3042	3043	3044	rBV	1333	438	0.03%	0.004%
68	11.090	3105	3110	3112	rBV5	2037	1811	0.13%	0.017%
69	11.151	3126	3129	3130	rBV3	1610	947	0.07%	0.009%
70	11.174	3133	3136	3137	rBV3	1317	806	0.06%	0.008%
71	11.270	3150	3166	3185	rBV	676833	1030367	72.31%	9.595%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016904.D
 Acq On : 13 Jun 2020 02:07
 Operator : SY/MD
 Sample : VIBLK52
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.460	3222	3225	3226	rBV3	1283	534	0.04%	0.005%
73	11.646	3271	3283	3299	rBV	688997	1067508	74.91%	9.941%
74	12.026	3397	3401	3402	rBV3	1516	1156	0.08%	0.011%
75	12.148	3437	3439	3442	rVB3	1994	1070	0.08%	0.010%
76	12.180	3446	3449	3450	rBV3	1046	639	0.04%	0.006%
77	12.241	3465	3468	3470	rBV4	1679	1103	0.08%	0.010%
78	12.456	3532	3535	3537	rBV3	1599	1171	0.08%	0.011%
79	12.547	3561	3563	3568	rBV5	1054	963	0.07%	0.009%
80	12.592	3575	3577	3580	rVB3	1765	814	0.06%	0.008%
81	12.611	3580	3583	3587	rBV5	1268	930	0.07%	0.009%
82	12.672	3599	3602	3604	rBV5	2462	1177	0.08%	0.011%
83	12.739	3621	3623	3625	rBV3	1247	801	0.06%	0.007%
84	12.977	3695	3697	3701	rBV5	1474	907	0.06%	0.008%
85	13.042	3714	3717	3721	rBV4	2171	1614	0.11%	0.015%
86	13.093	3729	3733	3736	rBV5	2031	1468	0.10%	0.014%
87	13.128	3741	3744	3746	rBV3	953	516	0.04%	0.005%
88	13.219	3770	3772	3773	rBV2	1450	644	0.05%	0.006%
89	13.286	3790	3793	3794	rBV3	1899	1321	0.09%	0.012%
90	13.569	3879	3881	3882	rBV2	1290	591	0.04%	0.006%
91	13.617	3894	3896	3898	rBV2	968	570	0.04%	0.005%
92	13.682	3914	3916	3918	rBV	1053	535	0.04%	0.005%
93	13.723	3927	3929	3934	rBV6	1918	2001	0.14%	0.019%
94	13.762	3939	3941	3944	rBV4	1987	1170	0.08%	0.011%
95	13.807	3953	3955	3958	rBV4	1035	548	0.04%	0.005%
96	13.987	4008	4011	4014	rBV4	1449	989	0.07%	0.009%
97	14.212	4078	4081	4083	rBV3	1296	926	0.06%	0.009%
98	14.280	4099	4102	4104	rBV4	1892	1107	0.08%	0.010%
99	14.289	4104	4105	4109	rVV4	1374	719	0.05%	0.007%
100	14.527	4175	4179	4180	rBV3	1184	916	0.06%	0.009%


Sum of corrected areas: 10738758

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016904.D
Acq On : 13 Jun 2020 02:07
Operator : SY/MD
Sample : VIBLK52
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK52

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

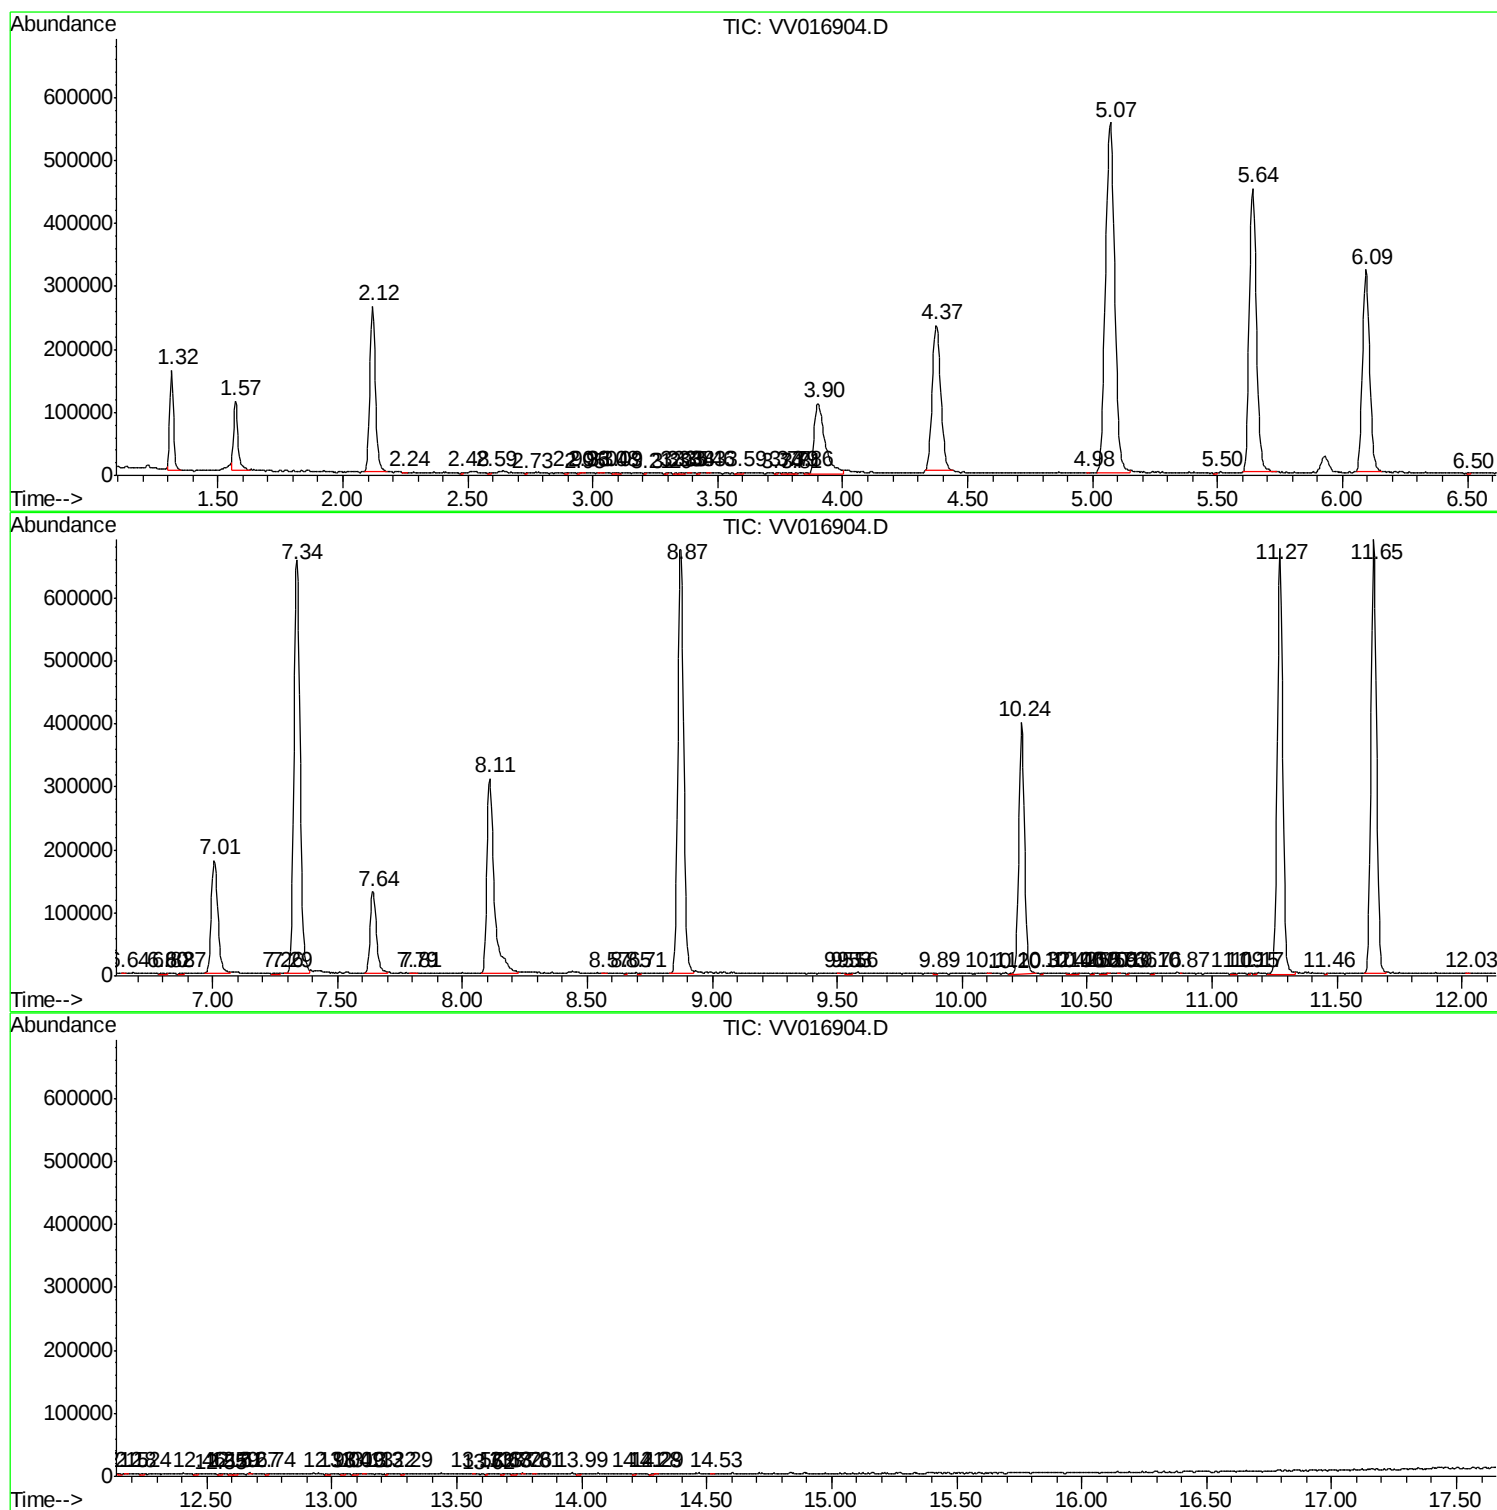

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016904.D
Acq On : 13 Jun 2020 02:07
Operator : SY/MD
Sample : VIBLK52
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK52

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV061220\
Data File : VV016904.D
Acq On : 13 Jun 2020 02:07
Operator : SY/MD
Sample : VIBLK52
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK52

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc