

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016905.D
 Acq On : 13 Jun 2020 02:30
 Operator : SY/MD
 Sample : L2915-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB	151403	147666	11.45%	1.468%
2	1.557	139	145	158	rVB	104980	123544	9.58%	1.228%
3	2.113	310	318	333	rVB	233672	349515	27.10%	3.474%
4	2.364	393	396	401	rBV6	2246	1494	0.12%	0.015%
5	2.431	414	417	420	rBV3	1968	1179	0.09%	0.012%
6	2.724	505	508	512	rBV5	1626	1725	0.13%	0.017%
7	2.807	532	534	538	rBV4	1428	1052	0.08%	0.010%
8	2.929	569	572	573	rBV3	1184	603	0.05%	0.006%
9	2.987	588	590	591	rBV2	1161	550	0.04%	0.005%
10	2.994	591	592	594	rVV2	1204	442	0.03%	0.004%
11	3.077	614	618	620	rBV5	1388	1113	0.09%	0.011%
12	3.296	682	686	687	rBV4	1460	1024	0.08%	0.010%
13	3.409	717	721	723	rBV4	1403	748	0.06%	0.007%
14	3.466	737	739	740	rBV2	1650	569	0.04%	0.006%
15	3.566	768	770	775	rVB6	2116	1534	0.12%	0.015%
16	3.589	775	777	779	rBV3	1820	1096	0.08%	0.011%
17	3.624	786	788	793	rBV6	582	525	0.04%	0.005%
18	3.669	799	802	806	rBV5	1095	1101	0.09%	0.011%
19	3.717	815	817	819	rBV3	900	367	0.03%	0.004%
20	3.743	819	825	826	rBV3	1590	1244	0.10%	0.012%
21	3.897	862	873	901	rBV	107761	295411	22.90%	2.936%
22	4.373	1008	1021	1045	rVB	213420	518072	40.17%	5.150%
23	4.569	1080	1082	1085	rBV3	2232	1342	0.10%	0.013%
24	4.634	1100	1102	1104	rBV3	1427	720	0.06%	0.007%
25	4.749	1136	1138	1139	rBV2	1018	482	0.04%	0.005%
26	4.826	1160	1162	1163	rBV2	1274	585	0.05%	0.006%
27	4.852	1166	1170	1172	rBV4	2175	1654	0.13%	0.016%
28	5.068	1221	1237	1265	rBV2	505715	1289749	100.00%	12.820%
29	5.405	1340	1342	1345	rBV4	1477	919	0.07%	0.009%
30	5.547	1384	1386	1388	rBV3	1198	527	0.04%	0.005%
31	5.637	1401	1414	1437	rBV	410735	827922	64.19%	8.229%
32	6.093	1543	1556	1576	rBV	291376	588737	45.65%	5.852%
33	6.325	1625	1628	1629	rBV3	1788	911	0.07%	0.009%
34	6.389	1647	1648	1650	rBV2	1194	465	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016905.D
 Acq On : 13 Jun 2020 02:30
 Operator : SY/MD
 Sample : L2915-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.447	1663	1666	1668	rVB3	1468	801	0.06%	0.008%
36	6.569	1701	1704	1708	rBV4	1864	1568	0.12%	0.016%
37	6.685	1737	1740	1744	rVB7	2120	1594	0.12%	0.016%
38	6.823	1779	1783	1785	rBV4	1571	1153	0.09%	0.011%
39	6.855	1790	1793	1794	rBV3	1461	743	0.06%	0.007%
40	6.910	1807	1810	1813	rBV4	1349	1007	0.08%	0.010%
41	6.945	1819	1821	1824	rBV3	1222	893	0.07%	0.009%
42	6.961	1824	1826	1829	rBV4	1537	1105	0.09%	0.011%
43	7.006	1829	1840	1858	rVV	166870	297309	23.05%	2.955%
44	7.180	1892	1894	1895	rBV2	1334	650	0.05%	0.006%
45	7.338	1931	1943	1961	rBV	596951	1021909	79.23%	10.158%
46	7.640	2028	2037	2051	rBV	119415	204811	15.88%	2.036%
47	7.897	2115	2117	2120	rBV4	1205	859	0.07%	0.009%
48	7.997	2146	2148	2149	rBV2	1353	461	0.04%	0.005%
49	8.109	2172	2183	2215	rBV2	310309	627497	48.65%	6.237%
50	8.312	2244	2246	2248	rBV3	1718	669	0.05%	0.007%
51	8.871	2409	2420	2436	rBV	626084	1001594	77.66%	9.956%
52	9.074	2481	2483	2484	rBV2	1798	726	0.06%	0.007%
53	9.231	2529	2532	2534	rBV4	1327	881	0.07%	0.009%
54	9.527	2621	2624	2626	rBV4	1341	752	0.06%	0.007%
55	9.617	2648	2652	2655	rBV6	1716	1496	0.12%	0.015%
56	9.743	2688	2691	2694	rBV3	1461	1093	0.08%	0.011%
57	10.006	2771	2773	2775	rBV3	904	379	0.03%	0.004%
58	10.064	2790	2791	2794	rBV3	1227	690	0.05%	0.007%
59	10.109	2803	2805	2810	rVB5	1429	981	0.08%	0.010%
60	10.238	2834	2845	2861	rBV	386645	605373	46.94%	6.017%
61	10.363	2880	2884	2887	rBV5	1384	1255	0.10%	0.012%
62	10.408	2897	2898	2900	rVB2	1284	435	0.03%	0.004%
63	10.437	2906	2907	2911	rBV3	1126	658	0.05%	0.007%
64	10.460	2911	2914	2916	rBV3	1494	835	0.06%	0.008%
65	10.524	2932	2934	2937	rVB3	1002	470	0.04%	0.005%
66	10.550	2937	2942	2943	rBV5	2528	1796	0.14%	0.018%
67	10.630	2965	2967	2969	rBV3	983	464	0.04%	0.005%
68	10.733	2997	2999	3003	rBV5	1609	1622	0.13%	0.016%
69	10.801	3018	3020	3024	rBV4	1183	830	0.06%	0.008%
70	10.964	3067	3071	3073	rBV4	1900	1248	0.10%	0.012%
71	11.016	3084	3087	3091	rVB4	1881	1340	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016905.D
 Acq On : 13 Jun 2020 02:30
 Operator : SY/MD
 Sample : L2915-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.038	3092	3094	3098	rBV2	1161	832	0.06%	0.008%
73	11.138	3123	3125	3128	rBV4	1120	544	0.04%	0.005%
74	11.270	3155	3166	3180	rBV	658221	1006480	78.04%	10.004%
75	11.646	3271	3283	3301	rBV	685608	1075131	83.36%	10.687%
76	12.077	3415	3417	3421	rBV4	1745	1119	0.09%	0.011%
77	12.112	3426	3428	3433	rVB5	2425	1622	0.13%	0.016%
78	12.138	3435	3436	3439	rBV2	725	409	0.03%	0.004%
79	12.186	3449	3451	3453	rBV3	1088	551	0.04%	0.005%
80	12.292	3483	3484	3487	rBV3	993	376	0.03%	0.004%
81	12.360	3503	3505	3509	rBV4	825	430	0.03%	0.004%
82	12.424	3523	3525	3530	rVB6	1800	1239	0.10%	0.012%
83	12.624	3582	3587	3588	rBV4	1654	1124	0.09%	0.011%
84	12.807	3641	3644	3646	rBV4	1166	592	0.05%	0.006%
85	12.916	3677	3678	3682	rVB4	1545	843	0.07%	0.008%
86	13.032	3713	3714	3717	rBV3	867	395	0.03%	0.004%
87	13.064	3722	3724	3726	rBV3	1077	698	0.05%	0.007%
88	13.183	3759	3761	3766	rVB5	1361	856	0.07%	0.009%
89	13.218	3769	3772	3774	rBV3	1830	984	0.08%	0.010%
90	13.263	3777	3786	3790	rBV3	2073	3036	0.24%	0.030%
91	13.312	3797	3801	3804	rBV6	999	857	0.07%	0.009%
92	13.418	3831	3834	3836	rBV3	1869	1088	0.08%	0.011%
93	13.460	3842	3847	3850	rBV6	1902	1801	0.14%	0.018%
94	13.527	3865	3868	3873	rBV6	2180	1801	0.14%	0.018%
95	13.630	3898	3900	3902	rBV3	1714	1009	0.08%	0.010%
96	13.935	3993	3995	3999	rBV3	1132	496	0.04%	0.005%
97	14.058	4031	4033	4035	rBV3	2392	1189	0.09%	0.012%
98	14.247	4089	4092	4094	rBV2	1512	1166	0.09%	0.012%
99	14.292	4104	4106	4107	rBV2	1158	444	0.03%	0.004%
100	14.334	4117	4119	4122	rVB3	1549	778	0.06%	0.008%


Sum of corrected areas: 10060424

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016905.D
Acq On : 13 Jun 2020 02:30
Operator : SY/MD
Sample : L2915-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

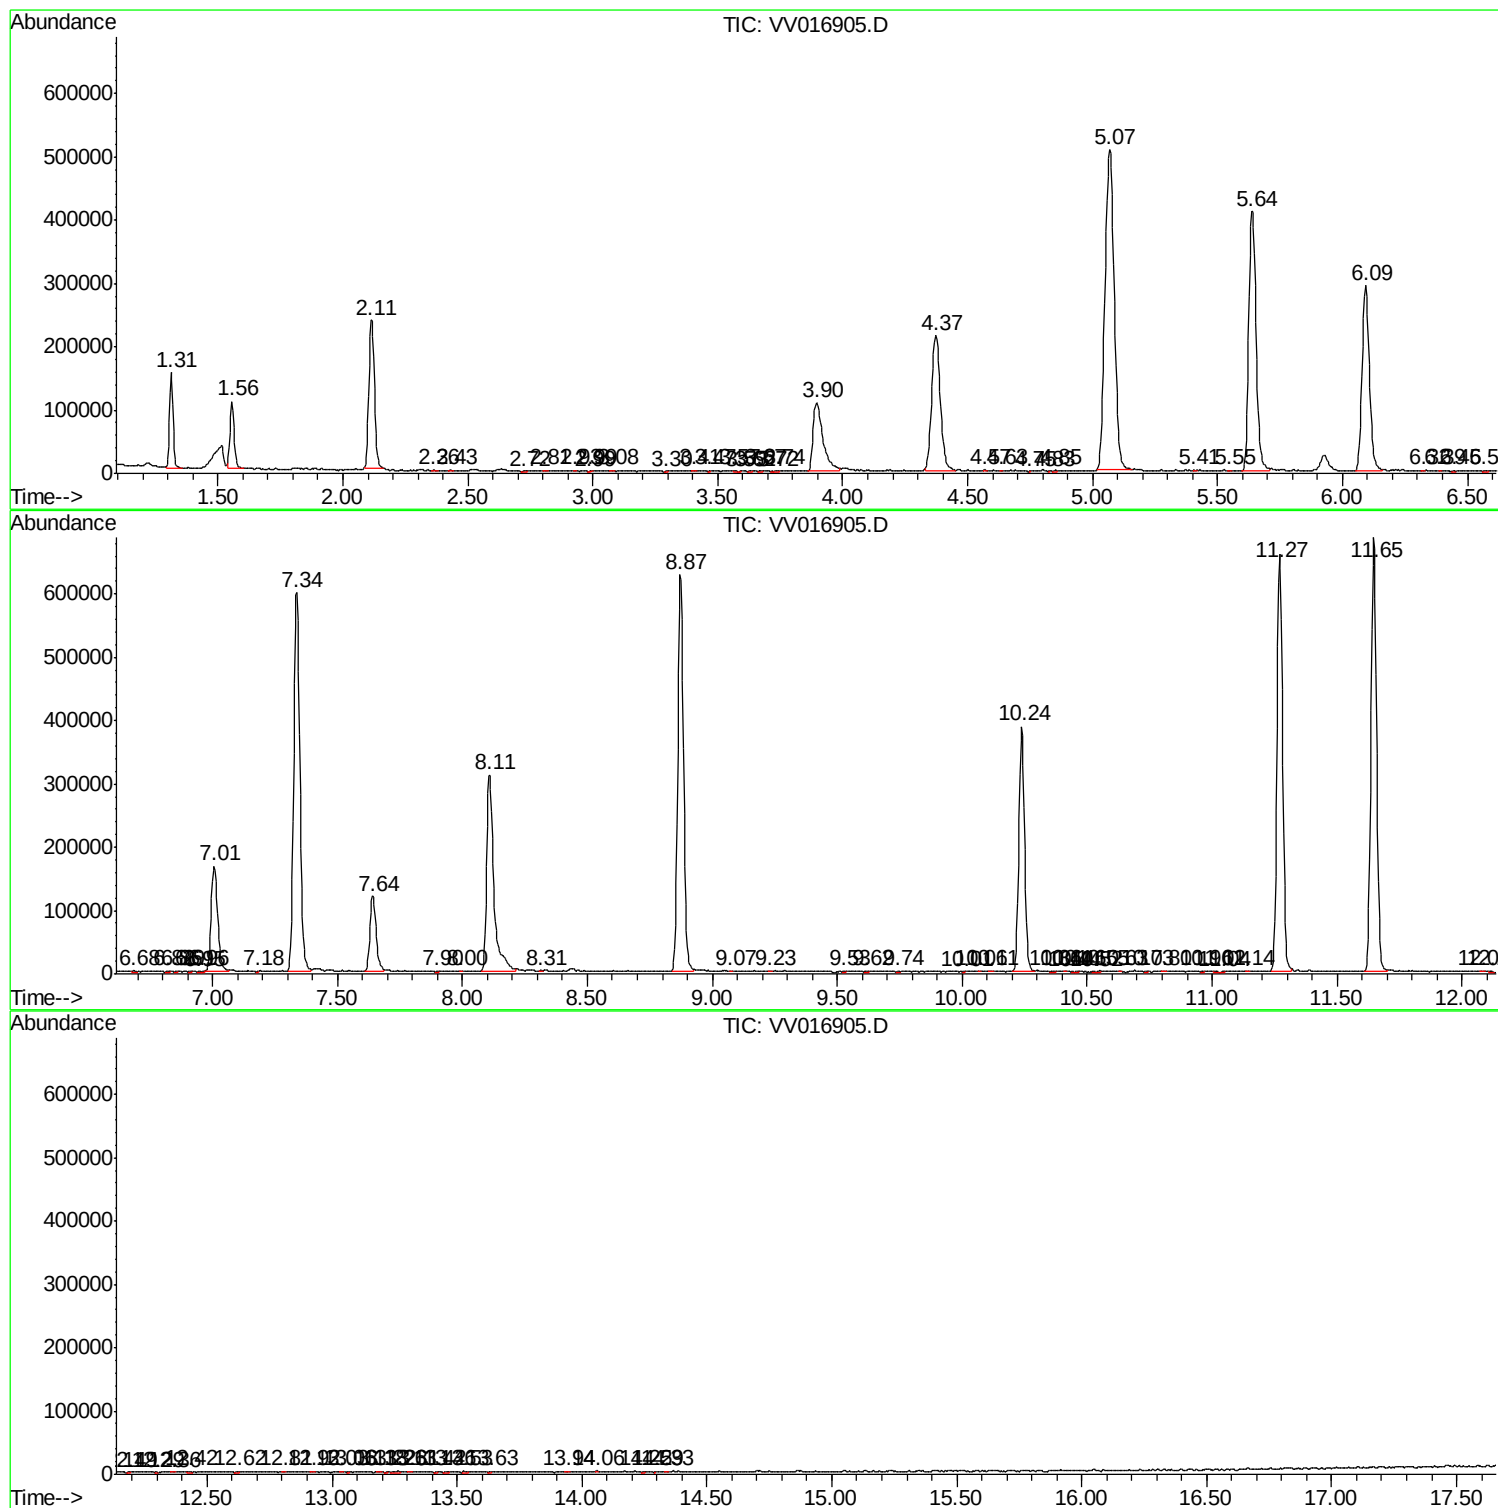

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016905.D
Acq On : 13 Jun 2020 02:30
Operator : SY/MD
Sample : L2915-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016905.D
Acq On : 13 Jun 2020 02:30
Operator : SY/MD
Sample : L2915-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc