

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016906.D
 Acq On : 13 Jun 2020 02:54
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	166945	171773	12.58%	1.663%
2	1.563	143	147	160	rVB	112289	129884	9.51%	1.258%
3	2.119	310	320	335	rBV	264933	392287	28.73%	3.798%
4	2.486	429	434	438	rBV7	2362	2330	0.17%	0.023%
5	2.608	469	472	474	rBV3	1334	784	0.06%	0.008%
6	2.708	501	503	506	rBV4	955	709	0.05%	0.007%
7	2.942	573	576	579	rVB4	1877	1160	0.08%	0.011%
8	3.020	596	600	604	rVB6	1619	1256	0.09%	0.012%
9	3.058	609	612	614	rBV4	946	833	0.06%	0.008%
10	3.087	617	621	622	rBV4	1249	1046	0.08%	0.010%
11	3.216	658	661	665	rVB5	1476	944	0.07%	0.009%
12	3.245	665	670	671	rBV4	2022	1537	0.11%	0.015%
13	3.309	687	690	691	rBV3	1106	662	0.05%	0.006%
14	3.402	716	719	721	rBV4	1789	1146	0.08%	0.011%
15	3.457	734	736	739	rBV4	1750	1045	0.08%	0.010%
16	3.492	744	747	748	rBV3	2421	1385	0.10%	0.013%
17	3.634	788	791	792	rBV3	1237	662	0.05%	0.006%
18	3.730	820	821	825	rBV4	1249	1045	0.08%	0.010%
19	3.901	863	874	903	rBV	104265	282918	20.72%	2.739%
20	4.373	1007	1021	1049	rVB	222710	546710	40.04%	5.293%
21	4.579	1083	1085	1088	rVB2	1501	723	0.05%	0.007%
22	4.753	1134	1139	1140	rBV4	1835	1563	0.11%	0.015%
23	4.843	1164	1167	1170	rBV4	1131	693	0.05%	0.007%
24	5.071	1221	1238	1262	rBV3	525692	1365572	100.00%	13.222%
25	5.212	1280	1282	1285	rBV3	1420	1108	0.08%	0.011%
26	5.421	1344	1347	1348	rBV2	1924	910	0.07%	0.009%
27	5.499	1367	1371	1373	rBV4	1930	1334	0.10%	0.013%
28	5.585	1395	1398	1400	rBV3	1660	949	0.07%	0.009%
29	5.640	1403	1415	1435	rVV	430514	850170	62.26%	8.232%
30	5.926	1492	1504	1519	rBV2	26256	59822	4.38%	0.579%
31	6.093	1543	1556	1581	rVB	308403	621969	45.55%	6.022%
32	6.180	1581	1583	1586	rBV3	1849	1135	0.08%	0.011%
33	6.521	1687	1689	1691	rBV2	1306	682	0.05%	0.007%
34	6.569	1700	1704	1707	rBV5	2027	1586	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016906.D
 Acq On : 13 Jun 2020 02:54
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.704	1742	1746	1750	rBV7	1838	1937	0.14%	0.019%
36	6.743	1756	1758	1763	rVB5	1643	919	0.07%	0.009%
37	6.855	1790	1793	1796	rBV4	1545	1264	0.09%	0.012%
38	6.949	1817	1822	1826	rBV7	1648	2177	0.16%	0.021%
39	7.007	1827	1840	1863	rVV2	173093	310488	22.74%	3.006%
40	7.203	1895	1901	1904	rBV7	1679	1835	0.13%	0.018%
41	7.286	1925	1927	1929	rBV3	1616	826	0.06%	0.008%
42	7.338	1929	1943	1961	rVV	632187	1082594	79.28%	10.482%
43	7.547	2006	2008	2013	rVB5	1511	955	0.07%	0.009%
44	7.595	2020	2023	2026	rBV4	1132	881	0.06%	0.009%
45	7.640	2026	2037	2056	rBV	124108	212847	15.59%	2.061%
46	7.743	2066	2069	2072	rVB4	2096	1488	0.11%	0.014%
47	7.833	2092	2097	2099	rBV5	1950	1343	0.10%	0.013%
48	7.904	2117	2119	2121	rBV3	1567	748	0.05%	0.007%
49	8.032	2154	2159	2160	rBV3	1181	1003	0.07%	0.010%
50	8.109	2172	2183	2212	rBV2	300439	606732	44.43%	5.875%
51	8.688	2359	2363	2370	rVB9	1554	1669	0.12%	0.016%
52	8.743	2377	2380	2383	rBV5	1632	1061	0.08%	0.010%
53	8.781	2388	2392	2394	rBV6	1524	1334	0.10%	0.013%
54	8.875	2409	2421	2443	rBV	640359	1036806	75.92%	10.039%
55	9.158	2506	2509	2510	rBV3	1350	886	0.06%	0.009%
56	9.431	2590	2594	2595	rBV4	1281	706	0.05%	0.007%
57	9.498	2611	2615	2619	rBV7	1952	1766	0.13%	0.017%
58	9.543	2625	2629	2632	rBV5	1606	1150	0.08%	0.011%
59	9.698	2672	2677	2684	rVB8	2463	3537	0.26%	0.034%
60	9.730	2684	2687	2691	rBV4	1770	1462	0.11%	0.014%
61	9.752	2691	2694	2695	rBV3	1630	841	0.06%	0.008%
62	9.791	2701	2706	2708	rBV6	1511	1369	0.10%	0.013%
63	10.145	2812	2816	2818	rVB4	1205	705	0.05%	0.007%
64	10.238	2834	2845	2863	rVB	371300	582610	42.66%	5.641%
65	10.386	2888	2891	2893	rBV4	1123	784	0.06%	0.008%
66	10.434	2902	2906	2909	rBV4	2016	1874	0.14%	0.018%
67	10.492	2920	2924	2926	rBV5	2123	1396	0.10%	0.014%
68	10.527	2933	2935	2937	rBV2	979	660	0.05%	0.006%
69	10.559	2941	2945	2946	rBV3	1855	1091	0.08%	0.011%
70	10.595	2953	2956	2962	rBV6	1104	987	0.07%	0.010%
71	10.743	2999	3002	3005	rBV3	1656	1110	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061220\
 Data File : VV016906.D
 Acq On : 13 Jun 2020 02:54
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.868	3038	3041	3042	rBV3	1334	657	0.05%	0.006%
73	10.878	3042	3044	3047	rVV2	1597	983	0.07%	0.010%
74	10.971	3070	3073	3077	rBV4	1180	932	0.07%	0.009%
75	11.106	3112	3115	3118	rBV4	1266	1135	0.08%	0.011%
76	11.170	3130	3135	3137	rBV5	1787	1509	0.11%	0.015%
77	11.206	3144	3146	3149	rBV4	2244	1128	0.08%	0.011%
78	11.270	3153	3166	3182	rBV	628096	964195	70.61%	9.336%
79	11.479	3229	3231	3233	rBV3	1288	740	0.05%	0.007%
80	11.492	3233	3235	3240	rVV6	1173	960	0.07%	0.009%
81	11.585	3262	3264	3267	rVB3	1621	712	0.05%	0.007%
82	11.646	3271	3283	3298	rBV	652357	1014213	74.27%	9.820%
83	11.913	3364	3366	3369	rVB3	2119	922	0.07%	0.009%
84	11.929	3369	3371	3375	rVB3	2728	1507	0.11%	0.015%
85	11.948	3375	3377	3379	rBV4	1608	993	0.07%	0.010%
86	11.997	3387	3392	3394	rBV3	1838	1396	0.10%	0.014%
87	12.199	3452	3455	3459	rVB5	1872	1412	0.10%	0.014%
88	12.328	3491	3495	3497	rBV5	966	748	0.05%	0.007%
89	12.376	3508	3510	3515	rBV5	1326	1078	0.08%	0.010%
90	12.418	3520	3523	3527	rBV3	1030	1087	0.08%	0.011%
91	12.527	3554	3557	3558	rBV4	1183	701	0.05%	0.007%
92	12.643	3591	3593	3597	rVB5	1844	1080	0.08%	0.010%
93	12.665	3597	3600	3603	rBV4	1519	833	0.06%	0.008%
94	12.829	3649	3651	3654	rBV4	965	825	0.06%	0.008%
95	13.019	3707	3710	3711	rBV3	1530	824	0.06%	0.008%
96	13.472	3846	3851	3853	rVV5	1794	1658	0.12%	0.016%
97	13.640	3899	3903	3907	rVB6	1872	1659	0.12%	0.016%
98	13.772	3943	3944	3948	rVB4	1370	701	0.05%	0.007%
99	14.064	4032	4035	4038	rBV3	949	658	0.05%	0.006%
100	15.675	4533	4536	4540	rBV6	2937	2799	0.20%	0.027%


Sum of corrected areas: 10328218

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061220\
Data File : VV016906.D
Acq On : 13 Jun 2020 02:54
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

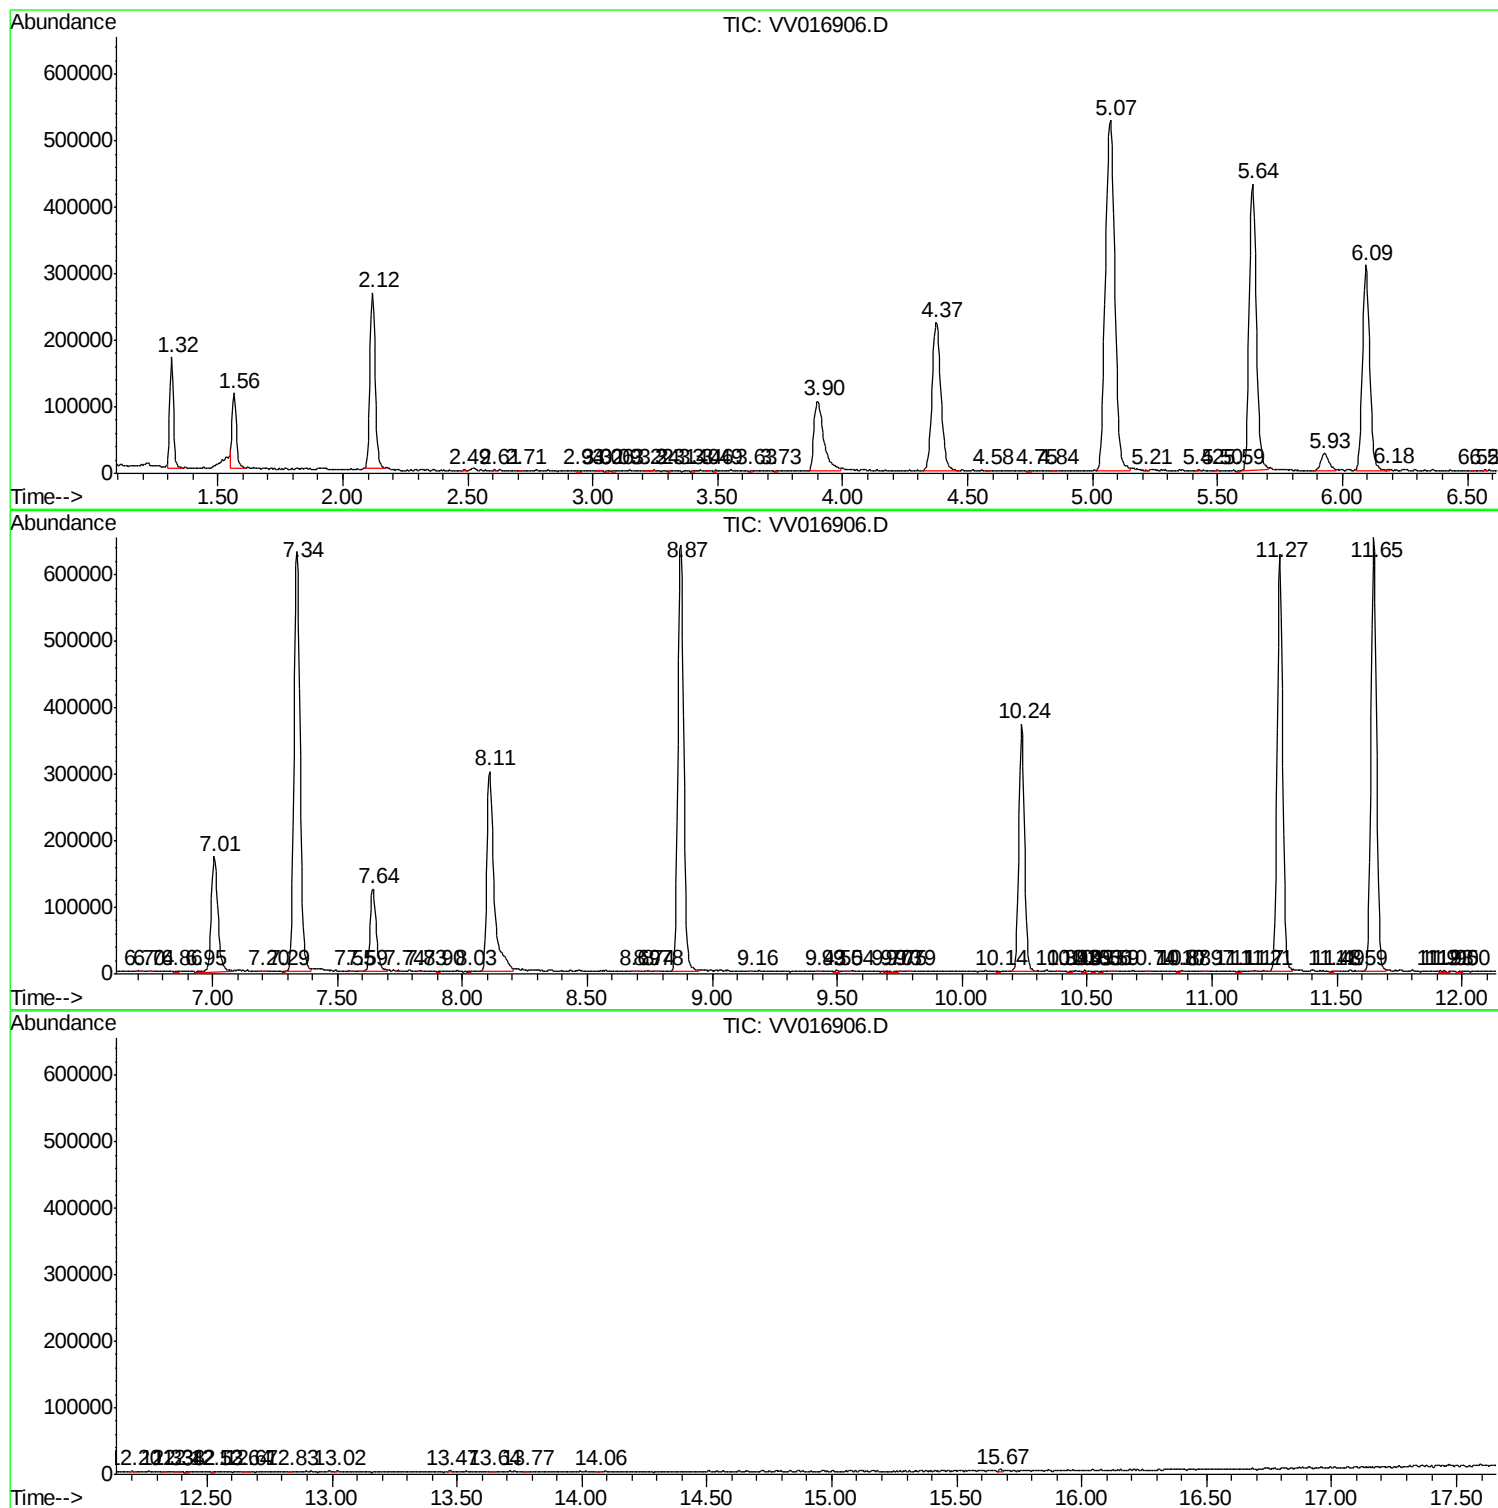

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016906.D
Acq On : 13 Jun 2020 02:54
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061220\
Data File : VV016906.D
Acq On : 13 Jun 2020 02:54
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc