


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061220\
 Data File : VV016871.D
 Acq On : 12 Jun 2020 11:26
 Operator : SY/MD
 Sample : BFB87
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB87

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Mon Jun 15 04:18:16 2020

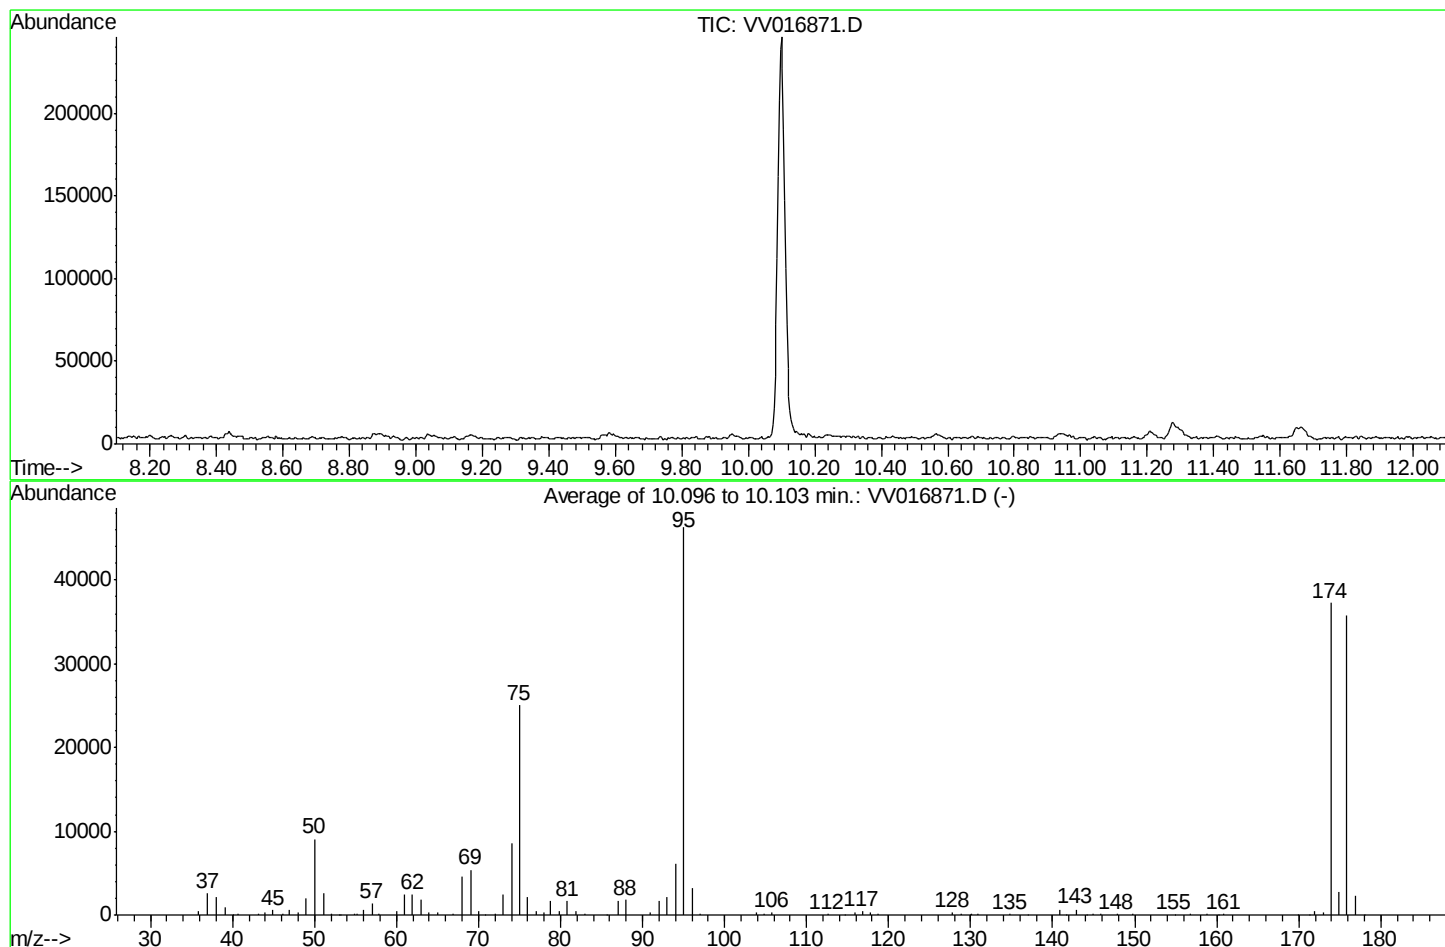

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	9051	PASS
75	95	30	80	54.1	25058	PASS
95	95	100	100	100.0	46293	PASS
96	95	5	9	6.9	3187	PASS
173	174	0.00	2	0.7	271	PASS
174	95	50	120	80.5	37253	PASS
175	174	5	9	7.6	2826	PASS
176	174	95	101	95.9	35728	PASS
177	176	5	9	6.6	2355	PASS

m/z	Abundance
36.00	612.0
37.00	2810.0
38.00	2290.0
39.10	1027.0
40.00	403.0
40.70	225.0
43.10	184.0
44.00	665.0
45.00	586.0
46.10	130.0
47.00	583.0
47.90	368.0
49.00	2296.0
50.00	9151.0
51.10	2666.0
52.10	229.0
52.90	105.0
54.40	113.0
54.80	195.0
55.20	173.0
55.90	669.0
57.00	1490.0
57.90	155.0
60.00	592.0
61.00	2389.0
61.90	2337.0
63.00	1956.0
64.10	342.0
65.00	332.0
65.90	128.0
67.00	233.0
68.00	4826.0
69.00	5528.0
70.00	370.0
72.00	227.0
73.00	2382.0
74.00	8847.0
75.00	25696.0
76.00	2201.0
77.00	396.0
78.00	233.0
78.80	1828.0
79.90	493.0
80.80	1737.0
81.90	477.0
83.00	206.0
85.70	223.0
87.00	1654.0
88.00	1773.0
90.90	280.0
92.00	1686.0
92.90	2119.0
94.00	6139.0
95.00	46904.0
96.00	3502.0
97.10	209.0
103.90	257.0
104.80	160.0
105.80	326.0
112.60	150.0
114.60	116.0
115.90	291.0
116.80	371.0
117.70	331.0
118.70	239.0
127.80	265.0
128.90	158.0
129.90	173.0
130.10	180.0
130.90	107.0
134.80	117.0
136.90	132.0
140.80	502.0
142.90	712.0
144.20	120.0
144.80	160.0
146.00	288.0
147.80	137.0
156.80	117.0
158.90	123.0
160.80	161.0
169.90	111.0
171.30	158.0
172.00	432.0
173.90	36288.0
174.90	3026.0
175.90	35048.0
176.90	2476.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.90	584.0
37.00	2755.0
38.00	2286.0
39.00	1019.0
40.00	408.0
40.60	183.0
42.40	106.0
43.10	183.0
44.00	683.0
44.90	602.0
46.10	168.0
47.00	565.0
47.90	375.0
49.00	2137.0
50.00	9339.0
51.00	2805.0
52.10	235.0
53.00	103.0
54.30	105.0
54.80	199.0
55.20	186.0
56.00	663.0
57.00	1549.0
57.80	146.0
60.00	570.0
60.90	2553.0
61.90	2552.0
63.00	1892.0
64.00	418.0
65.00	261.0
66.00	134.0
67.00	249.0
68.00	4914.0
69.00	5748.0
70.00	422.0
70.80	114.0
72.00	221.0
73.00	2598.0
74.00	8770.0
75.00	25952.0
76.00	2297.0
77.00	517.0
78.00	255.0
78.80	1903.0
79.90	497.0
80.80	1676.0
81.90	456.0
83.00	230.0
85.70	197.0
87.00	1844.0
87.90	1881.0
90.90	308.0
92.00	1773.0
92.90	2122.0
94.00	6334.0
95.00	47816.0
96.00	3242.0
97.00	171.0
103.90	257.0
104.80	183.0
105.80	271.0
112.60	163.0
115.80	261.0
116.80	414.0
117.70	339.0
118.80	233.0
127.80	307.0
128.90	135.0
130.10	212.0
130.80	138.0
134.80	149.0
136.90	106.0
140.80	605.0
141.70	108.0
142.90	613.0
144.80	173.0
145.90	232.0
147.80	152.0
149.80	123.0
156.90	118.0
158.80	114.0
160.90	139.0
171.90	420.0
173.00	815.0
173.90	38512.0
174.90	2866.0
175.90	37376.0
176.90	2417.0
178.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.90	531.0
37.00	2440.0
38.00	2036.0
39.00	917.0
40.00	371.0
40.70	125.0
42.40	140.0
43.10	132.0
44.00	698.0
44.90	544.0
46.20	167.0
46.90	484.0
48.00	367.0
49.00	1822.0
50.00	8663.0
51.00	2781.0
52.10	209.0
53.20	113.0
54.80	185.0
55.20	167.0
56.00	650.0
57.00	1371.0
57.80	161.0
60.00	514.0
60.90	2327.0
62.00	2401.0
63.00	1663.0
64.00	386.0
65.00	193.0
66.10	131.0
66.90	222.0
68.00	4495.0
69.00	5230.0
70.00	442.0
70.80	107.0
72.00	192.0
73.00	2357.0
74.00	7904.0
75.00	23528.0
76.00	2100.0
77.00	549.0
78.00	237.0
78.80	1636.0
79.80	482.0
80.90	1466.0
81.80	348.0
83.00	182.0
85.70	120.0
87.00	1789.0
87.90	1821.0
90.90	306.0
92.00	1510.0
93.00	2054.0
94.00	5846.0
95.00	44160.0
96.00	2818.0
96.90	136.0
103.90	253.0
104.80	163.0
105.90	193.0
112.60	123.0
115.80	260.0
116.80	428.0
117.80	253.0
118.80	232.0
127.80	278.0
128.90	112.0
130.00	227.0
130.90	121.0
134.80	158.0
140.80	607.0
142.80	546.0
144.90	165.0
145.80	123.0
147.90	159.0
149.80	138.0
154.90	107.0
156.90	135.0
158.80	111.0
160.20	110.0
160.90	120.0
171.90	427.0
173.90	36960.0
174.90	2587.0
175.90	35120.0
176.90	2172.0
178.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.40	145.0
35.90	140.0
37.00	135.0
38.00	121.0
38.60	100.0
39.50	164.0
40.00	318.0
41.00	166.0
42.30	129.0
42.80	173.0
44.10	368.0
45.20	150.0
45.90	107.0
48.60	116.0
49.20	102.0
51.10	105.0
52.20	106.0
54.40	103.0
56.20	182.0
57.00	105.0
60.10	128.0
63.40	135.0
64.00	101.0
66.20	132.0
67.90	101.0
69.00	130.0
78.80	107.0
85.50	109.0
88.90	131.0
91.40	150.0
132.70	112.0
161.60	107.0
176.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87