

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061222\
 Data File : VW026183.D
 Acq On : 13 Jun 2022 00:18
 Operator : SY/MD
 Sample : N3278-07 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE8

Quant Time: Jun 13 06:38:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 02:52:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	229500	5.000	ug/L	#-0.02
28) Chlorobenzene-d5	8.860	117	160191	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62125	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	37295	1.243	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	24.800%#
7) Chloroethane-d5	1.577	69	47392	2.005	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	40.000%#
11) 1,1-Dichloroethene-d2	2.114	63	59583	1.235	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	24.600%#
20) 2-Butanone-d5	3.973	46	166904	74.542	ug/L	0.06
Spiked Amount	50.000	Range	40 - 130	Recovery	=	149.080%#
24) Chloroform-d	4.368	84	117119	2.752	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	55.000%#
26) 1,2-Dichloroethane-d4	5.043	65	61482	3.583	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.600%
32) Benzene-d6	5.050	84	215946	3.458	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.200%#
36) 1,2-Dichloropropane-d6	6.069	67	65612	3.643	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	72.800%
41) Toluene-d8	7.333	98	126209	2.270	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	45.400%#
43) trans-1,3-Dichloroprop...	7.641	79	13298	2.447	ug/L	0.02
Spiked Amount	5.000	Range	55 - 130	Recovery	=	49.000%#
46) 2-Hexanone-d5	8.117	63	69468	41.046	ug/L	0.03
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.100%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	39354	3.668	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	73.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	44600	3.203	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	64.000%#
Target Compounds						
					Qvalue	
34) Trichloroethene	5.902	95	3028	0.231	ug/L	# 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026183.D
Acq On : 13 Jun 2022 00:18
Operator : SY/MD
Sample : N3278-07 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE8


Quant Time: Jun 13 06:38:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 02:52:24 2022
Response via : Initial Calibration

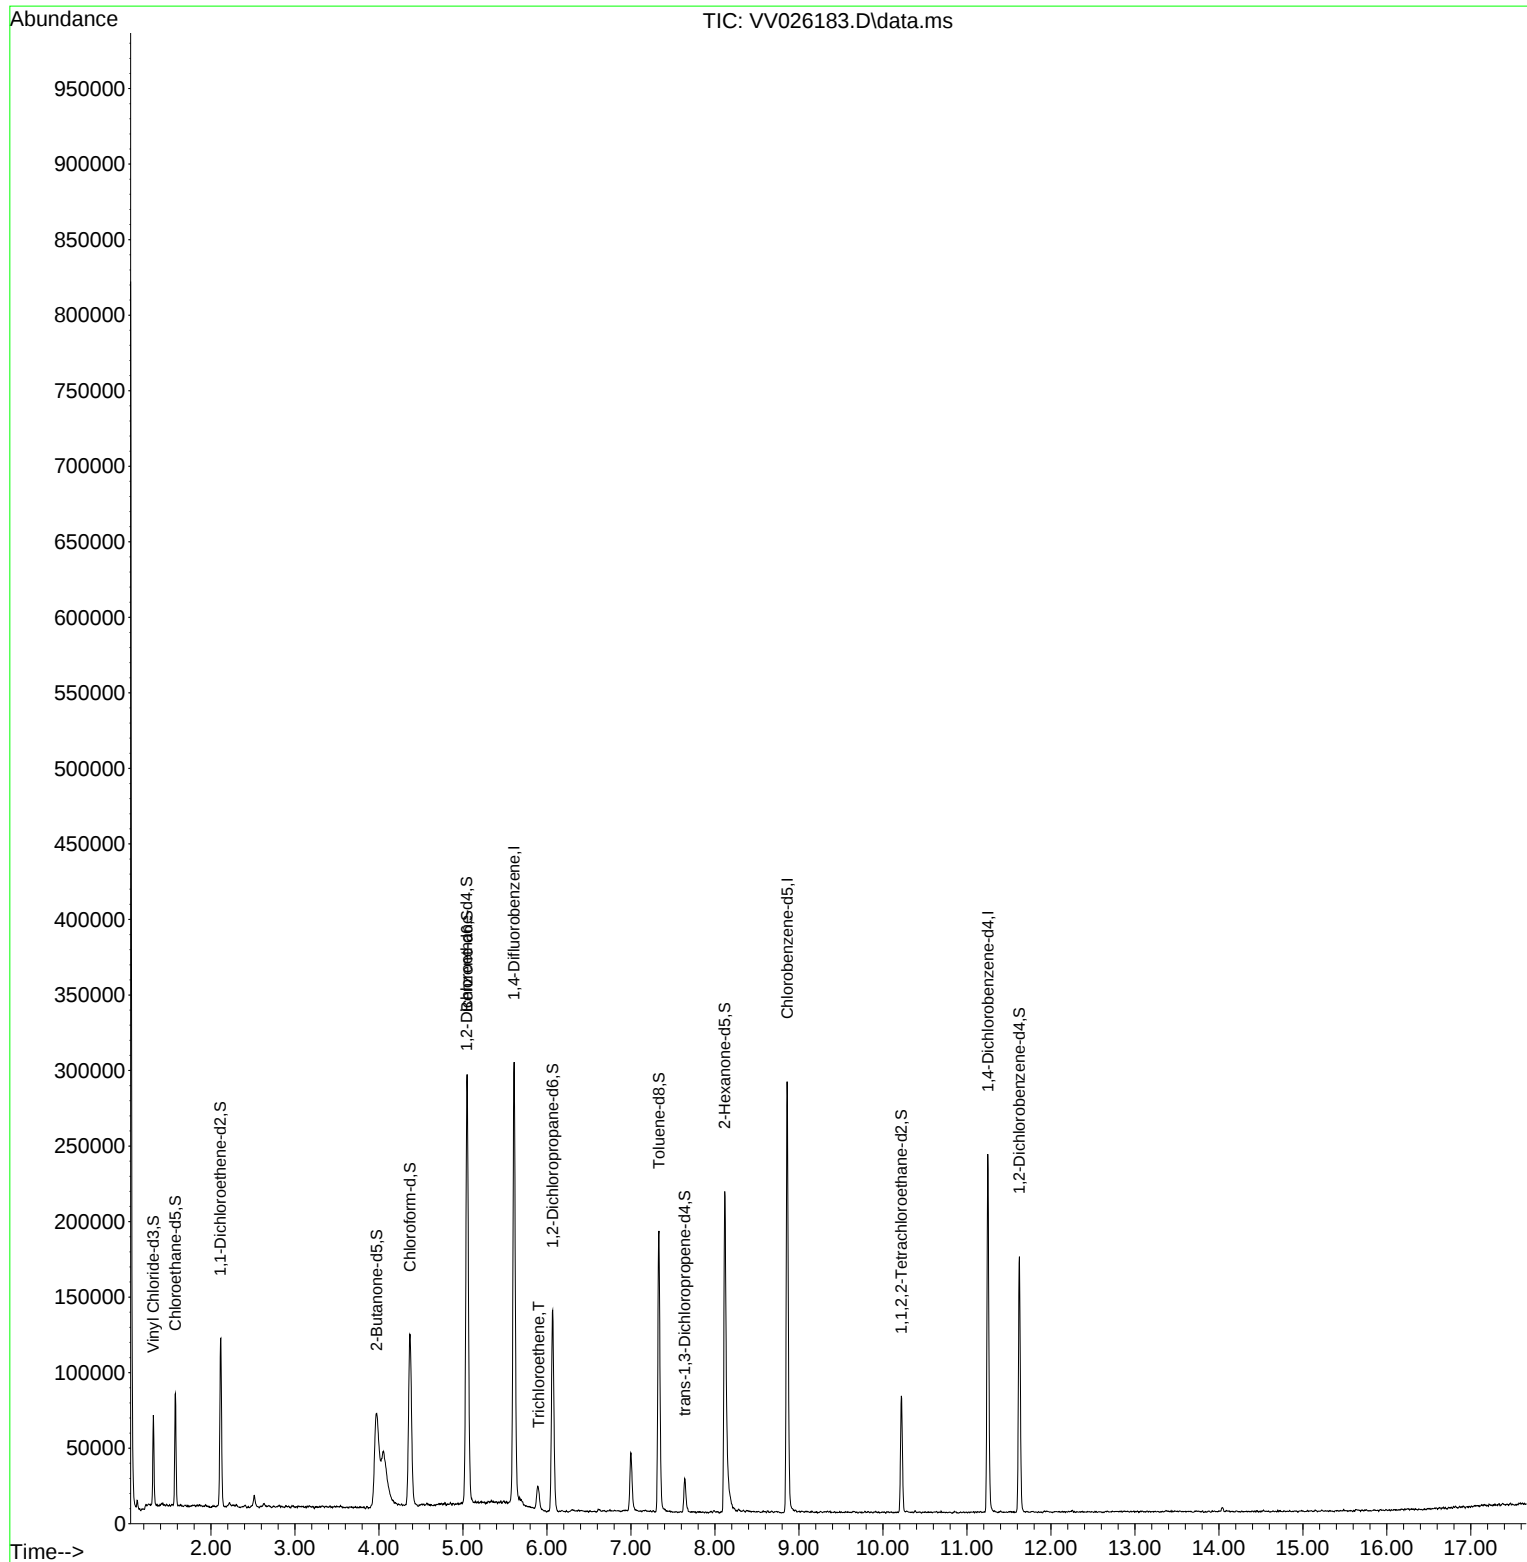

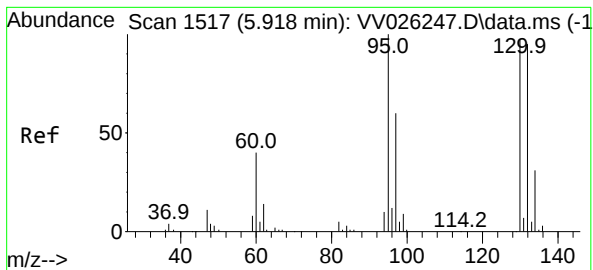

#34
 Trichloroethene
 Concen: 0.231 ug/L
 RT: 5.902 min Scan# 11
 Delta R.T. -0.019 min
 Lab File: VV026183.D
 Acq: 13 Jun 2022 00:18

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE8

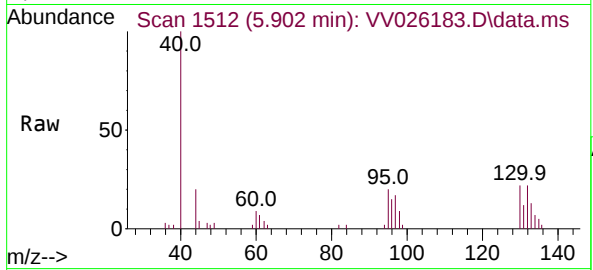

Tgt Ion: 95 Resp: 3028
 Ion Ratio Lower Upper
 95 100
 97 84.4 43.3 80.3#
 132 113.8 67.5 125.4
 130 110.9 70.9 131.7

