

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061222\
 Data File : VW026184.D
 Acq On : 13 Jun 2022 00:42
 Operator : SY/MD
 Sample : N3278-08 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE9

Quant Time: Jun 13 06:38:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Jun 13 02:52:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	166613	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	159153	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62701	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	36692	1.684	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	33.600%#
7) Chloroethane-d5	1.584	69	47651	2.777	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	55.600%#
11) 1,1-Dichloroethene-d2	2.121	63	61884	1.766	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	35.400%#
20) 2-Butanone-d5	3.915	46	75677	46.556	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.120%
24) Chloroform-d	4.362	84	104549	3.384	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	67.600%#
26) 1,2-Dichloroethane-d4	5.043	65	45162	3.625	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.600%
32) Benzene-d6	5.059	84	176178	2.839	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	56.800%#
36) 1,2-Dichloropropane-d6	6.075	67	61992	3.465	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	69.200%
41) Toluene-d8	7.320	98	129786	2.349	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	47.000%#
43) trans-1,3-Dichloroprop...	7.628	79	13205	2.445	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	49.000%#
46) 2-Hexanone-d5	8.091	63	71600	42.581	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.160%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39078	3.666	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	73.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	47181	3.357	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	67.200%#
Target Compounds						Qvalue
34) Trichloroethene	5.924	95	2935	0.226	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026184.D
Acq On : 13 Jun 2022 00:42
Operator : SY/MD
Sample : N3278-08 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE9

Quant Time: Jun 13 06:38:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 13 02:52:24 2022
Response via : Initial Calibration

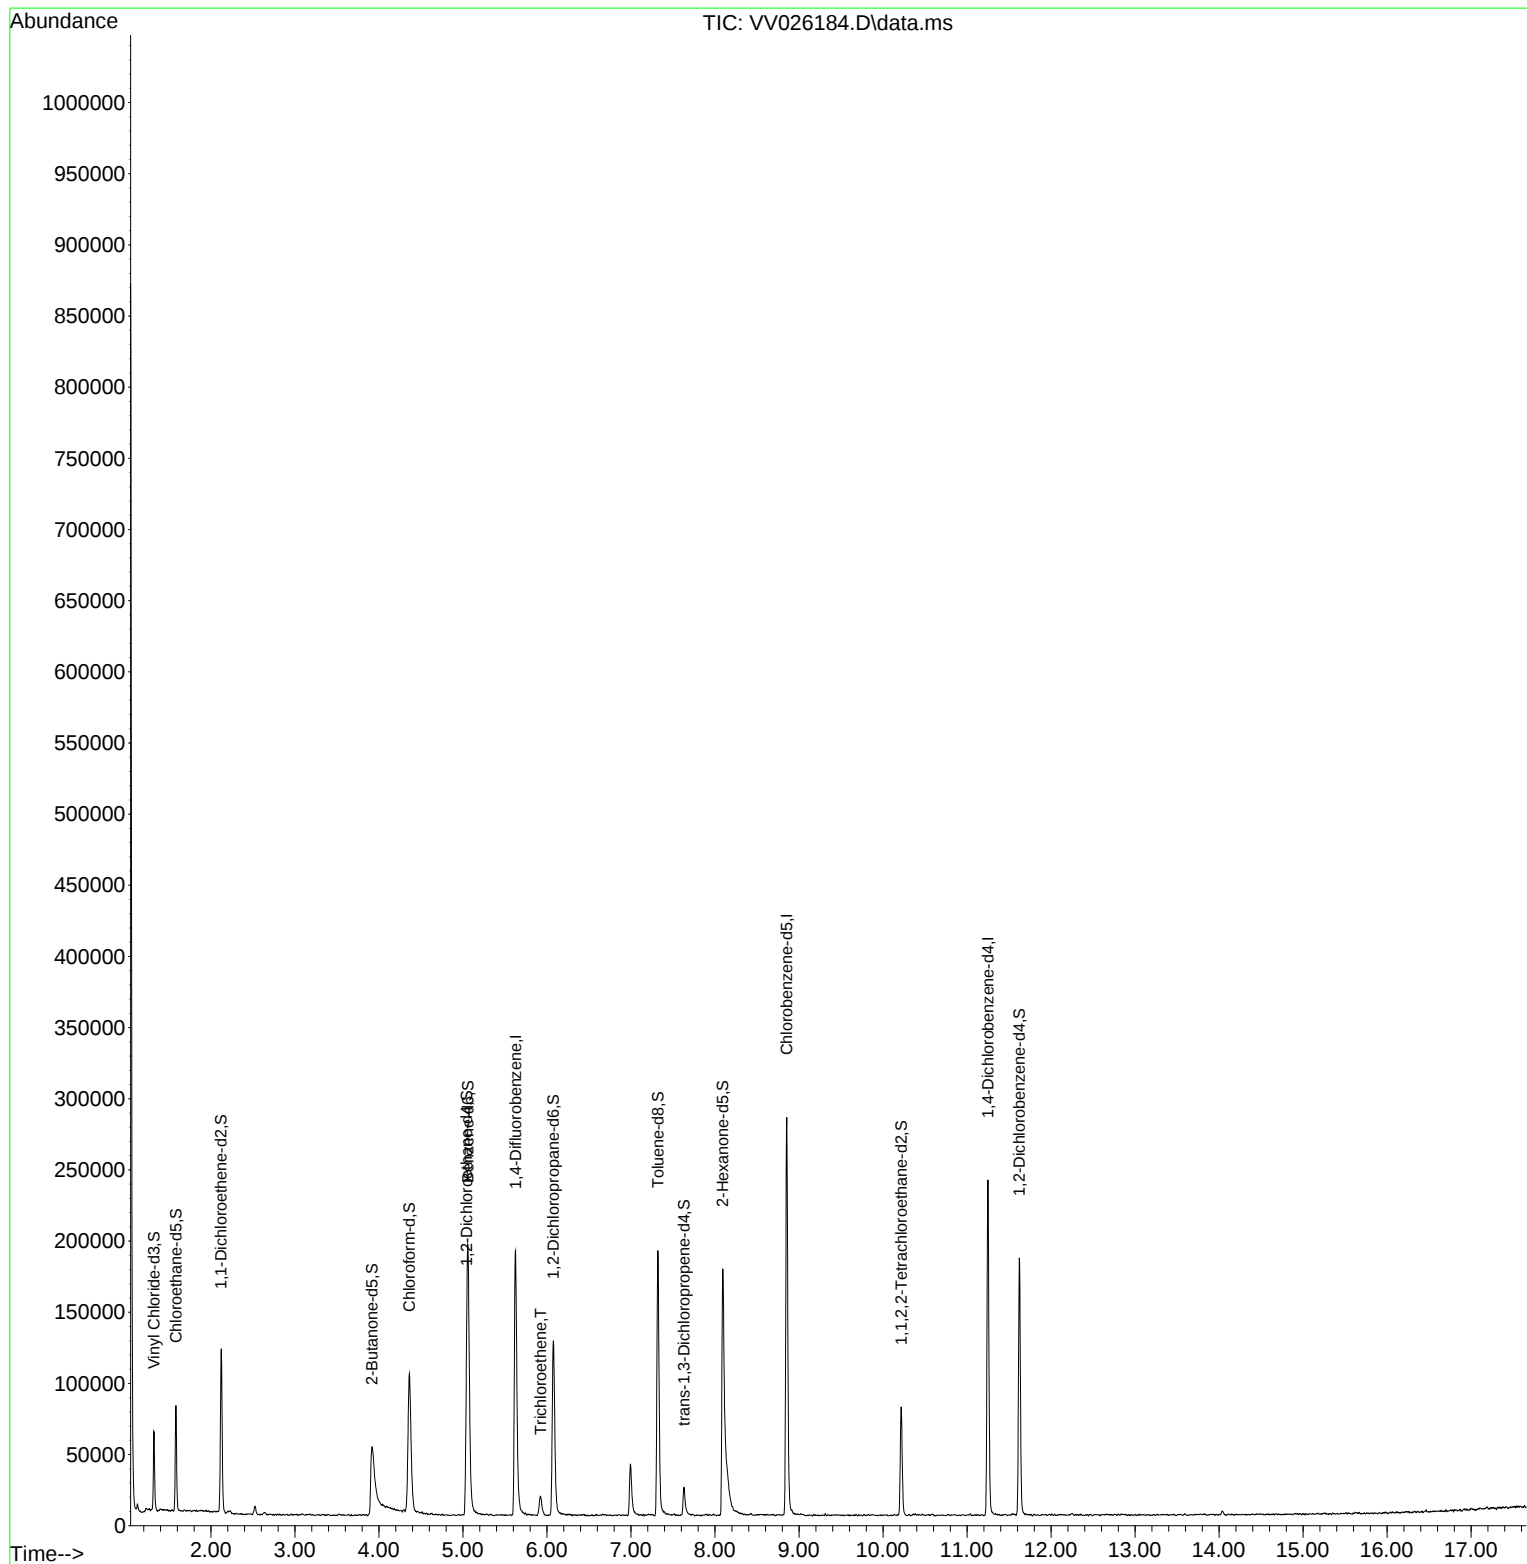

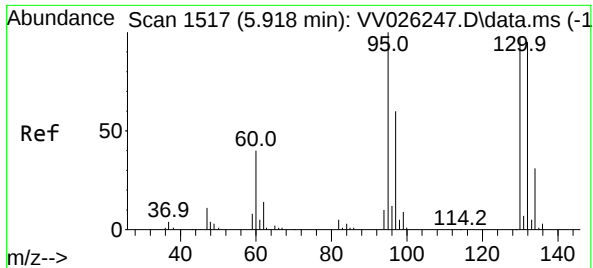

#34
 Trichloroethene
 Concen: 0.226 ug/L
 RT: 5.924 min Scan# 11
 Delta R.T. 0.003 min
 Lab File: VV026184.D
 Acq: 13 Jun 2022 00:42

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE9

Tgt Ion: 95 Resp: 2935

Ion	Ratio	Lower	Upper
95	100		
97	71.4	43.3	80.3
132	106.5	67.5	125.4
130	106.8	70.9	131.7

