

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
 Data File : VV026176.D
 Acq On : 12 Jun 2022 21:31
 Operator : SY/MD
 Sample : VV0612WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK369

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	106	rBV	165465	175370	20.75%	2.908%
2	1.584	160	169	182	rVB	133288	156195	18.49%	2.590%
3	2.121	326	336	353	rVB	267422	389123	46.05%	6.453%
4	3.915	882	894	927	rBV3	47364	185022	21.90%	3.068%
5	4.362	1018	1033	1062	rBV2	147420	375326	44.42%	6.224%
6	5.056	1231	1249	1278	rBV2	345583	844971	100.00%	14.013%
7	5.625	1415	1426	1452	rBV	197779	410162	48.54%	6.802%
8	5.921	1507	1518	1533	rBV7	7682	18016	2.13%	0.299%
9	6.076	1550	1566	1586	rBV	188746	393473	46.57%	6.525%
10	6.992	1838	1851	1874	rBV	78210	149963	17.75%	2.487%
11	7.320	1940	1953	1971	rBV	400017	698330	82.65%	11.581%
12	7.400	1974	1978	1997	rVB3	6862	13566	1.61%	0.225%
13	7.625	2038	2048	2076	rBV	43991	84996	10.06%	1.410%
14	8.092	2179	2193	2244	rBV2	224724	541039	64.03%	8.972%
15	8.419	2286	2295	2309	rVB4	10347	17680	2.09%	0.293%
16	8.854	2415	2430	2461	rBV	296734	495106	58.59%	8.211%
17	10.217	2843	2854	2868	rBV2	106385	172606	20.43%	2.862%
18	11.249	3164	3175	3196	rBV	256259	402565	47.64%	6.676%
19	11.622	3279	3291	3309	rBV	320969	506576	59.95%	8.401%




Sum of corrected areas: 6030085

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026176.D
Acq On : 12 Jun 2022 21:31
Operator : SY/MD
Sample : VV0612WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK369

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

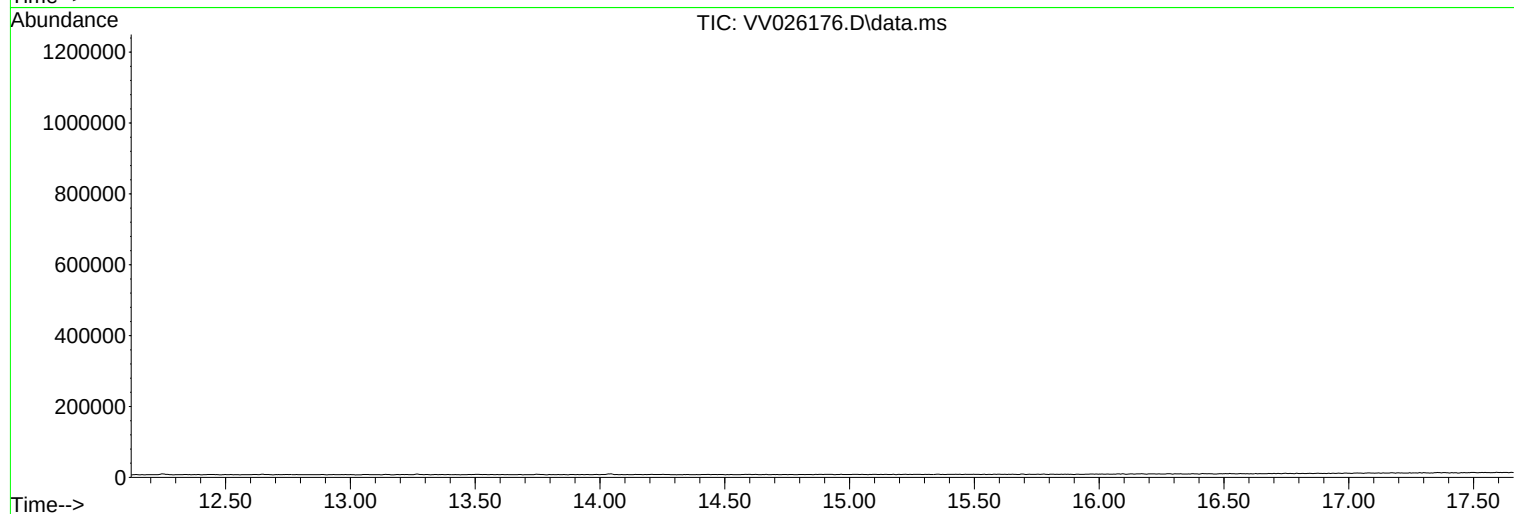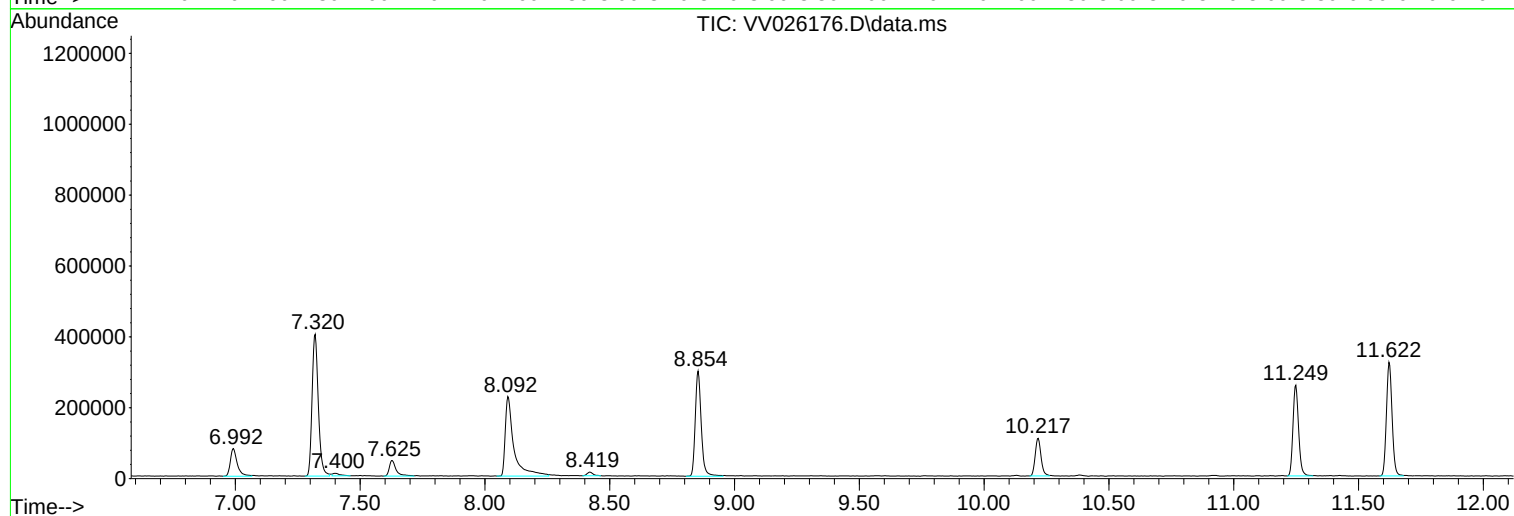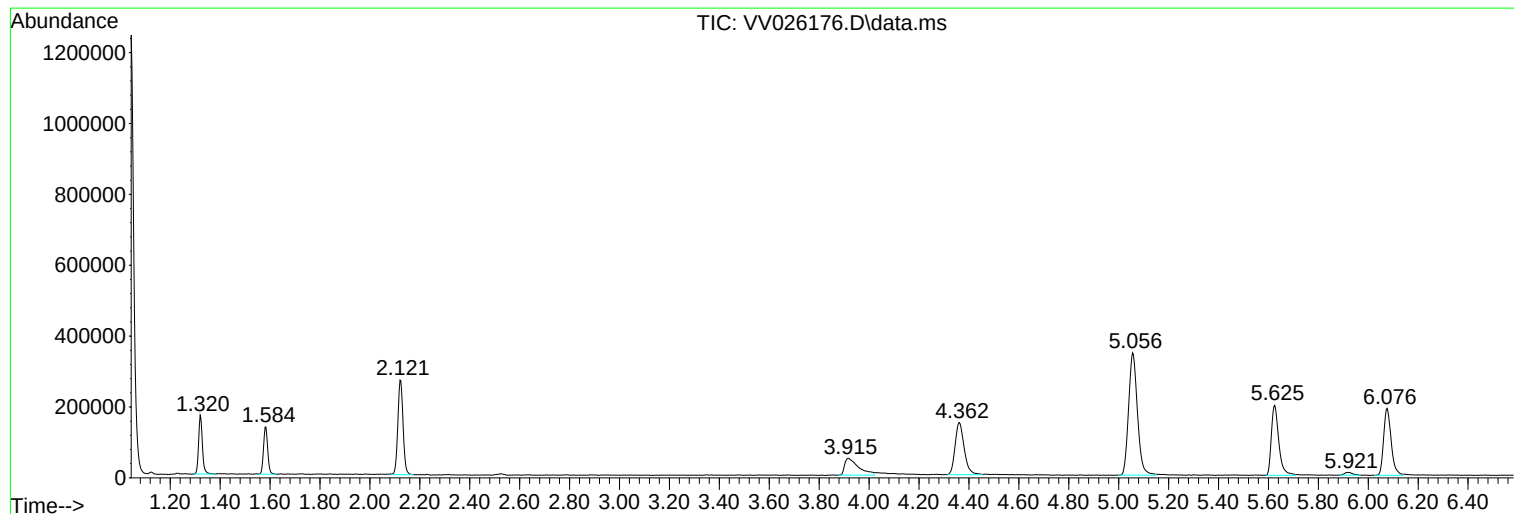

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026176.D
Acq On : 12 Jun 2022 21:31
Operator : SY/MD
Sample : VV0612WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK369

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026176.D
Acq On : 12 Jun 2022 21:31
Operator : SY/MD
Sample : VV0612WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK369

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
