

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
 Data File : VV026177.D
 Acq On : 12 Jun 2022 21:55
 Operator : SY/MD
 Sample : N3278-01 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	100	rVB	57652	61667	12.31%	1.376%
2	1.584	161	169	178	rBV	70682	80981	16.17%	1.807%
3	1.767	220	226	233	rVB3	9104	11928	2.38%	0.266%
4	2.124	326	337	354	rVB	115845	172365	34.41%	3.845%
5	3.918	883	895	927	rBV2	53542	198448	39.62%	4.427%
6	4.362	1018	1033	1055	rBV2	96756	240356	47.98%	5.362%
7	5.056	1234	1249	1273	rBV3	197212	500917	100.00%	11.175%
8	5.625	1413	1426	1457	rBV	196772	407361	81.32%	9.088%
9	5.921	1506	1518	1539	rBV3	80974	173169	34.57%	3.863%
10	6.076	1552	1566	1590	rBV	125553	260575	52.02%	5.813%
11	6.992	1842	1851	1872	rBV	38389	76650	15.30%	1.710%
12	7.320	1942	1953	1975	rBV	202628	358090	71.49%	7.989%
13	7.632	2039	2050	2068	rBV2	21384	42320	8.45%	0.944%
14	7.979	2147	2158	2178	rBV	79620	136535	27.26%	3.046%
15	8.092	2184	2193	2230	rBV2	188380	436282	87.10%	9.733%
16	8.854	2417	2430	2450	rBV	296147	495839	98.99%	11.062%
17	10.217	2843	2854	2874	rVB	77768	127586	25.47%	2.846%
18	11.249	3164	3175	3196	rBV	247089	389656	77.79%	8.693%
19	11.622	3280	3291	3308	rBV	195914	311772	62.24%	6.955%




Sum of corrected areas: 4482497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026177.D
Acq On : 12 Jun 2022 21:55
Operator : SY/MD
Sample : N3278-01 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

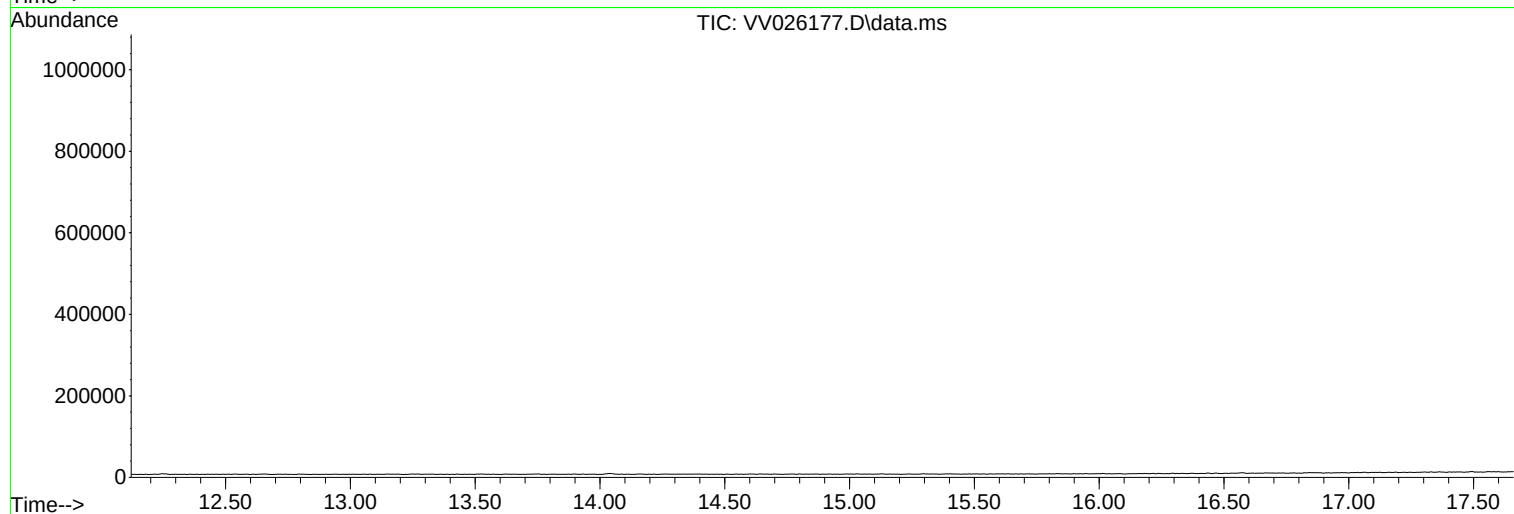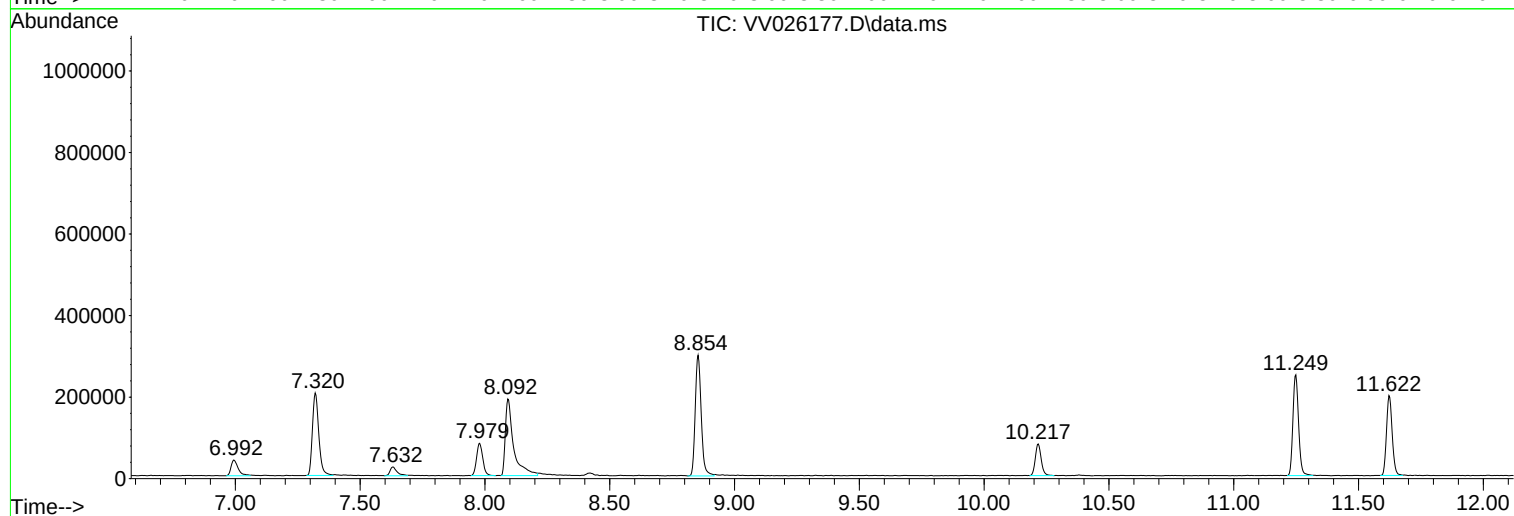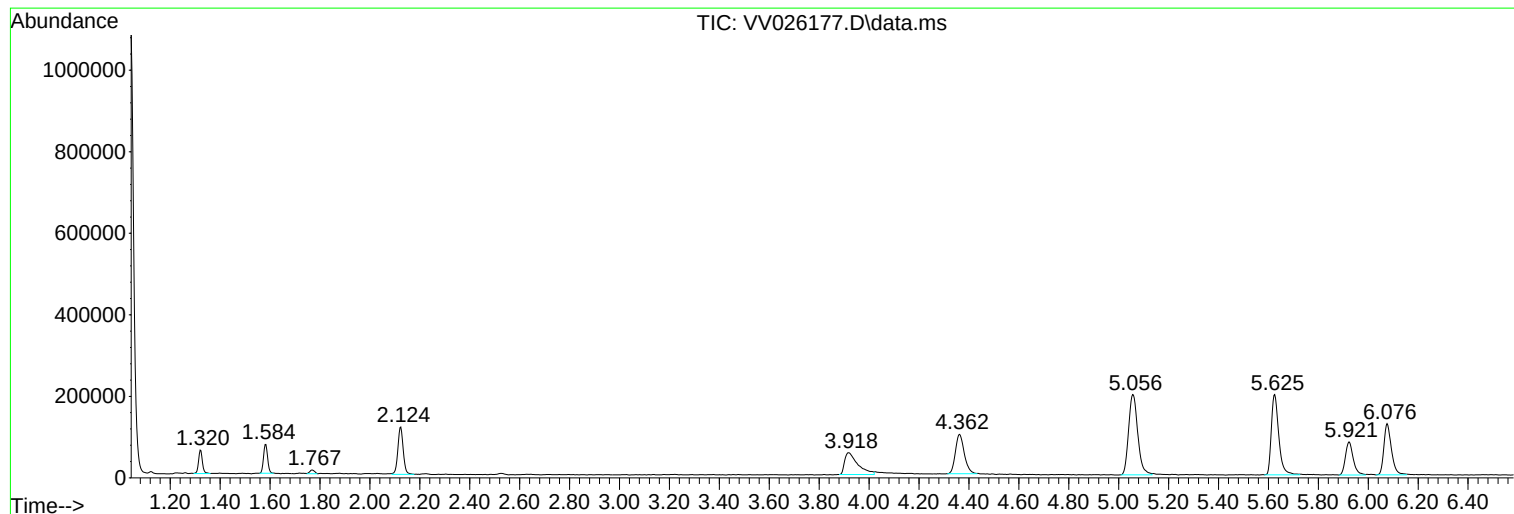

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026177.D
Acq On : 12 Jun 2022 21:55
Operator : SY/MD
Sample : N3278-01 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026177.D
Acq On : 12 Jun 2022 21:55
Operator : SY/MD
Sample : N3278-01 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc