

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
 Data File : VV026178.D
 Acq On : 12 Jun 2022 22:19
 Operator : SY/MD
 Sample : N3278-02 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	98	rVB	60212	67163	12.65%	1.490%
2	1.584	161	169	178	rVB	80693	88053	16.58%	1.953%
3	1.767	219	226	241	rBV3	8583	13390	2.52%	0.297%
4	2.124	326	337	350	rVB	124157	182182	34.31%	4.041%
5	3.921	877	896	924	rBV3	52660	200942	37.85%	4.457%
6	4.362	1017	1033	1059	rVB2	103133	261728	49.29%	5.806%
7	5.056	1233	1249	1275	rBV2	212211	530944	100.00%	11.777%
8	5.625	1413	1426	1453	rBV	203915	415635	78.28%	9.219%
9	5.921	1504	1518	1543	rVB10	9705	23118	4.35%	0.513%
10	6.076	1553	1566	1586	rBV	133031	274539	51.71%	6.090%
11	6.995	1842	1852	1869	rBV2	40521	78240	14.74%	1.735%
12	7.320	1941	1953	1971	rBV	211992	379071	71.40%	8.408%
13	7.629	2040	2049	2067	rBV3	21902	43822	8.25%	0.972%
14	7.979	2147	2158	2173	rBV	68516	116207	21.89%	2.578%
15	8.092	2183	2193	2243	rBV2	198887	473105	89.11%	10.494%
16	8.420	2284	2295	2304	rBV4	15166	27016	5.09%	0.599%
17	8.854	2416	2430	2457	rBV	295410	493100	92.87%	10.938%
18	10.217	2842	2854	2872	rBV	83527	135243	25.47%	3.000%
19	11.249	3164	3175	3194	rBV	244216	381556	71.86%	8.463%
20	11.622	3280	3291	3307	rBV	204446	323204	60.87%	7.169%




Sum of corrected areas: 4508258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026178.D
Acq On : 12 Jun 2022 22:19
Operator : SY/MD
Sample : N3278-02 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

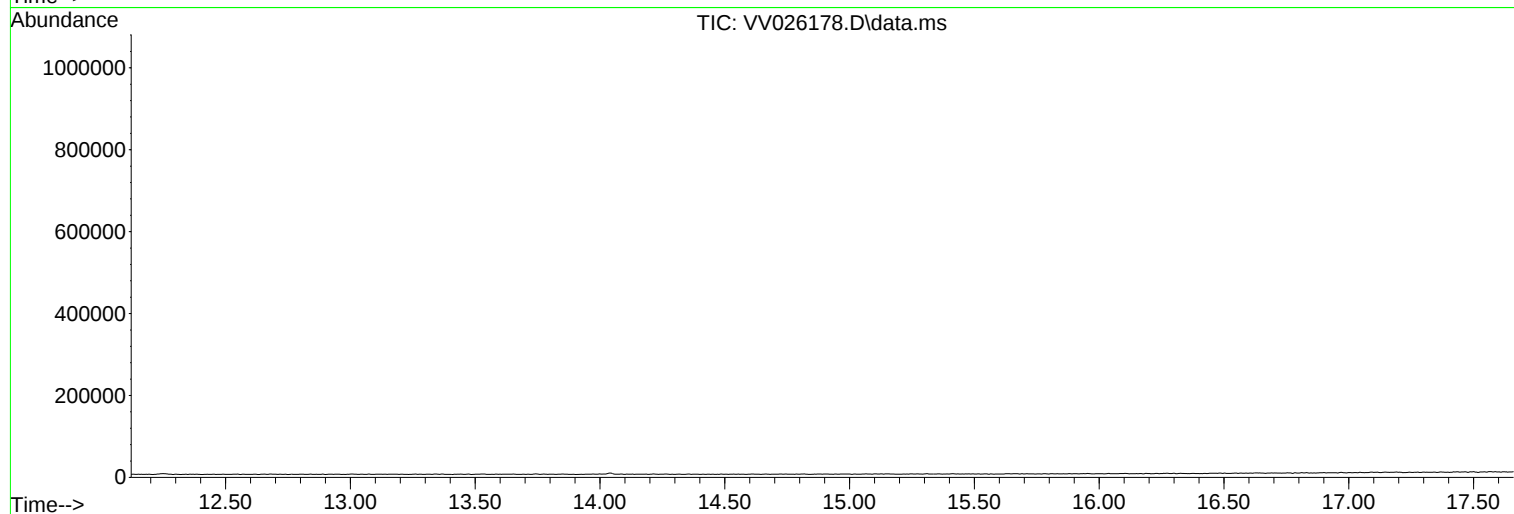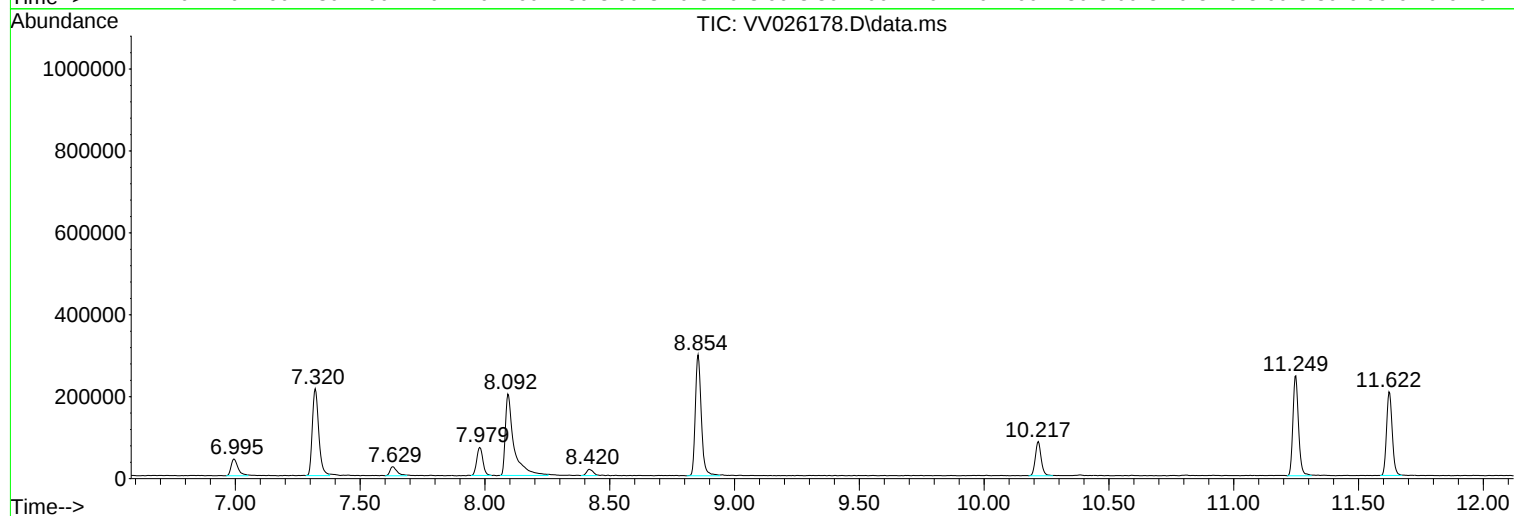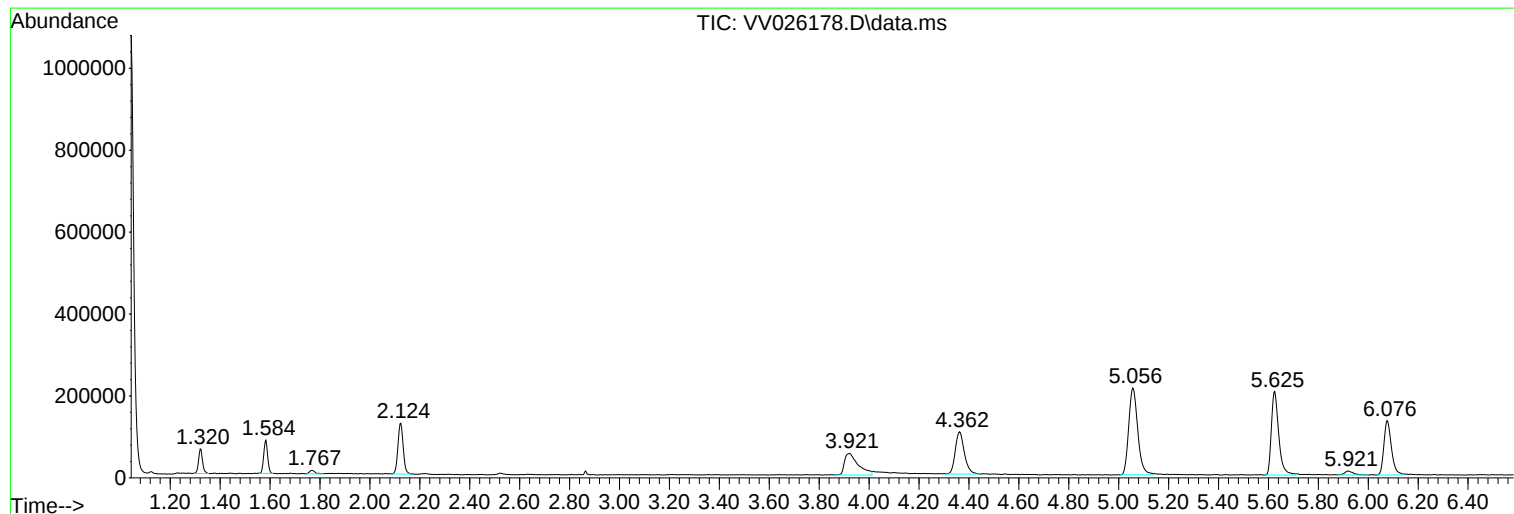

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026178.D
Acq On : 12 Jun 2022 22:19
Operator : SY/MD
Sample : N3278-02 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026178.D
Acq On : 12 Jun 2022 22:19
Operator : SY/MD
Sample : N3278-02 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc