

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
 Data File : VV026181.D
 Acq On : 12 Jun 2022 23:30
 Operator : SY/MD
 Sample : N3278-05 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	99	rVB	58906	62099	11.42%	1.358%
2	1.584	161	169	184	rVB	79400	91703	16.87%	2.006%
3	2.124	327	337	354	rVB	127309	185001	34.03%	4.046%
4	2.526	451	462	476	rVB4	5376	10002	1.84%	0.219%
5	3.918	876	895	929	rBV4	56393	218119	40.13%	4.770%
6	4.365	1018	1034	1059	rBV	102094	259588	47.76%	5.677%
7	5.060	1233	1250	1276	rBV2	210630	526589	96.88%	11.516%
8	5.625	1414	1426	1449	rBV	218893	445425	81.94%	9.741%
9	5.921	1508	1518	1533	rBV7	9415	19255	3.54%	0.421%
10	6.076	1551	1566	1595	rBV	130873	279847	51.48%	6.120%
11	6.992	1842	1851	1866	rBV2	39626	75860	13.96%	1.659%
12	7.320	1942	1953	1976	rBV	214319	375842	69.14%	8.220%
13	7.632	2041	2050	2064	rBV	22113	39041	7.18%	0.854%
14	7.979	2148	2158	2174	rVB	49911	86087	15.84%	1.883%
15	8.092	2184	2193	2238	rBV2	190868	449059	82.61%	9.821%
16	8.854	2419	2430	2446	rBV	336349	543566	100.00%	11.888%
17	10.217	2841	2854	2869	rBV	80760	133487	24.56%	2.919%
18	11.249	3163	3175	3194	rBV	281767	437595	80.50%	9.570%
19	11.622	3277	3291	3312	rBV	206338	334314	61.50%	7.311%




Sum of corrected areas: 4572479

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026181.D
Acq On : 12 Jun 2022 23:30
Operator : SY/MD
Sample : N3278-05 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

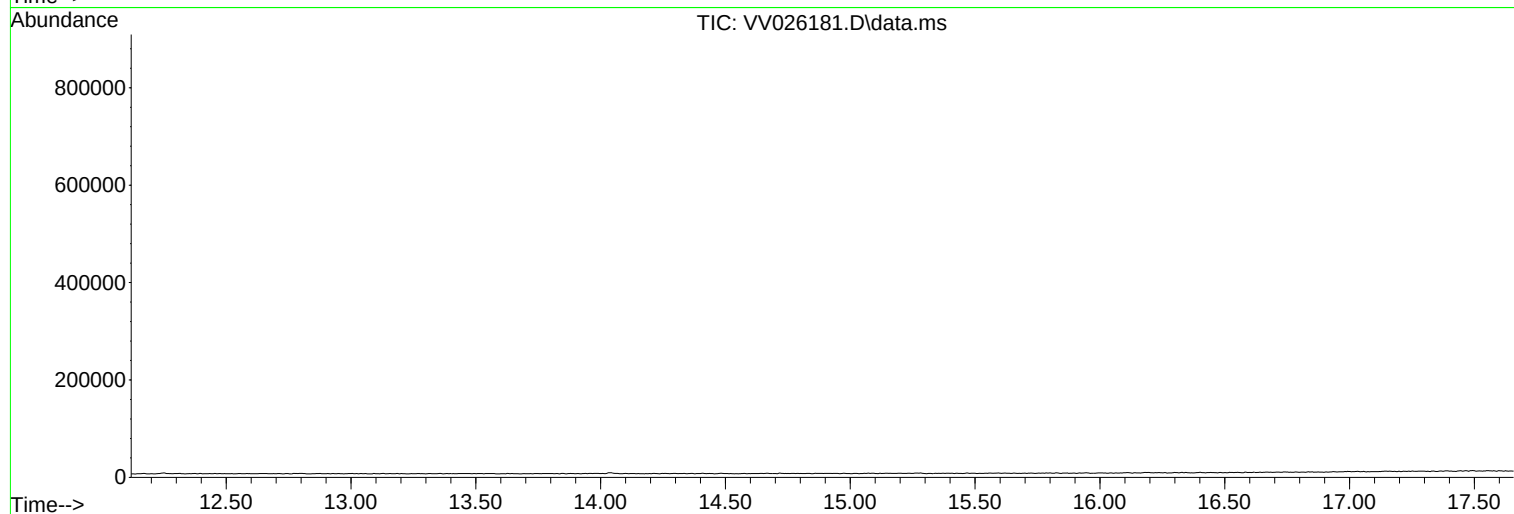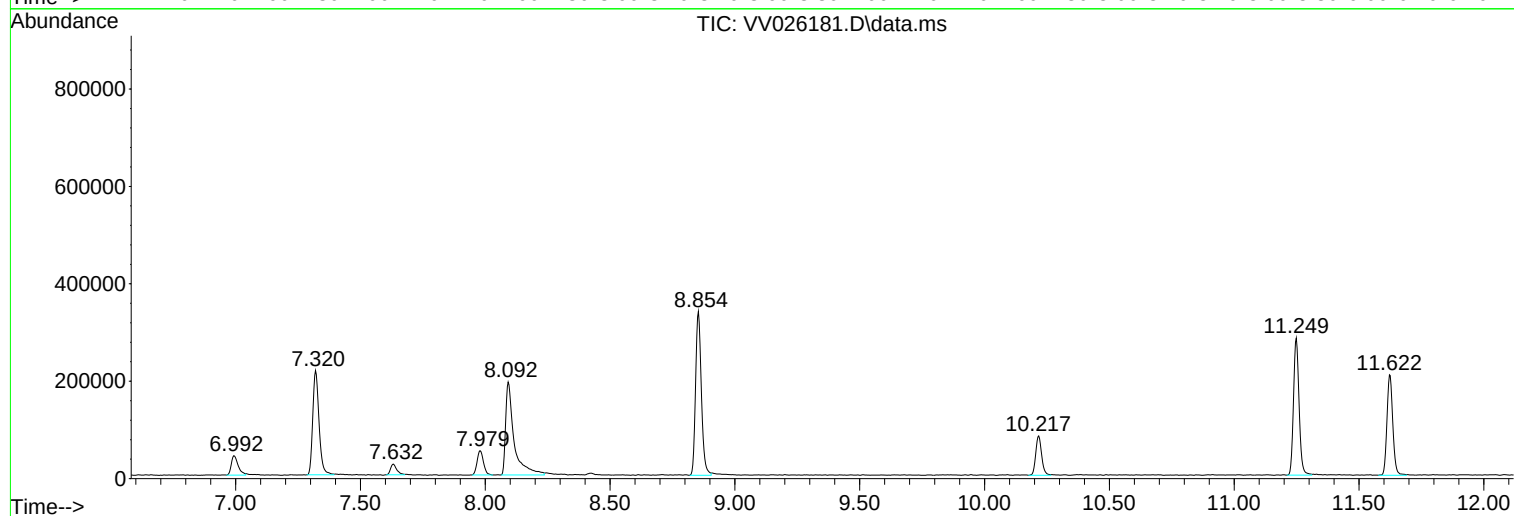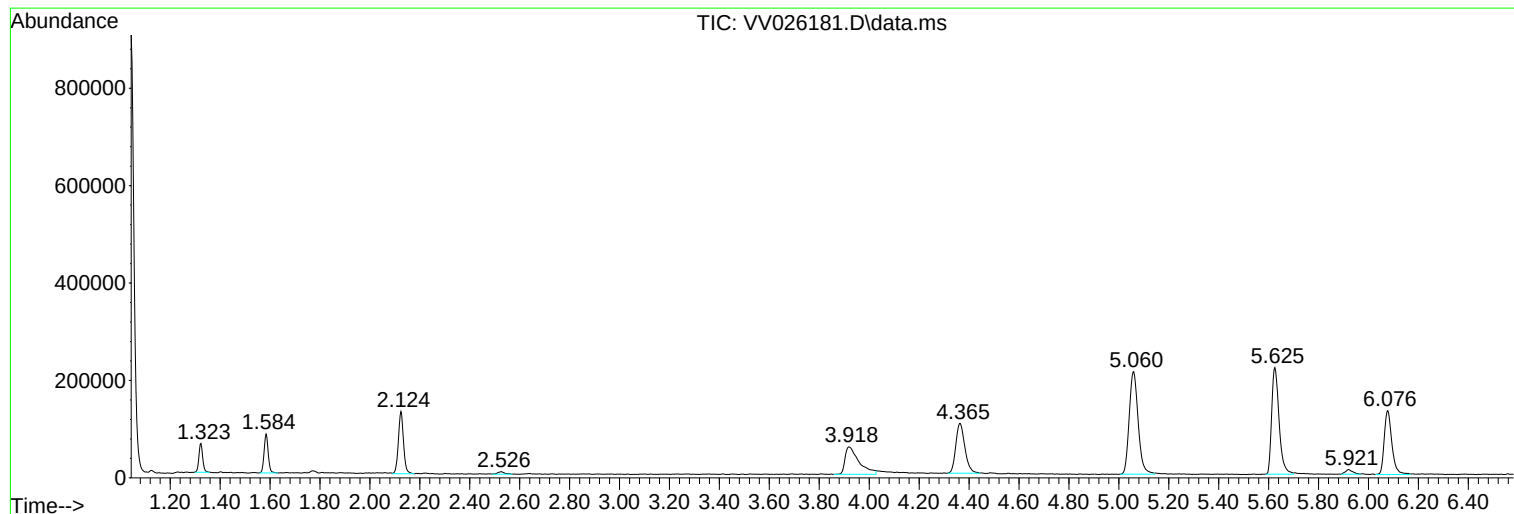

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026181.D
Acq On : 12 Jun 2022 23:30
Operator : SY/MD
Sample : N3278-05 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026181.D
Acq On : 12 Jun 2022 23:30
Operator : SY/MD
Sample : N3278-05 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
