

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
 Data File : VV026182.D
 Acq On : 12 Jun 2022 23:54
 Operator : SY/MD
 Sample : N3278-06 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	79	88	104	rVB	59284	65339	12.57%	1.452%
2	1.584	160	169	183	rVB	80986	90504	17.41%	2.011%
3	2.124	326	337	356	rVB	125375	184934	35.58%	4.110%
4	2.526	452	462	477	rVB4	6234	10768	2.07%	0.239%
5	3.918	879	895	932	rBV3	55901	218618	42.06%	4.858%
6	4.362	1018	1033	1057	rBV	99473	248685	47.84%	5.527%
7	5.056	1234	1249	1280	rBV2	206964	517685	99.60%	11.505%
8	5.625	1415	1426	1449	rBV	206709	428541	82.45%	9.524%
9	5.921	1507	1518	1531	rBV9	8364	17697	3.40%	0.393%
10	6.075	1554	1566	1589	rBV	128805	269000	51.75%	5.978%
11	6.995	1840	1852	1868	rBV2	39691	76551	14.73%	1.701%
12	7.320	1942	1953	1979	rBV	211920	380104	73.13%	8.447%
13	7.628	2037	2049	2067	rBV	21654	40874	7.86%	0.908%
14	7.979	2147	2158	2179	rVB	58262	100396	19.31%	2.231%
15	8.091	2183	2193	2240	rBV2	190252	461071	88.70%	10.247%
16	8.854	2419	2430	2453	rBV	315523	519783	100.00%	11.551%
17	10.217	2842	2854	2871	rBV	78593	129816	24.98%	2.885%
18	11.249	3163	3175	3194	rBV	264396	416692	80.17%	9.260%
19	11.622	3276	3291	3306	rBV	200547	322651	62.07%	7.170%




Sum of corrected areas: 4499709

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026182.D
Acq On : 12 Jun 2022 23:54
Operator : SY/MD
Sample : N3278-06 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

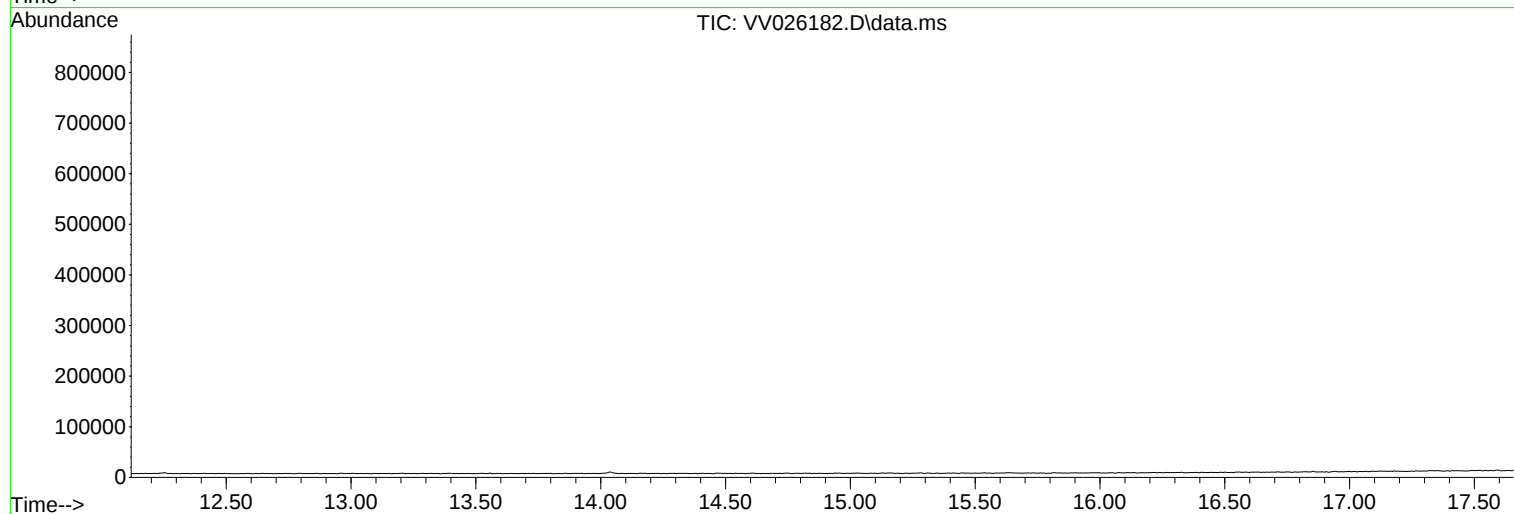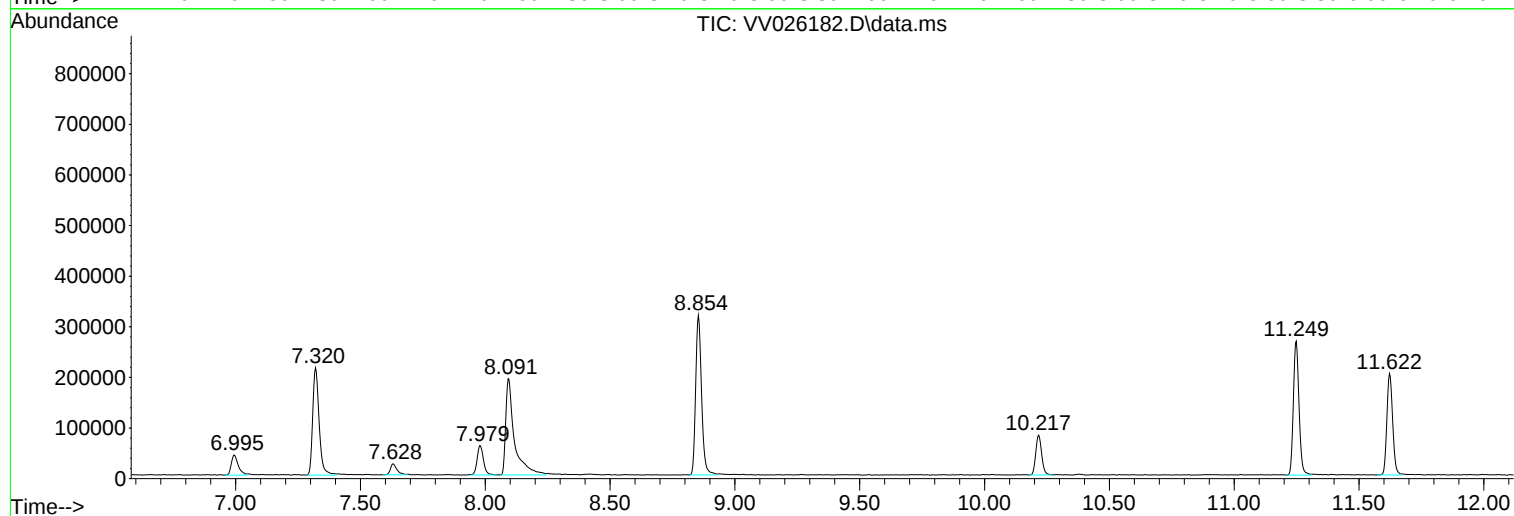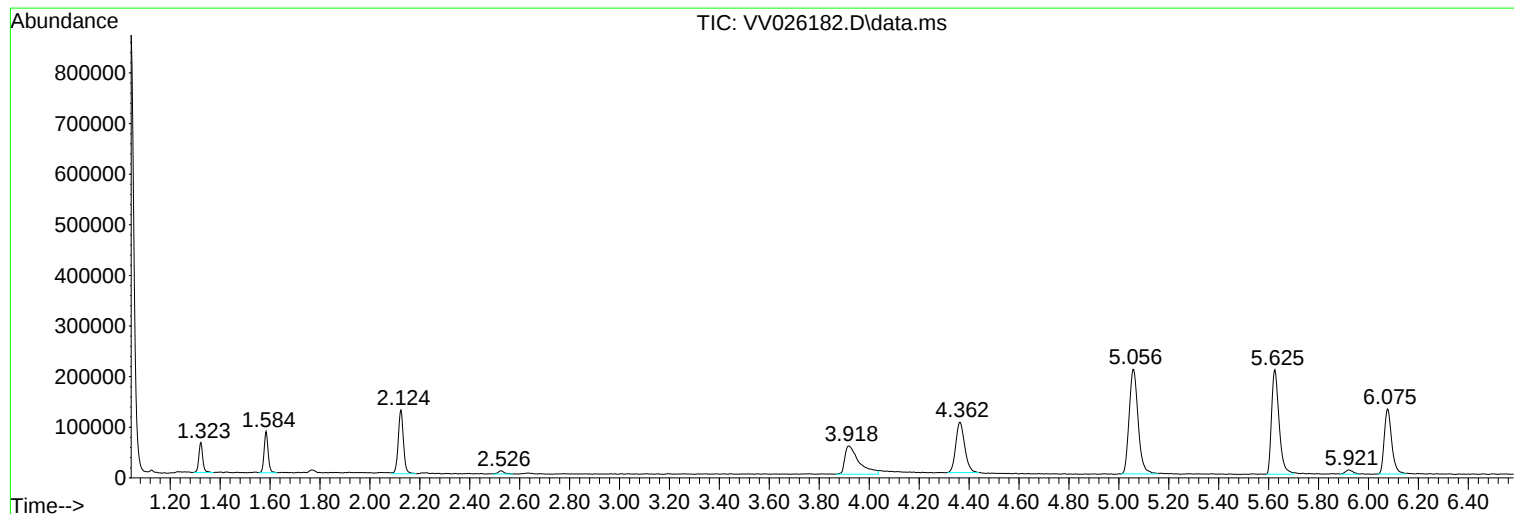

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026182.D
Acq On : 12 Jun 2022 23:54
Operator : SY/MD
Sample : N3278-06 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026182.D
Acq On : 12 Jun 2022 23:54
Operator : SY/MD
Sample : N3278-06 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
