

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
 Data File : VV026195.D
 Acq On : 13 Jun 2022 05:03
 Operator : SY/MD
 Sample : N3278-19 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	23	27	40	rVB3	7416	9625	1.90%	0.228%
2	1.326	81	89	101	rVB	59289	63834	12.60%	1.512%
3	1.587	162	170	184	rVB	74431	85693	16.92%	2.030%
4	2.127	327	338	352	rVB	121629	175796	34.70%	4.165%
5	2.526	453	462	477	rBV4	10226	17958	3.54%	0.425%
6	3.928	880	898	926	rBV4	78617	263200	51.95%	6.236%
7	4.365	1019	1034	1056	rVB2	95895	242365	47.84%	5.742%
8	5.059	1235	1250	1274	rBV3	193609	488114	96.35%	11.564%
9	5.625	1414	1426	1449	rBV	204073	414069	81.74%	9.810%
10	5.924	1507	1519	1535	rBV5	25261	55674	10.99%	1.319%
11	6.079	1553	1567	1589	rBV	120779	252530	49.85%	5.983%
12	6.995	1840	1852	1870	rBV2	35231	67558	13.34%	1.601%
13	7.320	1941	1953	1973	rBV	194356	347148	68.53%	8.224%
14	7.628	2041	2049	2064	rBV3	18386	35054	6.92%	0.830%
15	8.095	2184	2194	2238	rBV2	143817	376726	74.36%	8.925%
16	8.853	2418	2430	2451	rBV	309033	506596	100.00%	12.002%
17	10.217	2843	2854	2875	rVB	70686	116685	23.03%	2.764%
18	11.249	3160	3175	3194	rBV	253025	395888	78.15%	9.379%
19	11.622	3280	3291	3312	rBV	178619	288498	56.95%	6.835%
20	15.924	4616	4629	4630	rBV8	10752	17946	3.54%	0.425%




Sum of corrected areas: 4220957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026195.D
Acq On : 13 Jun 2022 05:03
Operator : SY/MD
Sample : N3278-19 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

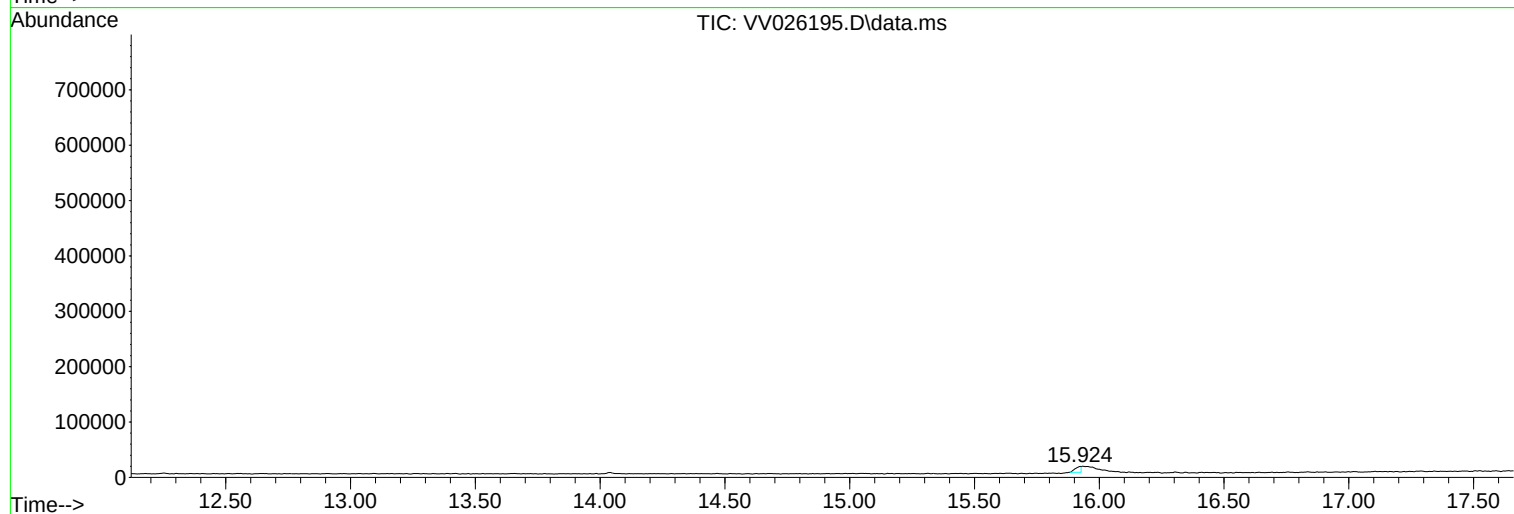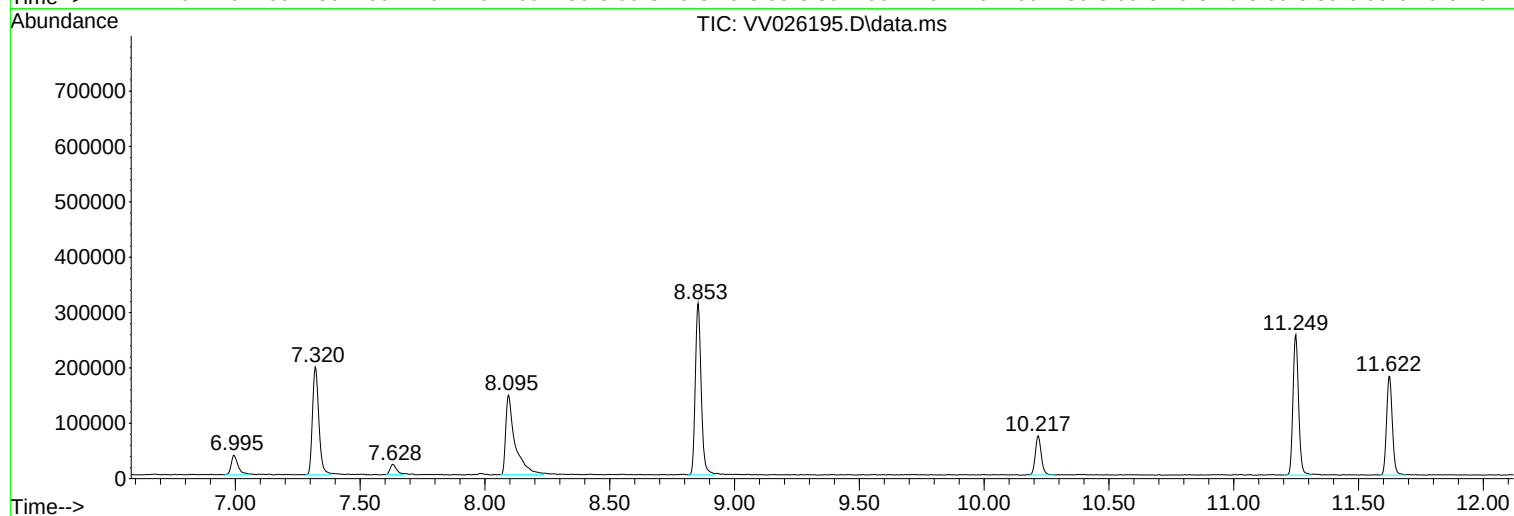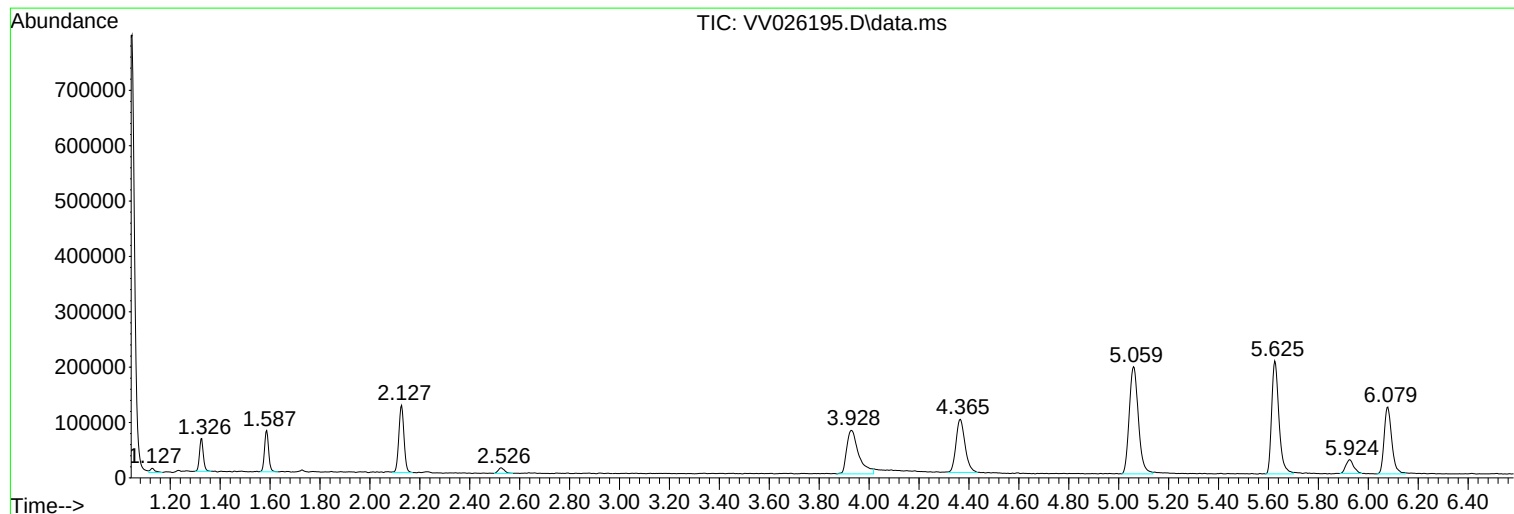

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026195.D
Acq On : 13 Jun 2022 05:03
Operator : SY/MD
Sample : N3278-19 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026195.D
Acq On : 13 Jun 2022 05:03
Operator : SY/MD
Sample : N3278-19 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc