

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
 Data File : VV026196.D
 Acq On : 13 Jun 2022 05:27
 Operator : SY/MD
 Sample : N3278-20 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BG1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	80	88	101	rVB	59820	64141	12.61%	1.488%
2	1.584	162	169	182	rVB	74953	86724	17.06%	2.012%
3	2.124	328	337	355	rVB	121405	177648	34.94%	4.121%
4	2.526	452	462	471	rBV2	11566	18923	3.72%	0.439%
5	3.921	880	896	922	rBV3	41016	156095	30.70%	3.621%
6	4.365	1017	1034	1056	rBV2	96728	241755	47.55%	5.609%
7	5.059	1234	1250	1280	rBV2	195754	489948	96.36%	11.367%
8	5.625	1412	1426	1453	rBV	204201	427267	84.03%	9.912%
9	5.921	1504	1518	1553	rBV2	112759	239512	47.11%	5.557%
10	6.079	1553	1567	1586	rBV2	120601	253994	49.95%	5.893%
11	6.992	1842	1851	1868	rBV2	33544	65235	12.83%	1.513%
12	7.320	1941	1953	1971	rBV	200390	350793	68.99%	8.138%
13	7.632	2041	2050	2067	rBV2	17653	35106	6.90%	0.814%
14	7.982	2150	2159	2172	rVB5	9272	16054	3.16%	0.372%
15	8.095	2184	2194	2239	rBV2	145365	376194	73.99%	8.728%
16	8.853	2419	2430	2447	rBV	306775	508459	100.00%	11.796%
17	10.217	2841	2854	2867	rBV	70822	114809	22.58%	2.664%
18	11.249	3161	3175	3199	rBV	253121	399821	78.63%	9.276%
19	11.622	3281	3291	3310	rBV	183994	287942	56.63%	6.680%




Sum of corrected areas: 4310420

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026196.D
Acq On : 13 Jun 2022 05:27
Operator : SY/MD
Sample : N3278-20 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

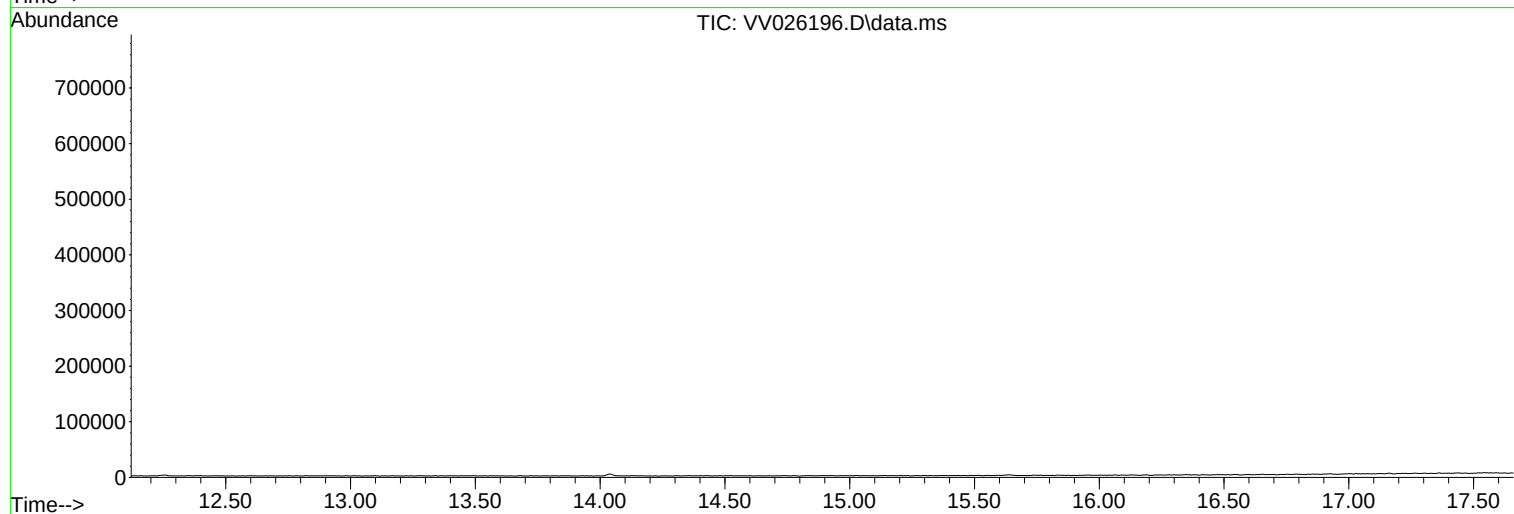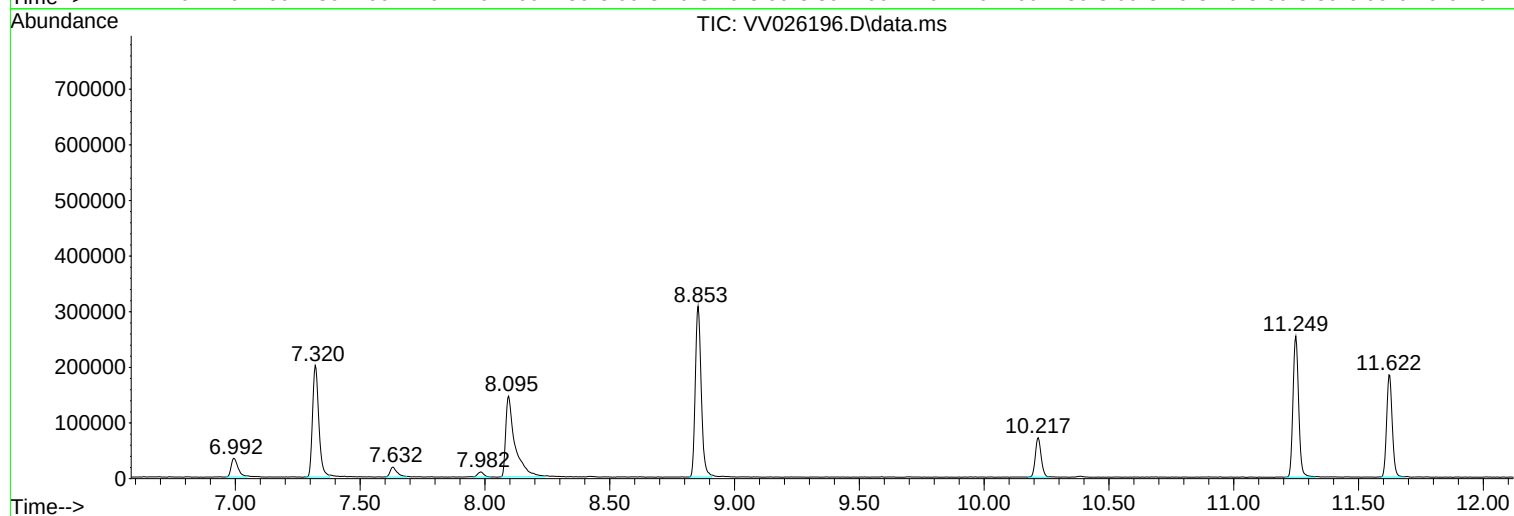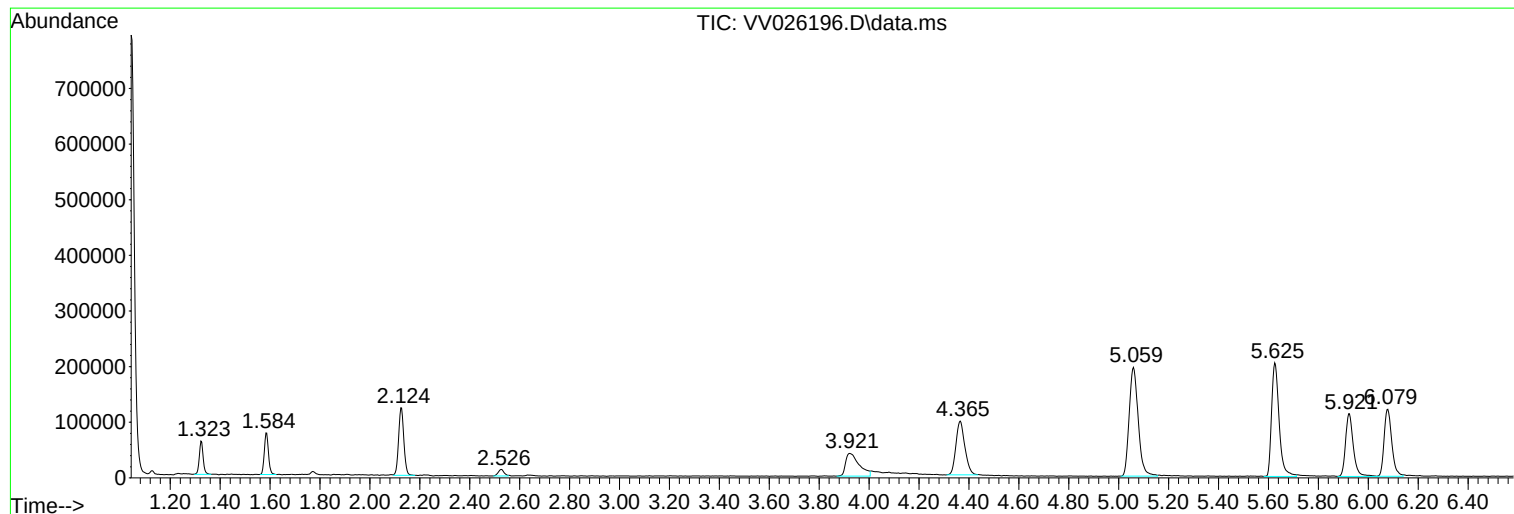

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026196.D
Acq On : 13 Jun 2022 05:27
Operator : SY/MD
Sample : N3278-20 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061222\
Data File : VV026196.D
Acq On : 13 Jun 2022 05:27
Operator : SY/MD
Sample : N3278-20 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BG1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
