

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
 Data File : VV031499.D
 Acq On : 12 Jun 2023 10:27
 Operator : SY/MD
 Sample : VV0612MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	93863	104537	10.90%	1.433%
2	1.532	146	153	163	rVB	98955	116501	12.15%	1.597%
3	2.060	307	317	332	rBV	196877	296031	30.87%	4.058%
4	2.452	432	439	447	rVB4	1804	3067	0.32%	0.042%
5	2.683	508	511	512	rBV	533	317	0.03%	0.004%
6	2.809	546	550	552	rBV2	511	283	0.03%	0.004%
7	2.899	575	578	580	rBV	372	167	0.02%	0.002%
8	2.957	592	596	599	rBV2	345	276	0.03%	0.004%
9	3.005	608	611	614	rBV2	345	214	0.02%	0.003%
10	3.028	615	618	621	rBV2	440	255	0.03%	0.003%
11	3.127	647	649	653	rVB2	330	169	0.02%	0.002%
12	3.211	673	675	679	rVB	343	161	0.02%	0.002%
13	3.230	679	681	683	rBV	471	245	0.03%	0.003%
14	3.262	688	691	693	rBV3	532	304	0.03%	0.004%
15	3.320	707	709	712	rVB2	338	168	0.02%	0.002%
16	3.349	712	718	720	rBV	292	236	0.02%	0.003%
17	3.362	720	722	725	rBV2	321	193	0.02%	0.003%
18	3.400	730	734	735	rBV	422	238	0.02%	0.003%
19	3.542	774	778	780	rBV	302	219	0.02%	0.003%
20	3.564	780	785	788	rVV3	202	210	0.02%	0.003%
21	3.683	819	822	826	rVB3	334	248	0.03%	0.003%
22	3.796	847	857	889	rBV2	84884	252688	26.35%	3.464%
23	4.256	984	1000	1028	rBV2	162500	424448	44.25%	5.818%
24	4.490	1070	1073	1077	rBV3	541	556	0.06%	0.008%
25	4.687	1131	1134	1137	rBV4	422	375	0.04%	0.005%
26	4.748	1150	1153	1154	rBV2	498	354	0.04%	0.005%
27	4.963	1203	1220	1245	rBV2	355647	959108	100.00%	13.147%
28	5.249	1308	1309	1314	rVB4	698	333	0.03%	0.005%
29	5.272	1314	1316	1318	rBV	377	174	0.02%	0.002%
30	5.330	1331	1334	1338	rVB2	1433	829	0.09%	0.011%
31	5.394	1348	1354	1355	rBV2	354	301	0.03%	0.004%
32	5.445	1364	1370	1375	rVB4	590	648	0.07%	0.009%
33	5.539	1387	1399	1422	rBV	267312	551519	57.50%	7.560%
34	5.831	1478	1490	1508	rBV2	35645	78068	8.14%	1.070%
35	5.937	1521	1523	1526	rVB2	531	232	0.02%	0.003%
36	5.995	1526	1541	1580	rBV	230824	493559	51.46%	6.765%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
 Data File : VV031499.D
 Acq On : 12 Jun 2023 10:27
 Operator : SY/MD
 Sample : VV0612MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.297	1632	1635	1637	rVV	555	295	0.03%	0.004%
38	6.317	1637	1641	1644	rVV2	383	295	0.03%	0.004%
39	6.352	1650	1652	1655	rVV	439	182	0.02%	0.002%
40	6.429	1673	1676	1681	rVB3	446	382	0.04%	0.005%
41	6.452	1681	1683	1687	rBV2	276	157	0.02%	0.002%
42	6.481	1687	1692	1695	rBV2	360	267	0.03%	0.004%
43	6.516	1702	1703	1707	rVB	379	183	0.02%	0.003%
44	6.539	1707	1710	1711	rBV	407	204	0.02%	0.003%
45	6.561	1711	1717	1719	rBV3	1412	1427	0.15%	0.020%
46	6.696	1757	1759	1762	rBV2	572	388	0.04%	0.005%
47	6.773	1781	1783	1786	rBV3	426	174	0.02%	0.002%
48	6.867	1809	1812	1814	rVB2	550	309	0.03%	0.004%
49	6.918	1814	1828	1852	rBV	100076	199000	20.75%	2.728%
50	7.249	1919	1931	1956	rBV	365323	661255	68.94%	9.064%
51	7.523	2013	2016	2017	rBV2	329	157	0.02%	0.002%
52	7.558	2017	2027	2047	rBV2	75561	142227	14.83%	1.950%
53	7.831	2110	2112	2114	rVB2	598	237	0.02%	0.003%
54	7.912	2135	2137	2140	rBV3	763	428	0.04%	0.006%
55	8.034	2165	2175	2216	rBV2	217441	502795	52.42%	6.892%
56	8.423	2294	2296	2297	rBV2	707	320	0.03%	0.004%
57	8.645	2363	2365	2367	rVB	667	264	0.03%	0.004%
58	8.706	2382	2384	2390	rVB3	360	256	0.03%	0.004%
59	8.735	2390	2393	2395	rBV3	915	481	0.05%	0.007%
60	8.789	2399	2410	2446	rBV	417434	714234	74.47%	9.790%
61	9.085	2499	2502	2503	rBV2	729	382	0.04%	0.005%
62	9.172	2527	2529	2531	rVV2	290	170	0.02%	0.002%
63	9.217	2537	2543	2545	rBV3	570	531	0.06%	0.007%
64	9.265	2556	2558	2561	rVB2	555	266	0.03%	0.004%
65	9.288	2561	2565	2567	rBV2	365	245	0.03%	0.003%
66	9.323	2574	2576	2577	rBV	391	176	0.02%	0.002%
67	9.413	2602	2604	2607	rVB	464	232	0.02%	0.003%
68	9.471	2616	2622	2623	rBV2	483	322	0.03%	0.004%
69	9.493	2623	2629	2631	rBV3	881	867	0.09%	0.012%
70	9.616	2664	2667	2668	rBV2	423	313	0.03%	0.004%
71	9.654	2677	2679	2683	rBV2	374	238	0.02%	0.003%
72	9.699	2691	2693	2695	rBV3	383	184	0.02%	0.003%
73	9.735	2702	2704	2710	rVB	450	303	0.03%	0.004%
74	9.767	2710	2714	2715	rBV	414	311	0.03%	0.004%
75	9.873	2739	2747	2752	rBV3	918	1169	0.12%	0.016%
76	9.895	2752	2754	2758	rVB2	418	242	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
 Data File : VV031499.D
 Acq On : 12 Jun 2023 10:27
 Operator : SY/MD
 Sample : VV0612MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	9.928	2762	2764	2769	rBV	426	285	0.03%	0.004%
78	9.963	2773	2775	2777	rBV2	389	221	0.02%	0.003%
79	10.059	2803	2805	2809	rBV2	676	457	0.05%	0.006%
80	10.159	2823	2836	2853	rBV	271408	441172	46.00%	6.047%
81	10.339	2883	2892	2895	rBV4	1025	1629	0.17%	0.022%
82	10.429	2914	2920	2922	rBV2	369	402	0.04%	0.006%
83	10.474	2931	2934	2935	rBV2	583	257	0.03%	0.004%
84	10.519	2945	2948	2950	rBV2	335	202	0.02%	0.003%
85	10.606	2971	2975	2977	rBV2	354	274	0.03%	0.004%
86	10.741	3015	3017	3024	rVB3	527	426	0.04%	0.006%
87	10.789	3030	3032	3036	rVB2	467	243	0.03%	0.003%
88	10.857	3049	3053	3055	rBV4	824	673	0.07%	0.009%
89	11.092	3123	3126	3128	rBV	380	202	0.02%	0.003%
90	11.191	3146	3157	3175	rBV	414491	654938	68.29%	8.977%
91	11.461	3240	3241	3243	rBV	447	160	0.02%	0.002%
92	11.567	3262	3274	3291	rBV	417482	658643	68.67%	9.028%
93	11.683	3308	3310	3311	rBV2	675	230	0.02%	0.003%
94	12.091	3435	3437	3443	rVB3	634	435	0.05%	0.006%
95	12.596	3588	3594	3601	rBV6	1525	2287	0.24%	0.031%
96	12.683	3617	3621	3623	rBV3	828	507	0.05%	0.007%
97	12.712	3628	3630	3632	rBV2	486	261	0.03%	0.004%
98	13.204	3779	3783	3784	rBV4	2120	1304	0.14%	0.018%
99	13.448	3855	3859	3871	rVB2	5540	8367	0.87%	0.115%
100	13.689	3930	3934	3940	rVB4	2685	2755	0.29%	0.038%




Sum of corrected areas: 7295429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
Data File : VV031499.D
Acq On : 12 Jun 2023 10:27
Operator : SY/MD
Sample : VV0612MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

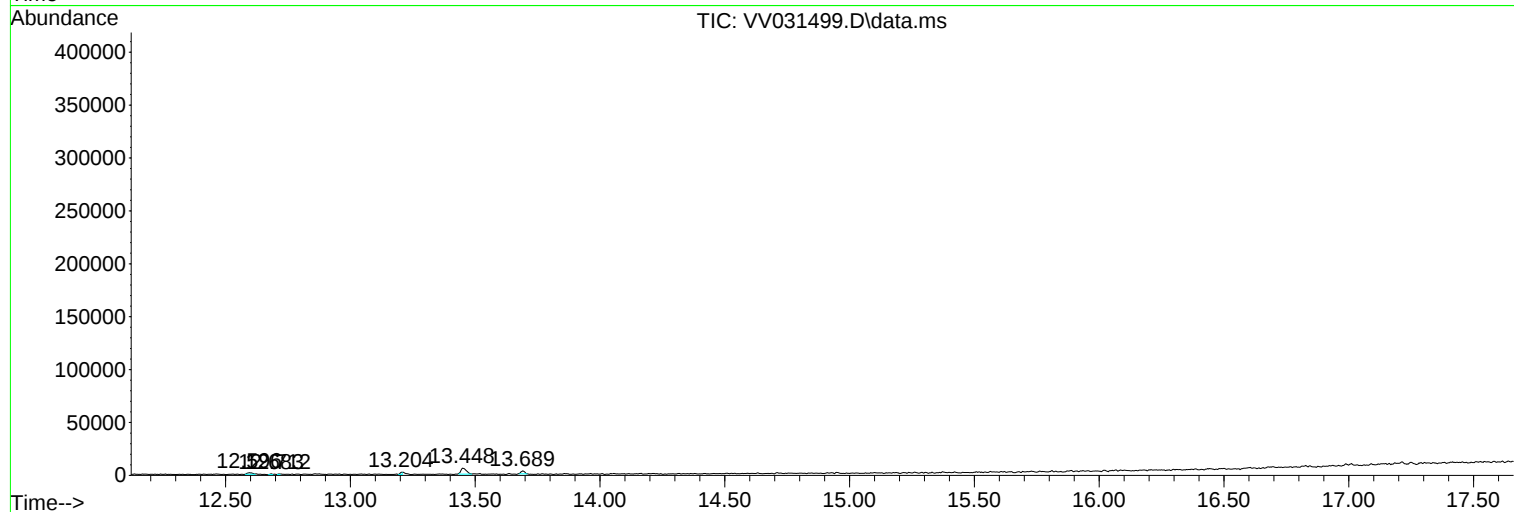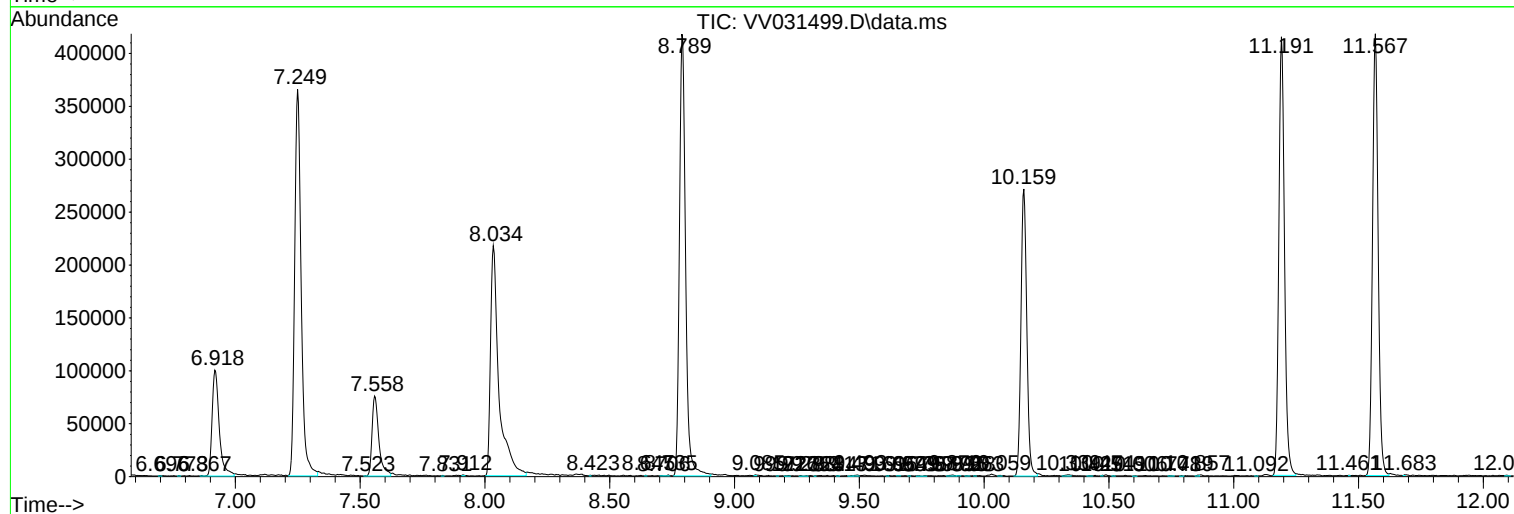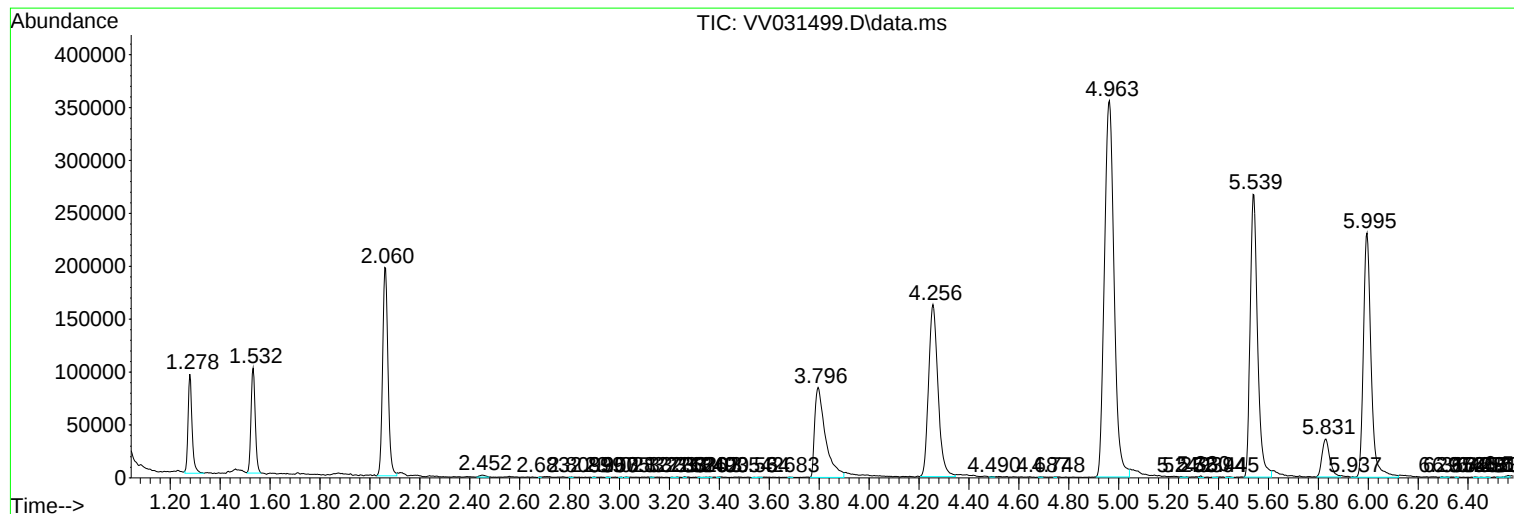

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
Data File : VV031499.D
Acq On : 12 Jun 2023 10:27
Operator : SY/MD
Sample : VV0612MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
Data File : VV031499.D
Acq On : 12 Jun 2023 10:27
Operator : SY/MD
Sample : VV0612MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc