

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
 Data File : VV031503.D
 Acq On : 12 Jun 2023 12:43
 Operator : SY/MD
 Sample : VIBLK217
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	85	rVB	85897	90576	9.55%	1.255%
2	1.532	147	153	165	rVB	95360	110523	11.66%	1.531%
3	2.059	308	317	332	rBV	177747	263037	27.74%	3.644%
4	2.449	431	438	449	rBV6	2756	4734	0.50%	0.066%
5	2.529	459	463	465	rBV2	611	489	0.05%	0.007%
6	2.629	489	494	497	rBV2	498	318	0.03%	0.004%
7	2.690	509	513	515	rBV4	848	718	0.08%	0.010%
8	2.773	535	539	542	rBV2	373	246	0.03%	0.003%
9	2.793	542	545	550	rVV2	362	308	0.03%	0.004%
10	2.834	556	558	561	rVB	403	207	0.02%	0.003%
11	2.857	561	565	568	rBV2	545	530	0.06%	0.007%
12	2.963	595	598	602	rVB3	451	210	0.02%	0.003%
13	3.011	610	613	617	rVB3	389	216	0.02%	0.003%
14	3.047	621	624	626	rBV2	374	236	0.02%	0.003%
15	3.104	640	642	643	rBV2	499	240	0.03%	0.003%
16	3.182	662	666	671	rVV2	444	455	0.05%	0.006%
17	3.297	699	702	705	rBV3	324	231	0.02%	0.003%
18	3.330	709	712	713	rBV	390	201	0.02%	0.003%
19	3.487	757	761	764	rVB2	305	229	0.02%	0.003%
20	3.661	812	815	818	rBV2	504	411	0.04%	0.006%
21	3.796	846	857	890	rBV2	93479	277580	29.27%	3.845%
22	4.256	983	1000	1024	rBV	156024	409103	43.14%	5.668%
23	4.648	1119	1122	1125	rVB3	357	225	0.02%	0.003%
24	4.712	1139	1142	1144	rBV	280	229	0.02%	0.003%
25	4.767	1154	1159	1160	rBV	321	260	0.03%	0.004%
26	4.796	1166	1168	1171	rBV2	313	198	0.02%	0.003%
27	4.860	1185	1188	1192	rVB3	459	339	0.04%	0.005%
28	4.889	1192	1197	1200	rVB2	390	337	0.04%	0.005%
29	4.963	1201	1220	1244	rBV2	353292	948224	100.00%	13.136%
30	5.317	1328	1330	1332	rVB2	611	234	0.02%	0.003%
31	5.436	1364	1367	1373	rVB3	482	400	0.04%	0.006%
32	5.464	1373	1376	1378	rBV3	354	267	0.03%	0.004%
33	5.542	1387	1400	1421	rBV	260256	541892	57.15%	7.507%
34	5.786	1474	1476	1479	rVB3	723	293	0.03%	0.004%
35	5.828	1479	1489	1507	rBV2	38811	83269	8.78%	1.154%
36	5.995	1525	1541	1570	rBV	230957	483926	51.03%	6.704%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
 Data File : VV031503.D
 Acq On : 12 Jun 2023 12:43
 Operator : SY/MD
 Sample : VIBLK217
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.246	1617	1619	1621	rBV	404	222	0.02%	0.003%
38	6.275	1621	1628	1630	rBV2	276	278	0.03%	0.004%
39	6.304	1635	1637	1640	rVB2	569	287	0.03%	0.004%
40	6.323	1640	1643	1647	rBV3	802	654	0.07%	0.009%
41	6.567	1711	1719	1721	rBV4	1559	1831	0.19%	0.025%
42	6.670	1749	1751	1754	rBV	424	265	0.03%	0.004%
43	6.702	1758	1761	1764	rVB3	619	333	0.04%	0.005%
44	6.770	1780	1782	1788	rBV5	834	646	0.07%	0.009%
45	6.828	1797	1800	1803	rVB4	513	367	0.04%	0.005%
46	6.866	1808	1812	1813	rBV3	383	251	0.03%	0.003%
47	6.918	1817	1828	1852	rBV	103212	201359	21.24%	2.790%
48	7.079	1875	1878	1880	rBV3	636	409	0.04%	0.006%
49	7.249	1919	1931	1964	rBV	357785	649197	68.46%	8.994%
50	7.558	2015	2027	2052	rBV	78680	147459	15.55%	2.043%
51	7.792	2096	2100	2104	rBV2	588	463	0.05%	0.006%
52	7.837	2112	2114	2116	rBV2	363	238	0.03%	0.003%
53	8.034	2164	2175	2211	rBV2	227881	511832	53.98%	7.091%
54	8.513	2322	2324	2326	rBV2	690	287	0.03%	0.004%
55	8.529	2326	2329	2331	rVV	548	330	0.03%	0.005%
56	8.564	2337	2340	2342	rBV2	518	374	0.04%	0.005%
57	8.638	2360	2363	2366	rBV2	586	394	0.04%	0.005%
58	8.789	2398	2410	2440	rBV	407999	696058	73.41%	9.643%
59	9.178	2528	2531	2537	rVB3	473	351	0.04%	0.005%
60	9.210	2537	2541	2543	rBV3	509	428	0.05%	0.006%
61	9.458	2614	2618	2623	rBV2	316	256	0.03%	0.004%
62	9.496	2623	2630	2635	rVV3	581	810	0.09%	0.011%
63	9.522	2635	2638	2641	rVV2	483	276	0.03%	0.004%
64	9.670	2679	2684	2685	rBV3	433	338	0.04%	0.005%
65	9.818	2725	2730	2734	rBV4	411	398	0.04%	0.006%
66	9.866	2740	2745	2746	rBV2	437	276	0.03%	0.004%
67	9.889	2747	2752	2757	rVB4	873	913	0.10%	0.013%
68	9.914	2757	2760	2762	rBV	397	233	0.02%	0.003%
69	9.943	2765	2769	2772	rBV4	487	481	0.05%	0.007%
70	10.050	2800	2802	2806	rVB4	449	354	0.04%	0.005%
71	10.159	2824	2836	2855	rBV	274869	440159	46.42%	6.098%
72	10.281	2871	2874	2876	rBV2	729	424	0.04%	0.006%
73	10.490	2935	2939	2945	rVB3	570	690	0.07%	0.010%
74	10.532	2950	2952	2958	rBV3	301	222	0.02%	0.003%
75	10.625	2977	2981	2986	rBV4	398	426	0.04%	0.006%
76	10.702	3003	3005	3012	rVB	702	622	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
 Data File : VV031503.D
 Acq On : 12 Jun 2023 12:43
 Operator : SY/MD
 Sample : VIBLK217
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.744	3013	3018	3020	rBV3	472	295	0.03%	0.004%
78	10.767	3020	3025	3027	rBV3	580	468	0.05%	0.006%
79	10.818	3039	3041	3043	rBV2	514	293	0.03%	0.004%
80	10.866	3050	3056	3060	rBV5	795	1009	0.11%	0.014%
81	10.963	3081	3086	3087	rBV	767	471	0.05%	0.007%
82	11.004	3095	3099	3102	rBV3	300	256	0.03%	0.004%
83	11.024	3103	3105	3110	rBV3	307	218	0.02%	0.003%
84	11.078	3118	3122	3126	rBV2	331	326	0.03%	0.005%
85	11.101	3126	3129	3133	rBV2	363	273	0.03%	0.004%
86	11.191	3145	3157	3177	rBV	422658	657241	69.31%	9.105%
87	11.567	3260	3274	3296	rBV	425334	666645	70.30%	9.235%
88	11.831	3351	3356	3359	rBV3	615	547	0.06%	0.008%
89	12.204	3466	3472	3479	rBV7	1434	1946	0.21%	0.027%
90	12.313	3502	3506	3510	rBV4	990	808	0.09%	0.011%
91	12.484	3557	3559	3560	rBV3	508	197	0.02%	0.003%
92	12.789	3651	3654	3659	rBV4	473	473	0.05%	0.007%
93	12.856	3669	3675	3681	rBV6	919	1096	0.12%	0.015%
94	13.101	3748	3751	3753	rBV	944	580	0.06%	0.008%
95	13.191	3773	3779	3781	rBV4	745	768	0.08%	0.011%
96	13.207	3781	3784	3785	rBV2	712	382	0.04%	0.005%
97	13.303	3811	3814	3817	rBV3	694	472	0.05%	0.007%
98	13.654	3919	3923	3924	rBV3	817	642	0.07%	0.009%
99	13.680	3930	3931	3932	rBV	652	240	0.03%	0.003%
100	14.075	4051	4054	4057	rBV2	952	651	0.07%	0.009%




Sum of corrected areas: 7218379

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
Data File : VV031503.D
Acq On : 12 Jun 2023 12:43
Operator : SY/MD
Sample : VIBLK217
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

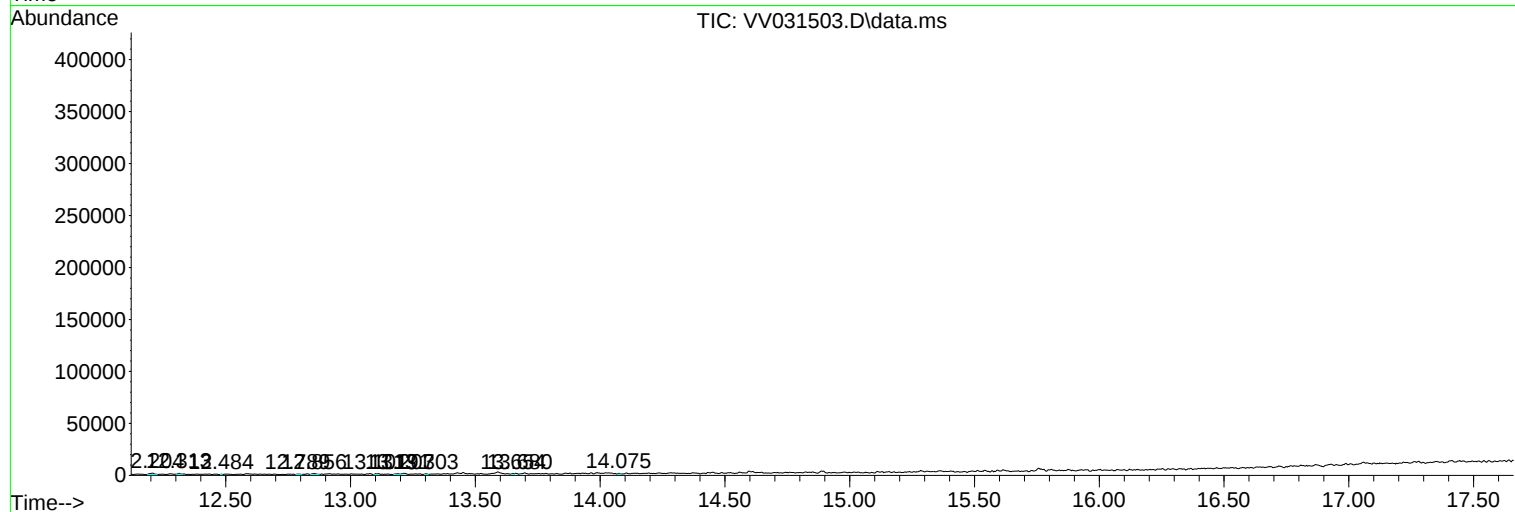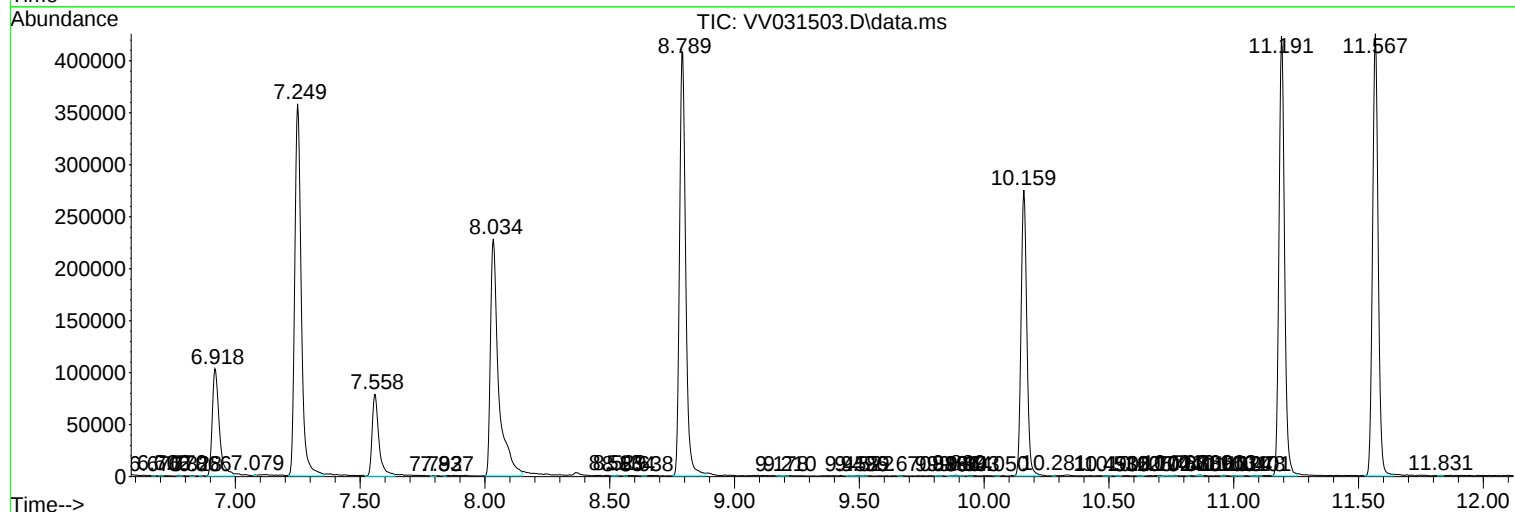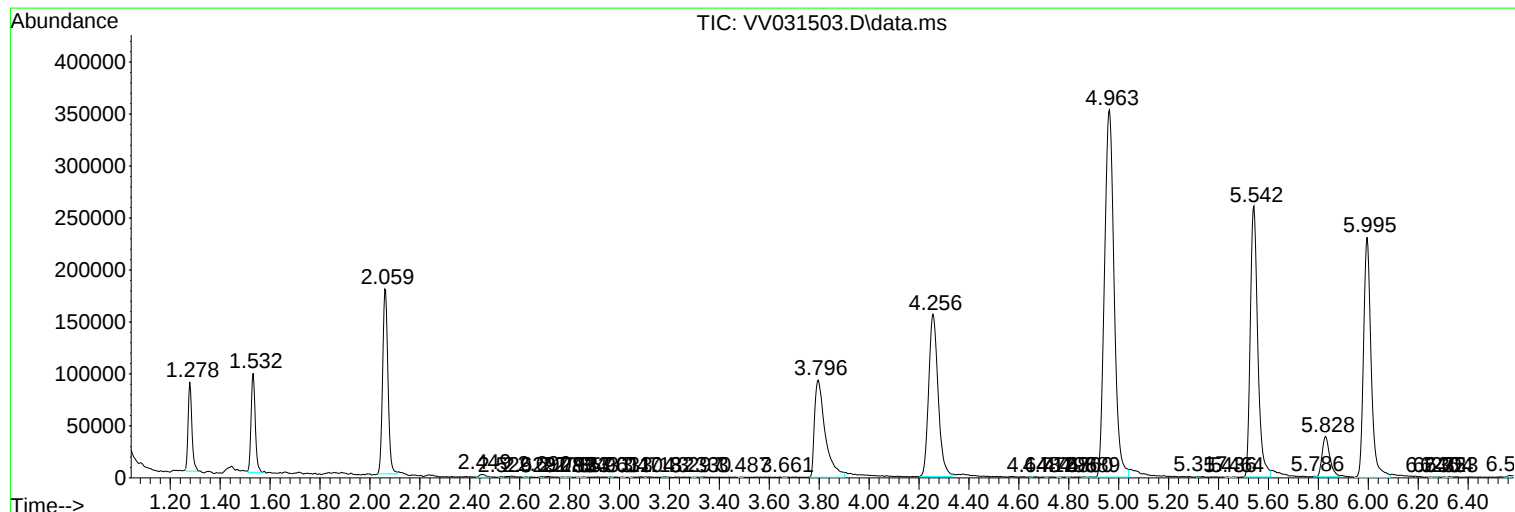

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
Data File : VV031503.D
Acq On : 12 Jun 2023 12:43
Operator : SY/MD
Sample : VIBLK217
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061223\
Data File : VV031503.D
Acq On : 12 Jun 2023 12:43
Operator : SY/MD
Sample : VIBLK217
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------