

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061225\
 Data File : VV038792.D
 Acq On : 12 Jun 2025 16:16
 Operator : SY/MD
 Sample : Q2275-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 OW-08B-72.5-060925-SIM

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.227	52	58	65	rVB	9516	12644	1.23%	0.165%
2	1.288	69	77	91	rVB	139828	183936	17.85%	2.396%
3	1.539	148	155	172	rVB	115810	165343	16.05%	2.154%
4	2.066	305	319	332	rBV	232626	403088	39.12%	5.251%
5	2.246	365	375	386	rVB3	10224	18955	1.84%	0.247%
6	3.786	846	854	893	rBV2	104588	345487	33.53%	4.501%
7	4.249	983	998	1029	rBV	168743	487435	47.31%	6.350%
8	4.954	1201	1217	1254	rBV2	359716	1030263	100.00%	13.421%
9	5.532	1387	1397	1436	rBV2	210403	517251	50.21%	6.738%
10	5.986	1525	1538	1562	rBV	225841	518830	50.36%	6.759%
11	6.912	1817	1826	1848	rBV2	85941	191529	18.59%	2.495%
12	7.240	1917	1928	1954	rBV	347865	695104	67.47%	9.055%
13	7.555	2012	2026	2045	rBV	53054	118238	11.48%	1.540%
14	8.014	2160	2169	2197	rBV	406373	828696	80.44%	10.795%
15	8.777	2396	2406	2435	rBV	387968	689205	66.90%	8.978%
16	10.143	2821	2831	2847	rBV	168125	279240	27.10%	3.638%
17	10.317	2874	2885	2892	rBV2	9179	12821	1.24%	0.167%
18	11.175	3142	3152	3176	rBV	338317	559074	54.27%	7.283%
19	11.551	3253	3269	3292	rBV	350264	591490	57.41%	7.705%
20	12.185	3457	3466	3476	rBV	7713	13603	1.32%	0.177%
21	13.976	4011	4023	4029	rBV2	7757	14086	1.37%	0.183%




Sum of corrected areas: 7676318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061225\
Data File : VV038792.D
Acq On : 12 Jun 2025 16:16
Operator : SY/MD
Sample : Q2275-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-060925-SIM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

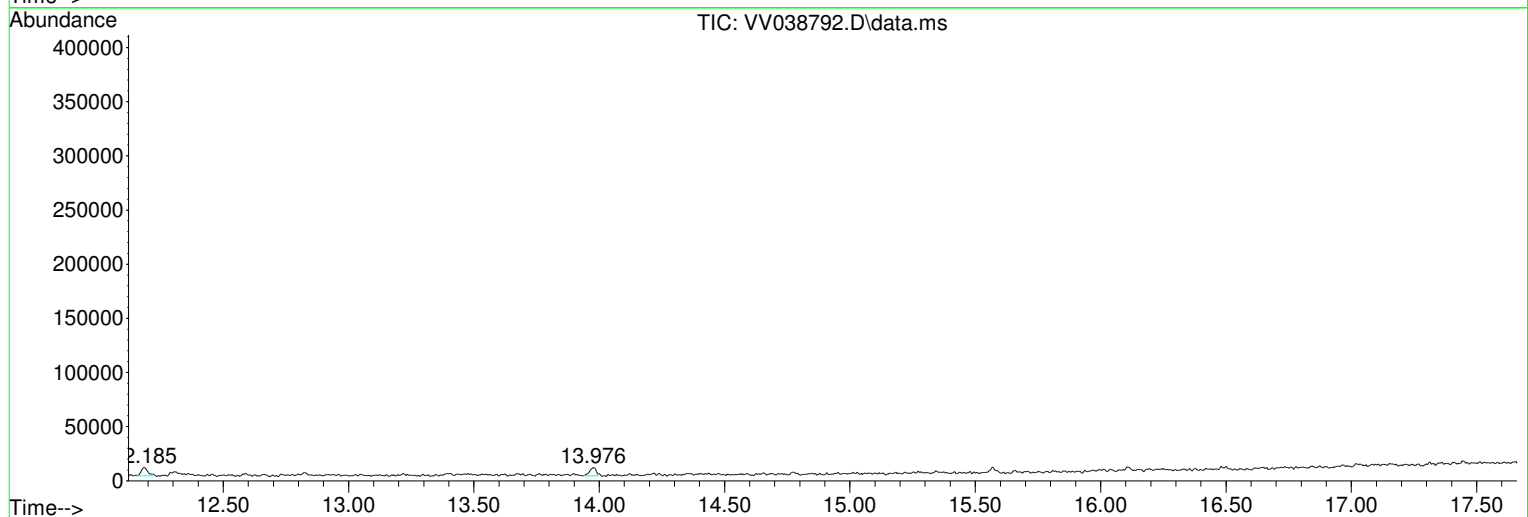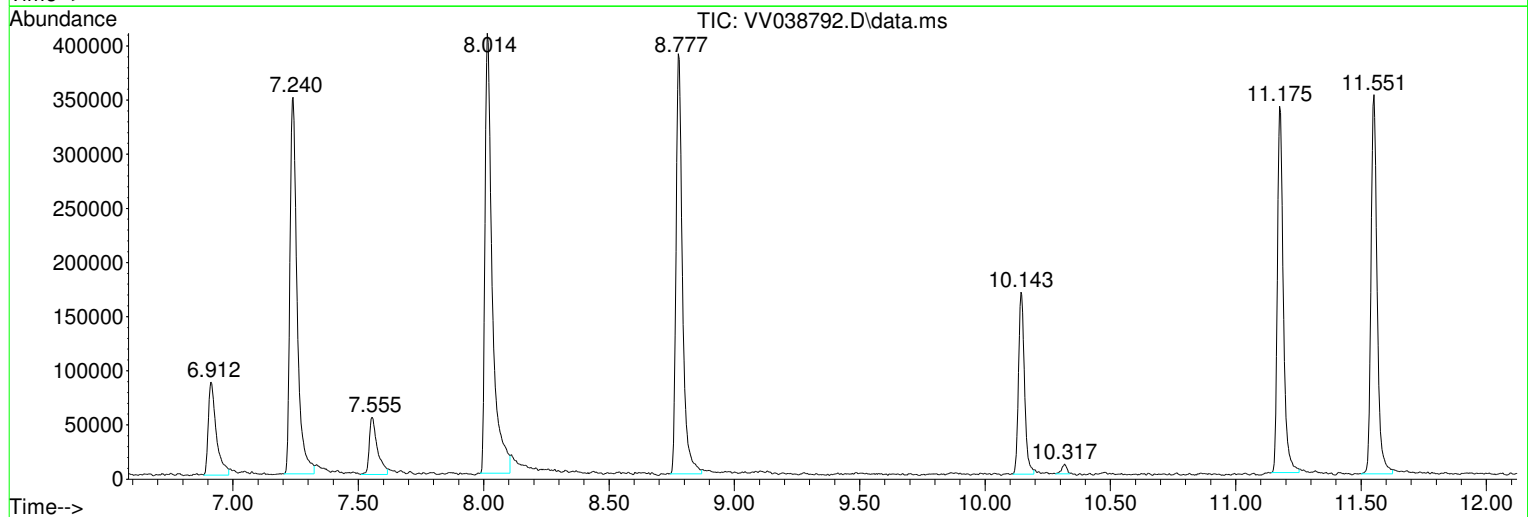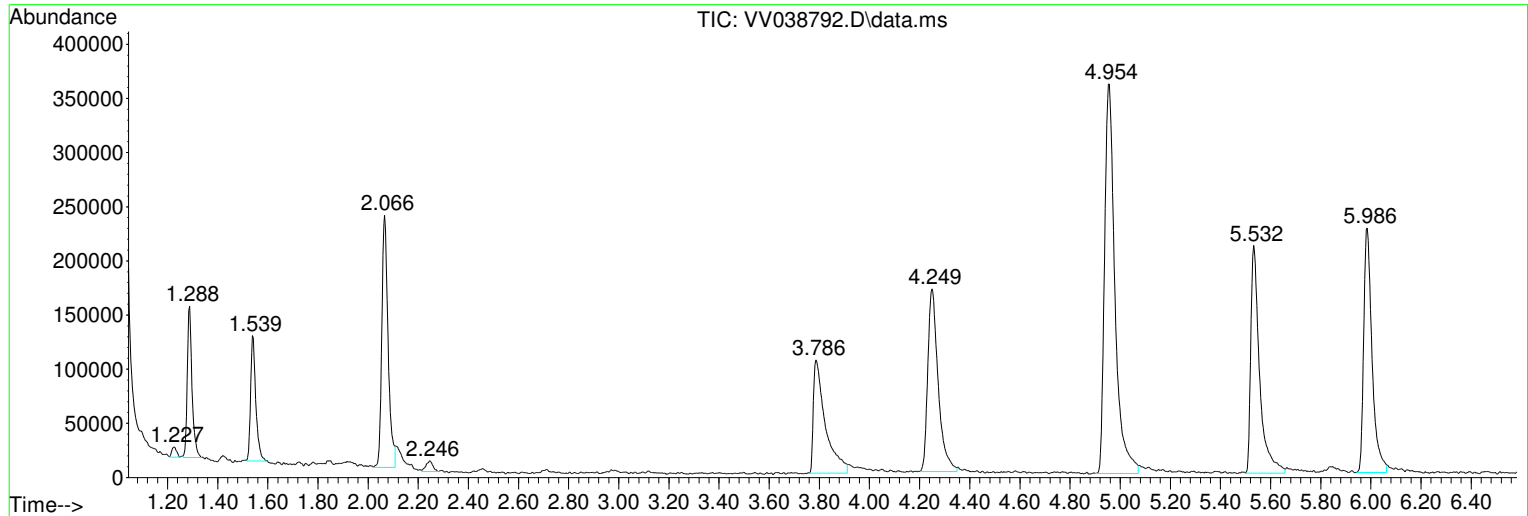

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061225\
Data File : VV038792.D
Acq On : 12 Jun 2025 16:16
Operator : SY/MD
Sample : Q2275-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-060925-SIM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061225\
Data File : VV038792.D
Acq On : 12 Jun 2025 16:16
Operator : SY/MD
Sample : Q2275-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
OW-08B-72.5-060925-SIM

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc