
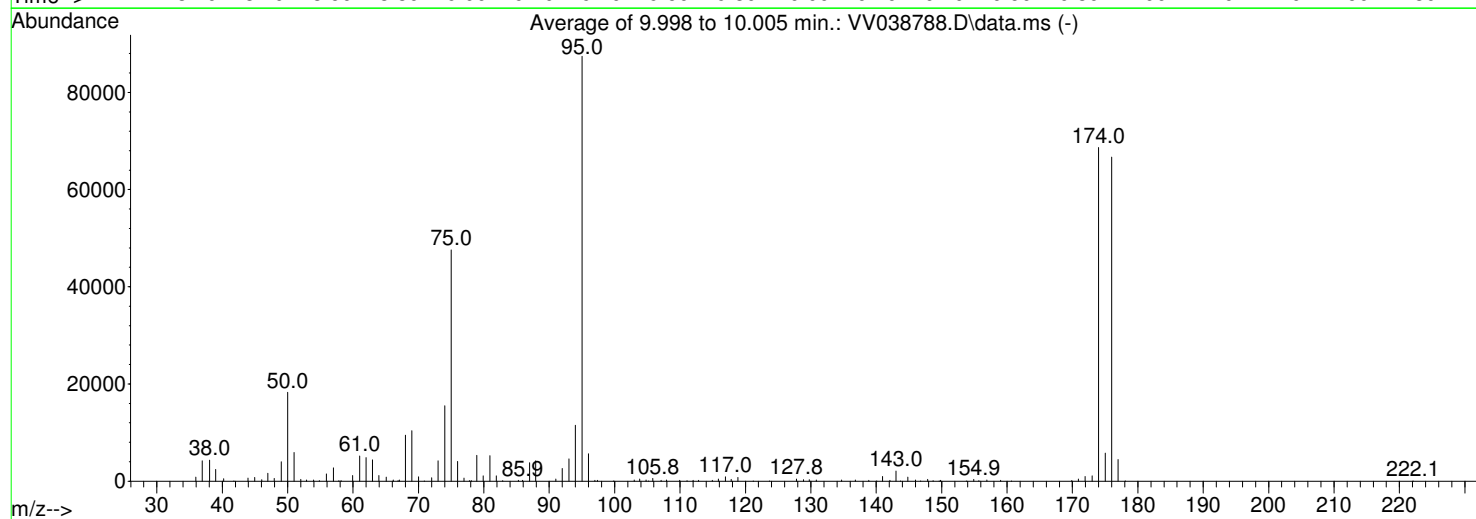


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV061225\
Data File : VV038788.D
Acq On : 12 Jun 2025 11:03
Operator : SY/MD
Sample : BFB209
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB209

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 13 10:50:34 2025

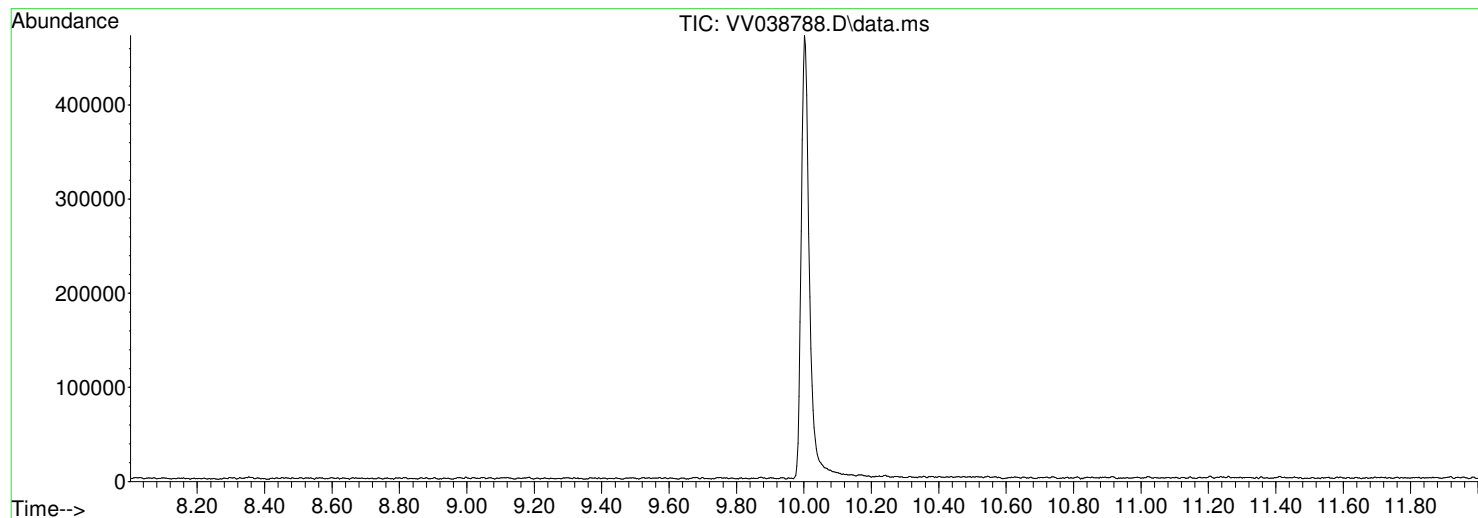

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	18277	PASS
75	95	30	80	54.4	47597	PASS
95	95	100	100	100.0	87435	PASS
96	95	5	9	6.4	5624	PASS
173	174	0.00	2	1.6	1099	PASS
174	95	50	120	78.5	68648	PASS
175	174	5	9	8.4	5783	PASS
176	174	95	105	97.2	66709	PASS
177	176	5	10	6.6	4418	PASS

m/z	Abundance
35.80	101.0
36.90	147.0
37.70	148.0
38.60	136.0
39.10	127.0
39.90	388.0
41.70	121.0
42.80	142.0
43.90	776.0
44.90	119.0
46.30	126.0
47.30	144.0
48.00	201.0
51.70	106.0
54.20	102.0
54.80	152.0
60.70	102.0
62.80	132.0
73.10	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	911.0
37.00	4222.0
38.00	4375.0
39.00	2412.0
40.20	462.0
41.90	152.0
44.00	1316.0
45.00	825.0
46.00	354.0
46.90	1727.0
47.90	810.0
49.00	4199.0
50.00	17856.0
51.00	5604.0
52.00	337.0
52.90	301.0
54.00	201.0
54.90	305.0
55.90	1488.0
57.00	2508.0
57.90	127.0
60.00	1013.0
61.00	5025.0
62.00	4715.0
63.00	4708.0
63.90	1166.0
65.10	875.0
66.20	176.0
66.90	354.0
68.00	9189.0
69.00	9648.0
70.00	805.0
72.00	644.0
73.00	4446.0
74.00	15207.0
75.00	45808.0
76.00	3890.0
77.00	622.0
77.80	400.0
78.90	5102.0
79.90	1049.0
80.90	4878.0
81.90	1180.0
85.30	244.0
85.90	183.0
87.00	3580.0
87.90	4068.0
91.00	343.0
92.00	2434.0
93.00	4099.0
94.00	11264.0
95.00	84264.0
96.00	5496.0
97.00	165.0
97.40	164.0
99.80	113.0
103.00	220.0
103.80	413.0
104.80	150.0
105.20	153.0
105.80	502.0
107.10	163.0
108.00	156.0
109.90	168.0
112.00	176.0
112.90	106.0
114.90	142.0
115.80	401.0
116.90	913.0
117.80	379.0
118.80	732.0
121.20	117.0
127.80	445.0
128.90	271.0
129.80	278.0
130.90	209.0
134.70	188.0
136.70	201.0
138.80	133.0
141.00	843.0
142.10	132.0
143.00	1968.0
144.90	752.0
146.00	292.0
147.90	279.0
148.70	157.0
149.60	116.0
154.90	279.0
157.00	174.0
159.00	139.0
160.70	121.0
170.90	478.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

171.90	860.0
173.10	1155.0
174.00	64664.0
175.00	5339.0
176.00	61736.0
177.00	4095.0
178.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	991.0
37.00	4522.0
38.10	4419.0
39.00	2647.0
40.20	519.0
41.90	186.0
44.00	1396.0
45.00	895.0
46.00	331.0
47.00	1667.0
47.90	766.0
49.00	4083.0
50.00	18880.0
51.00	6152.0
52.00	383.0
52.90	270.0
54.00	197.0
55.00	260.0
55.90	1518.0
57.00	2810.0
58.10	168.0
59.90	1178.0
61.00	5327.0
62.00	5028.0
63.00	4735.0
64.00	1180.0
65.10	890.0
66.10	246.0
67.10	327.0
68.00	9862.0
69.00	10766.0
70.00	930.0
72.00	746.0
73.00	4464.0
74.00	15939.0
75.00	49376.0
76.00	4164.0
76.90	607.0
78.90	5430.0
79.90	1130.0
80.90	5457.0
81.90	1116.0
82.90	121.0
85.30	171.0
85.90	199.0
87.00	3898.0
87.90	4377.0
91.00	415.0
92.00	2722.0
93.00	4807.0
94.00	11731.0
95.00	90424.0
96.00	5823.0
96.90	191.0
97.30	175.0
103.00	253.0
103.80	401.0
104.80	205.0
105.90	586.0
107.10	189.0
107.90	270.0
109.90	176.0
111.00	113.0
112.00	185.0
112.80	192.0
115.00	151.0
115.90	439.0
117.00	961.0
117.80	411.0
118.90	810.0
127.80	485.0
128.90	342.0
129.80	322.0
130.80	240.0
134.70	207.0
136.80	242.0
138.80	167.0
141.00	968.0
142.10	156.0
143.00	2200.0
144.90	829.0
146.00	238.0
147.80	384.0
148.70	131.0
149.80	205.0
153.80	104.0
154.90	433.0
155.70	128.0
156.90	205.0
159.00	163.0
169.90	135.0
170.90	447.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

171.90	981.0
173.00	1081.0
174.00	71112.0
175.00	6123.0
176.00	68992.0
177.00	4595.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	940.0
37.00	4180.0
38.10	4180.0
39.00	2485.0
40.20	482.0
41.90	159.0
44.00	1415.0
45.00	862.0
46.10	305.0
47.00	1445.0
48.00	627.0
49.00	3706.0
50.00	18096.0
51.00	5904.0
52.00	352.0
52.90	227.0
53.90	209.0
55.00	205.0
55.90	1492.0
57.00	2871.0
57.80	146.0
58.20	174.0
60.00	1231.0
61.00	5240.0
62.00	4868.0
63.00	4088.0
64.00	1058.0
65.00	809.0
66.10	239.0
67.10	275.0
68.00	9367.0
69.00	10704.0
70.00	948.0
70.90	123.0
72.00	714.0
73.00	4159.0
74.00	15378.0
75.00	47608.0
76.00	4117.0
76.90	595.0
78.10	397.0
78.90	5320.0
79.90	1113.0
80.90	5400.0
81.90	1010.0
82.90	133.0
85.90	163.0
87.00	3844.0
87.90	4014.0
91.00	486.0
92.00	2721.0
93.00	4885.0
94.00	11469.0
95.00	87616.0
96.00	5552.0
96.90	197.0
97.30	172.0
103.00	195.0
103.80	409.0
104.80	248.0
105.90	611.0
107.10	176.0
107.90	343.0
110.00	171.0
111.10	147.0
112.00	148.0
112.80	244.0
115.00	124.0
115.90	421.0
117.00	897.0
117.80	388.0
118.90	814.0
123.70	125.0
127.80	448.0
128.90	336.0
129.70	342.0
130.80	241.0
134.70	230.0
136.90	278.0
138.90	153.0
140.10	196.0
140.90	1030.0
142.10	172.0
143.00	2081.0
143.70	124.0
144.80	843.0
145.90	159.0
146.80	112.0
147.80	442.0
149.80	238.0
154.90	448.0
155.70	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

156.80	257.0
159.00	130.0
169.90	131.0
170.90	429.0
172.00	1038.0
172.90	1061.0
174.00	70168.0
175.00	5886.0
176.00	69400.0
177.00	4565.0
222.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209