
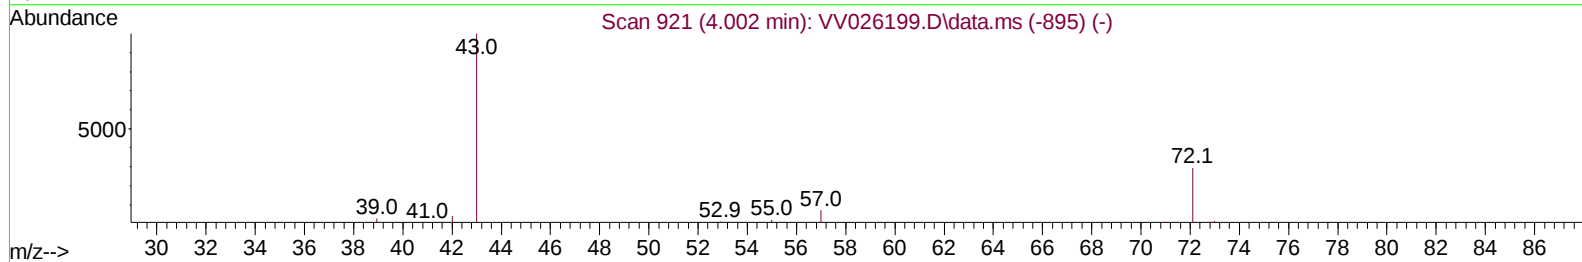
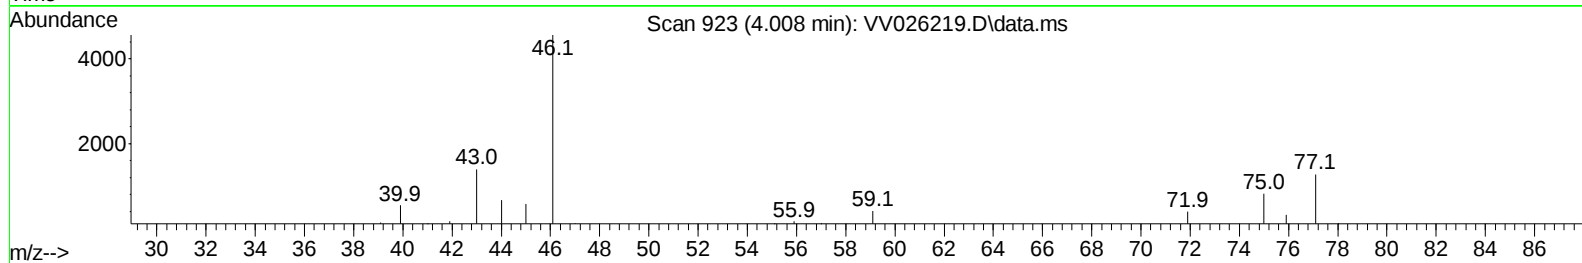


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026219.D
 Acq On : 13 Jun 2022 19:10
 Operator : SY/MD
 Sample : N3273-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: Jun 14 02:41:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

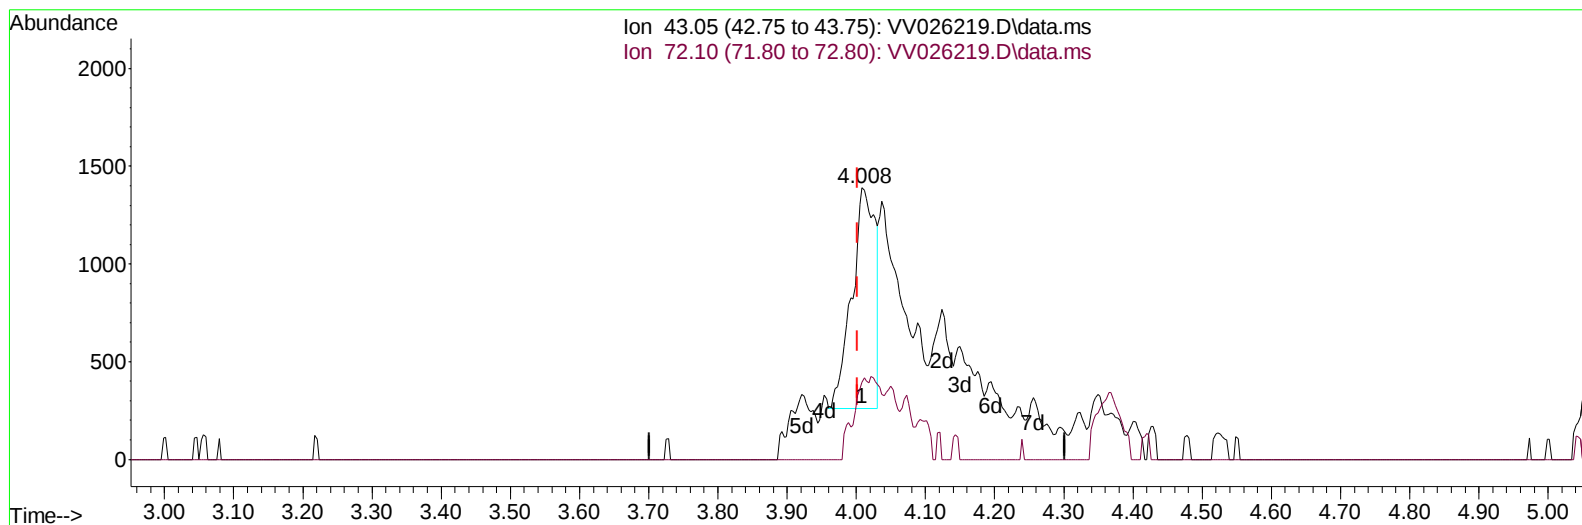

TIC: VV026219.D\data.ms

(21) 2-Butanone (T)




4.008min (+ 0.007) 2.22 ug/L

response 2655

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	21.20	24.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026219.D
Acq On : 13 Jun 2022 19:10
Operator : SY/MD
Sample : N3273-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Jun 14 02:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration

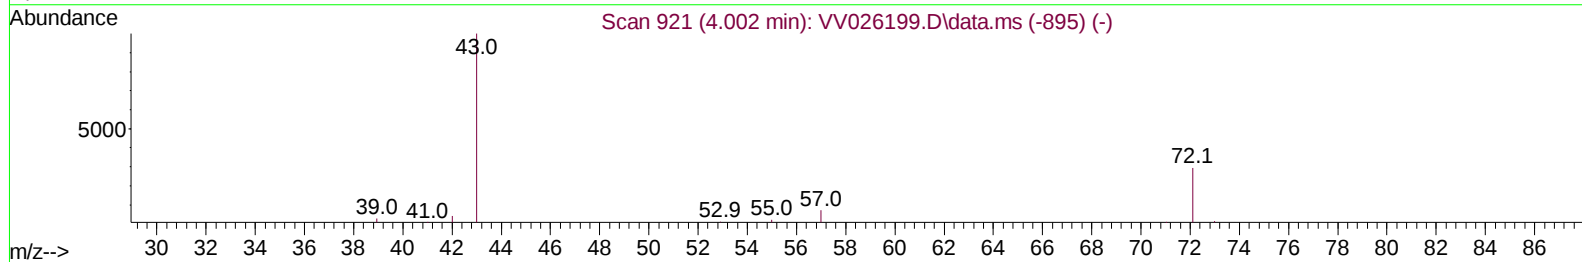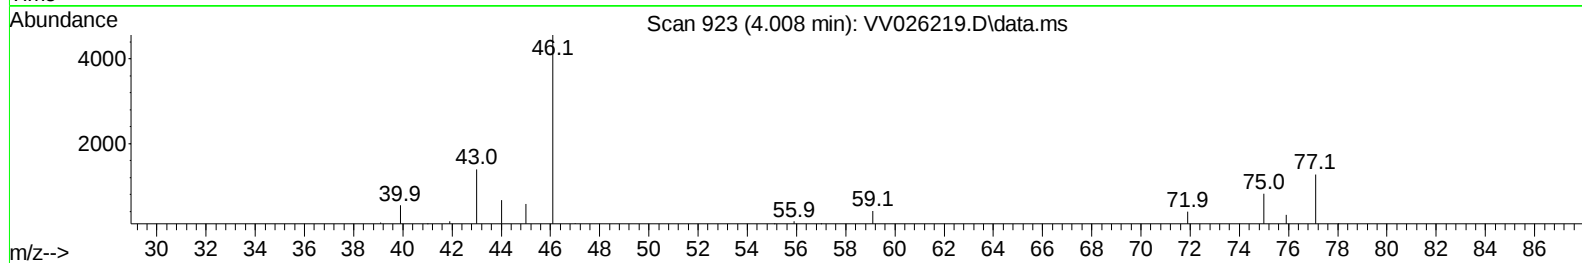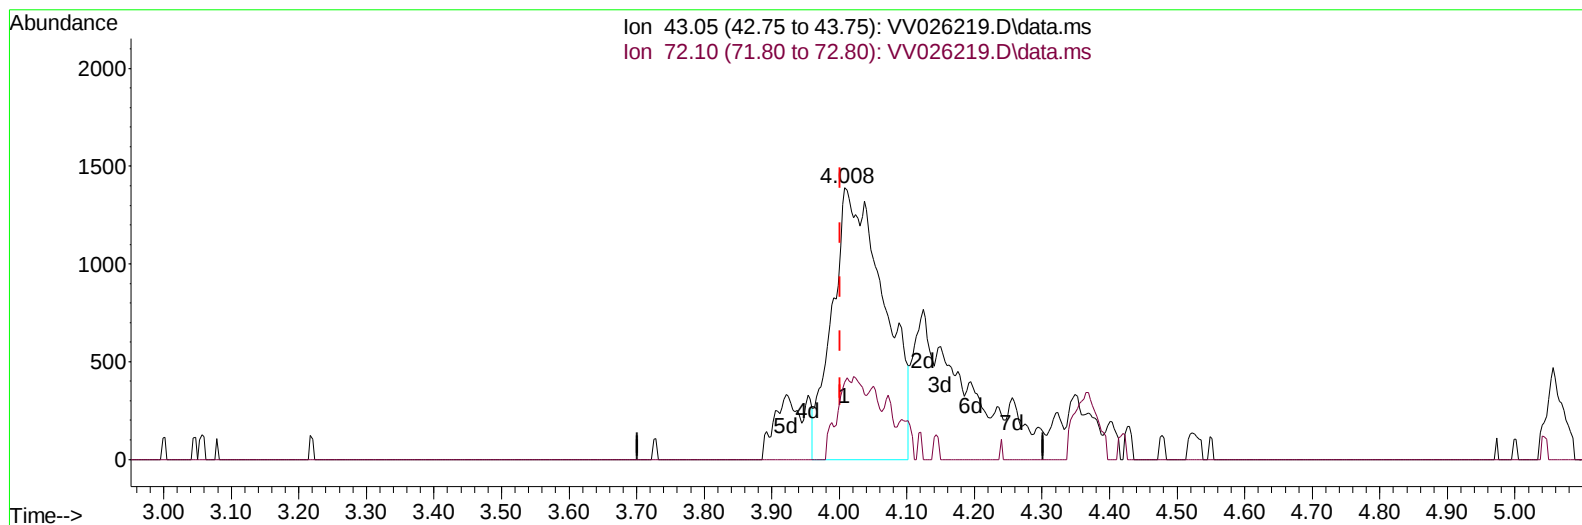

TIC: VV026219.D\data.ms

(21) 2-Butanone (T)

4.008min (+ 0.007) 6.14 ug/L m

response 7354

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	21.20	8.85#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026219.D
 Acq On : 13 Jun 2022 19:10
 Operator : SY/MD
 Sample : N3273-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: Jun 14 02:41:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	158010	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	156720	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64972	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	86077	4.166	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	83.400%	
7) Chloroethane-d5	1.577	69	72433	4.450	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.000%	
11) 1,1-Dichloroethene-d2	2.118	63	113947	3.430	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.600%	
20) 2-Butanone-d5	3.915	46	106286	68.946	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	137.900%#	
24) Chloroform-d	4.359	84	134098	4.576	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.600%	
26) 1,2-Dichloroethane-d4	5.044	65	56864	4.813	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.200%	
32) Benzene-d6	5.056	84	256270	4.194	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.800%	
36) 1,2-Dichloropropane-d6	6.072	67	79353	4.504	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.000%	
41) Toluene-d8	7.317	98	203639	3.743	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	74.800%	
43) trans-1,3-Dichloroprop...	7.625	79	21810	4.101	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.092	63	80626	48.694	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.380%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47868	4.560	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	69616	4.780	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	95.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.208	43	126061	143.223	ug/L	95
21) 2-Butanone	4.008	43	7354m	6.138	ug/L	
34) Trichloroethene	5.925	95	11466	0.896	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026219.D
Acq On : 13 Jun 2022 19:10
Operator : SY/MD
Sample : N3273-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Jun 14 02:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration

