

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026200.D
 Acq On : 13 Jun 2022 11:33
 Operator : SY/MD
 Sample : VV0613WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK370

Quant Time: Jun 14 02:37:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	164807	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	160769	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67868	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	94129	4.367	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.400%
7) Chloroethane-d5	1.574	69	76774	4.523	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.400%
11) 1,1-Dichloroethene-d2	2.114	63	125423	3.619	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.400%
20) 2-Butanone-d5	3.918	46	86986	54.099	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.200%
24) Chloroform-d	4.355	84	138916	4.545	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	5.040	65	62528	5.074	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.400%
32) Benzene-d6	5.056	84	282933	4.514	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%
36) 1,2-Dichloropropane-d6	6.072	67	86109	4.764	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%
41) Toluene-d8	7.317	98	227318	4.073	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	7.625	79	25833	4.736	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.800%
46) 2-Hexanone-d5	8.092	63	81135	47.767	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.540%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	50626	4.701	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	73588	4.837	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
16) Methylene chloride	2.516	84	9795	0.754	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026200.D
Acq On : 13 Jun 2022 11:33
Operator : SY/MD
Sample : VV0613WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Quant Time: Jun 14 02:37:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration

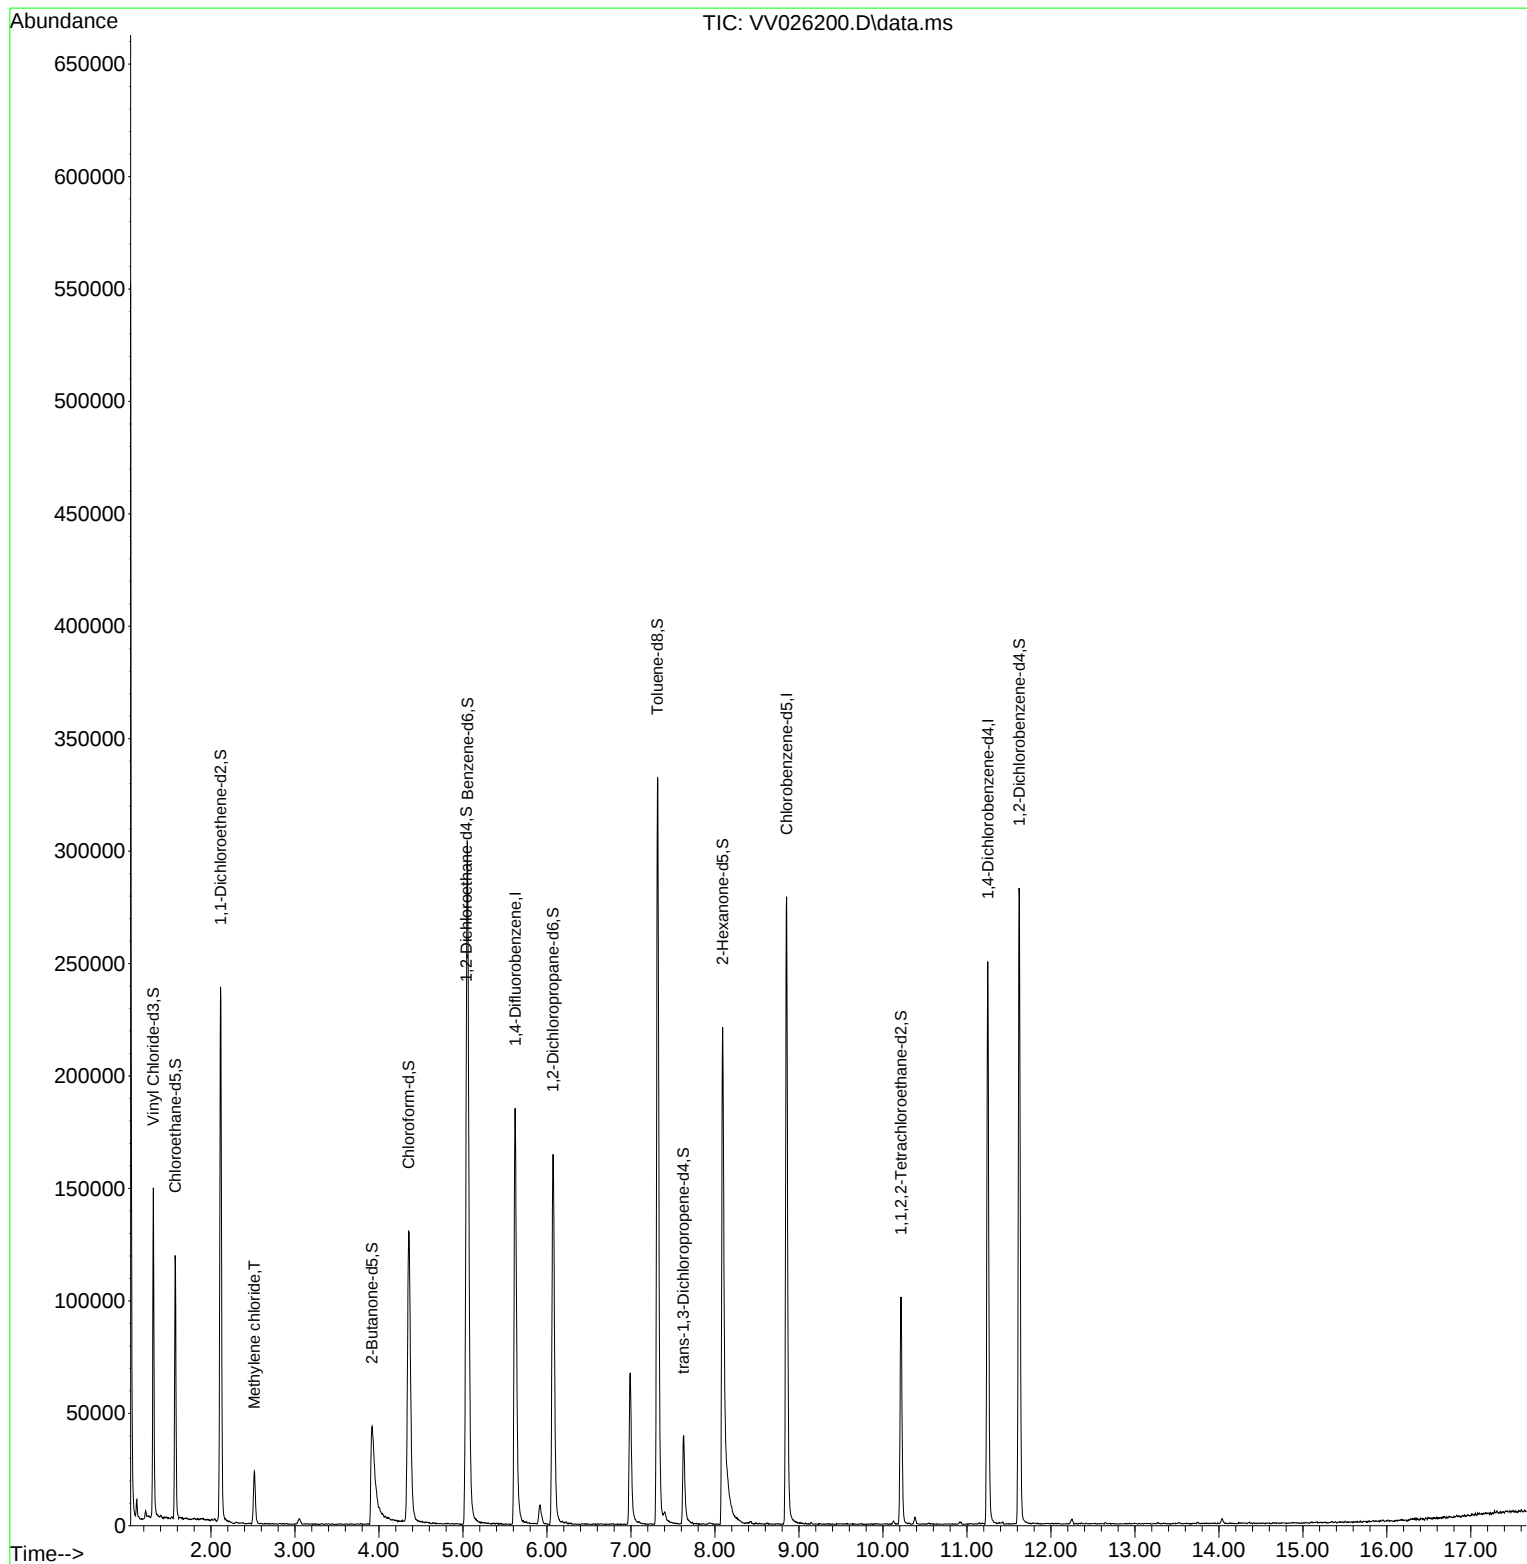

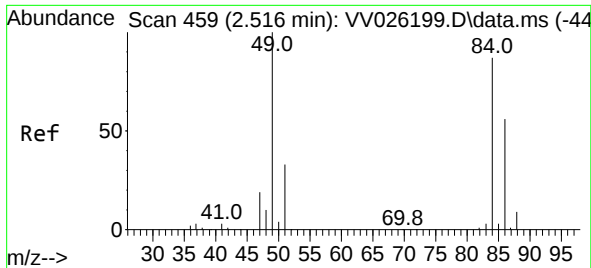

#16
Methylene chloride
Concen: 0.754 ug/L
RT: 2.516 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV026200.D
Acq: 13 Jun 2022 11:33

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Tgt Ion: 84 Resp: 9795
Ion Ratio Lower Upper
84 100
86 69.1 45.1 83.7
49 109.6 82.3 152.9

