

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061322\
 Data File : VW026206.D
 Acq On : 13 Jun 2022 13:58
 Operator : SY/MD
 Sample : N3289-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DT2

Quant Time: Jun 14 02:38:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	188673	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	182736	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75222	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	92157	3.735	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	74.800%	
7) Chloroethane-d5	1.577	69	73901	3.803	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	76.000%	
11) 1,1-Dichloroethene-d2	2.118	63	120551	3.039	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.800%	
20) 2-Butanone-d5	3.912	46	98712	53.626	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.260%	
24) Chloroform-d	4.359	84	138006	3.944	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	78.800%	
26) 1,2-Dichloroethane-d4	5.040	65	62166	4.407	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.200%	
32) Benzene-d6	5.056	84	274454	3.853	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	77.000%	
36) 1,2-Dichloropropane-d6	6.076	67	83168	4.048	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	81.000%	
41) Toluene-d8	7.320	98	219791	3.465	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	69.200%#	
43) trans-1,3-Dichloroprop...	7.629	79	22957	3.702	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	74.000%	
46) 2-Hexanone-d5	8.092	63	84375	43.703	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	87.400%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49893	4.076	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	81.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	71175	4.221	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	84.400%	
Target Compounds						Qvalue
34) Trichloroethene	5.924	95	7838	0.525	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026206.D
Acq On : 13 Jun 2022 13:58
Operator : SY/MD
Sample : N3289-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT2


Quant Time: Jun 14 02:38:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration

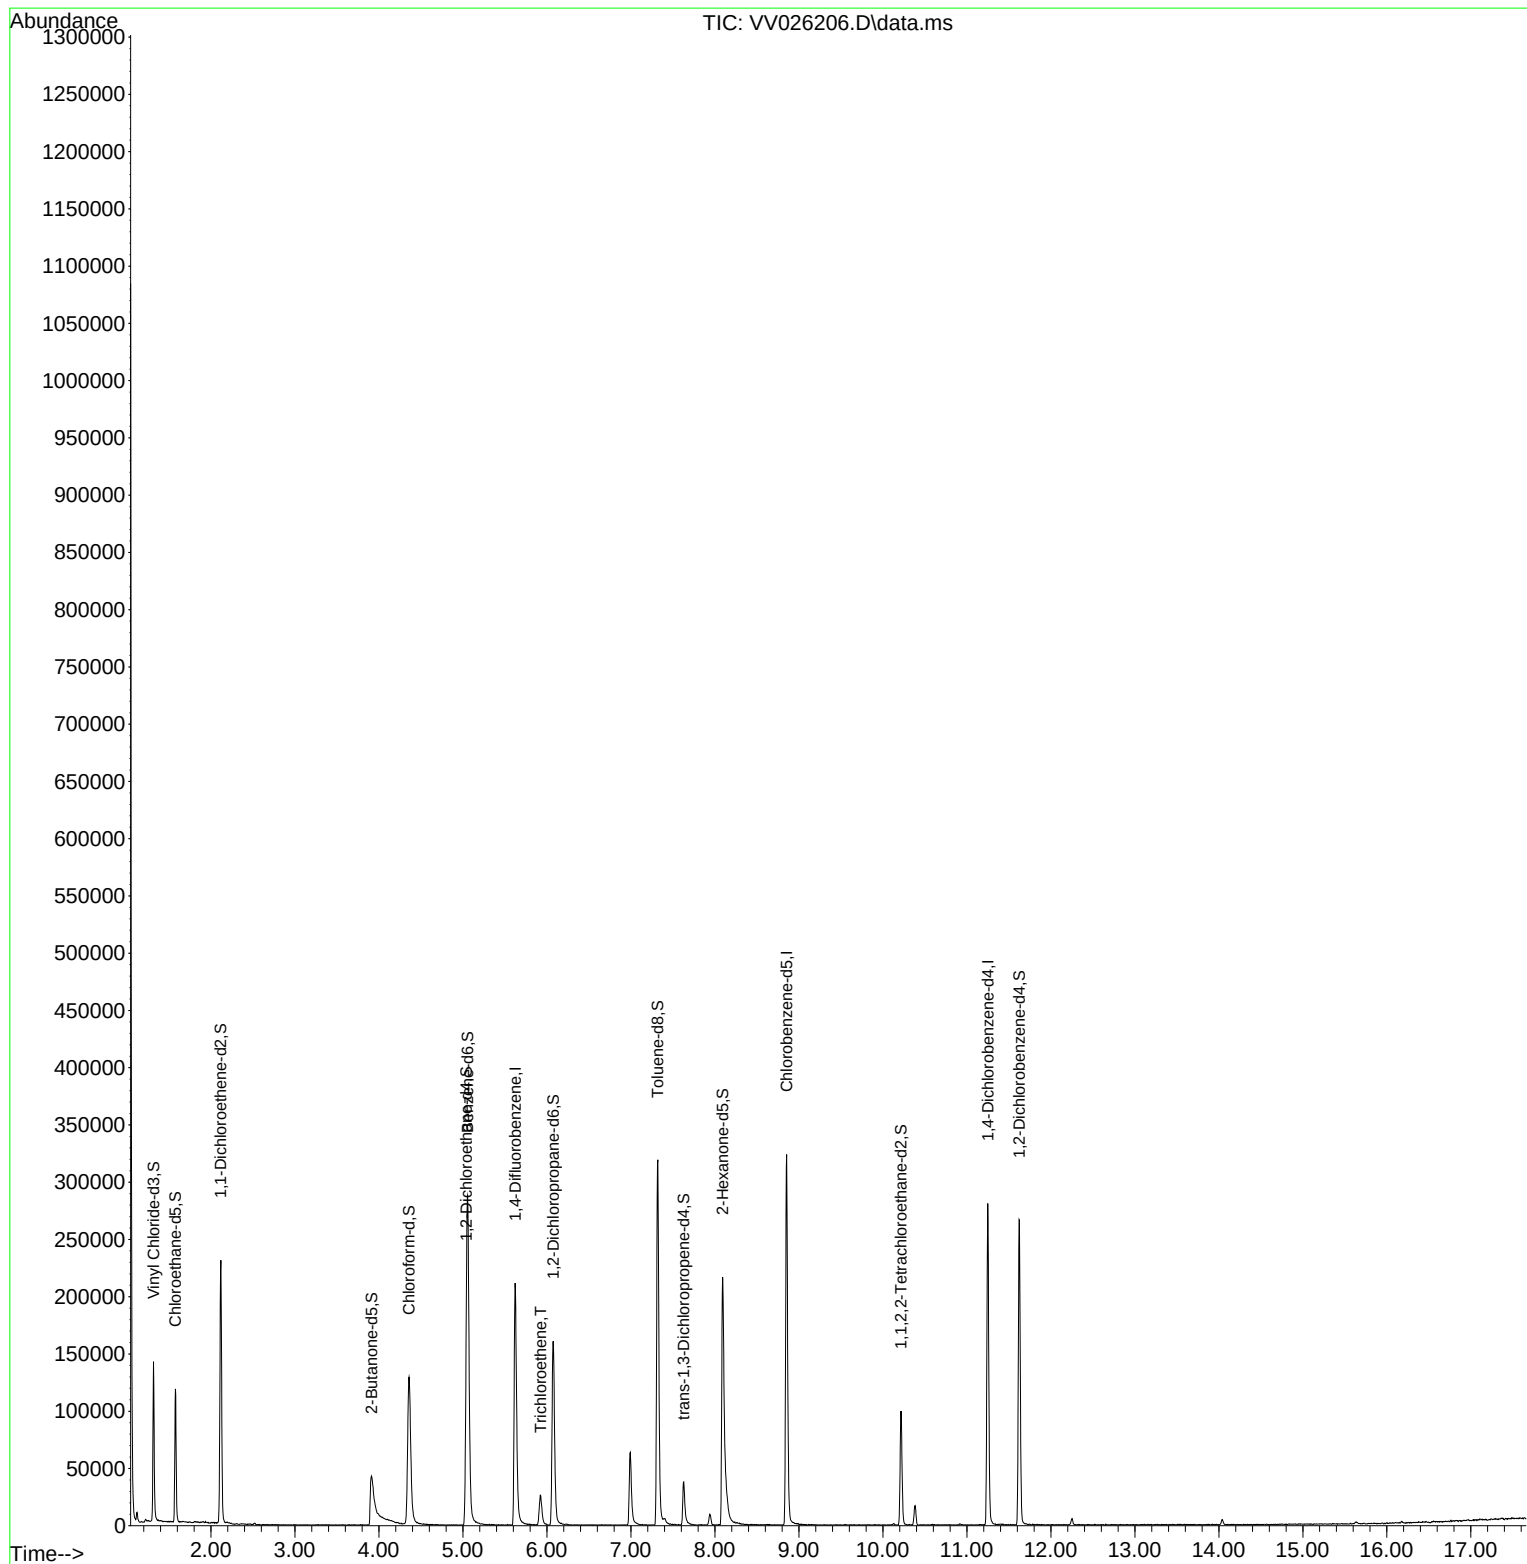

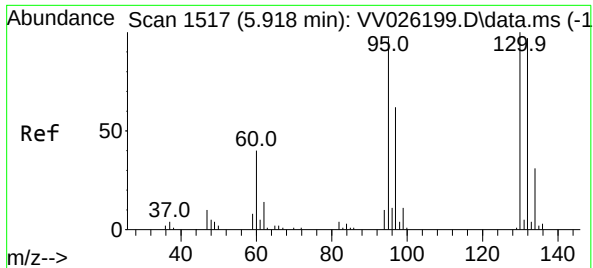

#34
 Trichloroethene
 Concen: 0.525 ug/L
 RT: 5.924 min Scan# 11
 Delta R.T. 0.007 min
 Lab File: VV026206.D
 Acq: 13 Jun 2022 13:58

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DT2

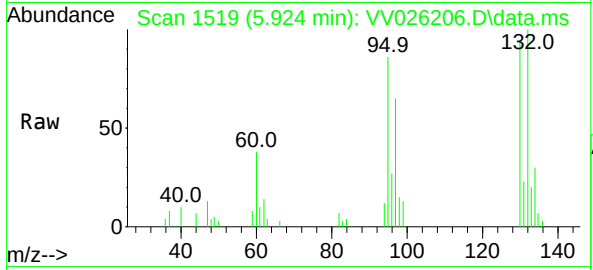

Tgt Ion: 95 Resp: 7838

Ion	Ratio	Lower	Upper
95	100		
97	75.3	43.3	80.3
132	115.8	67.5	125.4
130	109.2	70.9	131.7

