

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061322\
 Data File : VW026207.D
 Acq On : 13 Jun 2022 14:22
 Operator : SY/MD
 Sample : N3289-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DT3

Quant Time: Jun 14 02:38:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	187023	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	182693	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	74866	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	92175	3.769	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.400%
7) Chloroethane-d5	1.577	69	75249	3.906	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.200%
11) 1,1-Dichloroethene-d2	2.117	63	122770	3.122	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.400%
20) 2-Butanone-d5	3.915	46	114694	62.858	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.720%
24) Chloroform-d	4.359	84	142008	4.094	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.800%
26) 1,2-Dichloroethane-d4	5.040	65	61317	4.385	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
32) Benzene-d6	5.056	84	276107	3.877	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.600%
36) 1,2-Dichloropropane-d6	6.076	67	85333	4.155	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.000%
41) Toluene-d8	7.320	98	221713	3.496	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.000%
43) trans-1,3-Dichloroprop...	7.625	79	25499	4.113	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.200%
46) 2-Hexanone-d5	8.092	63	85841	44.473	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.940%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	50520	4.129	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	73765	4.396	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.000%
Target Compounds						
					Qvalue	
13) Acetone	2.208	43	4614	4.429	ug/L	76
34) Trichloroethene	5.928	95	7415	0.497	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026207.D
Acq On : 13 Jun 2022 14:22
Operator : SY/MD
Sample : N3289-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT3

Quant Time: Jun 14 02:38:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration




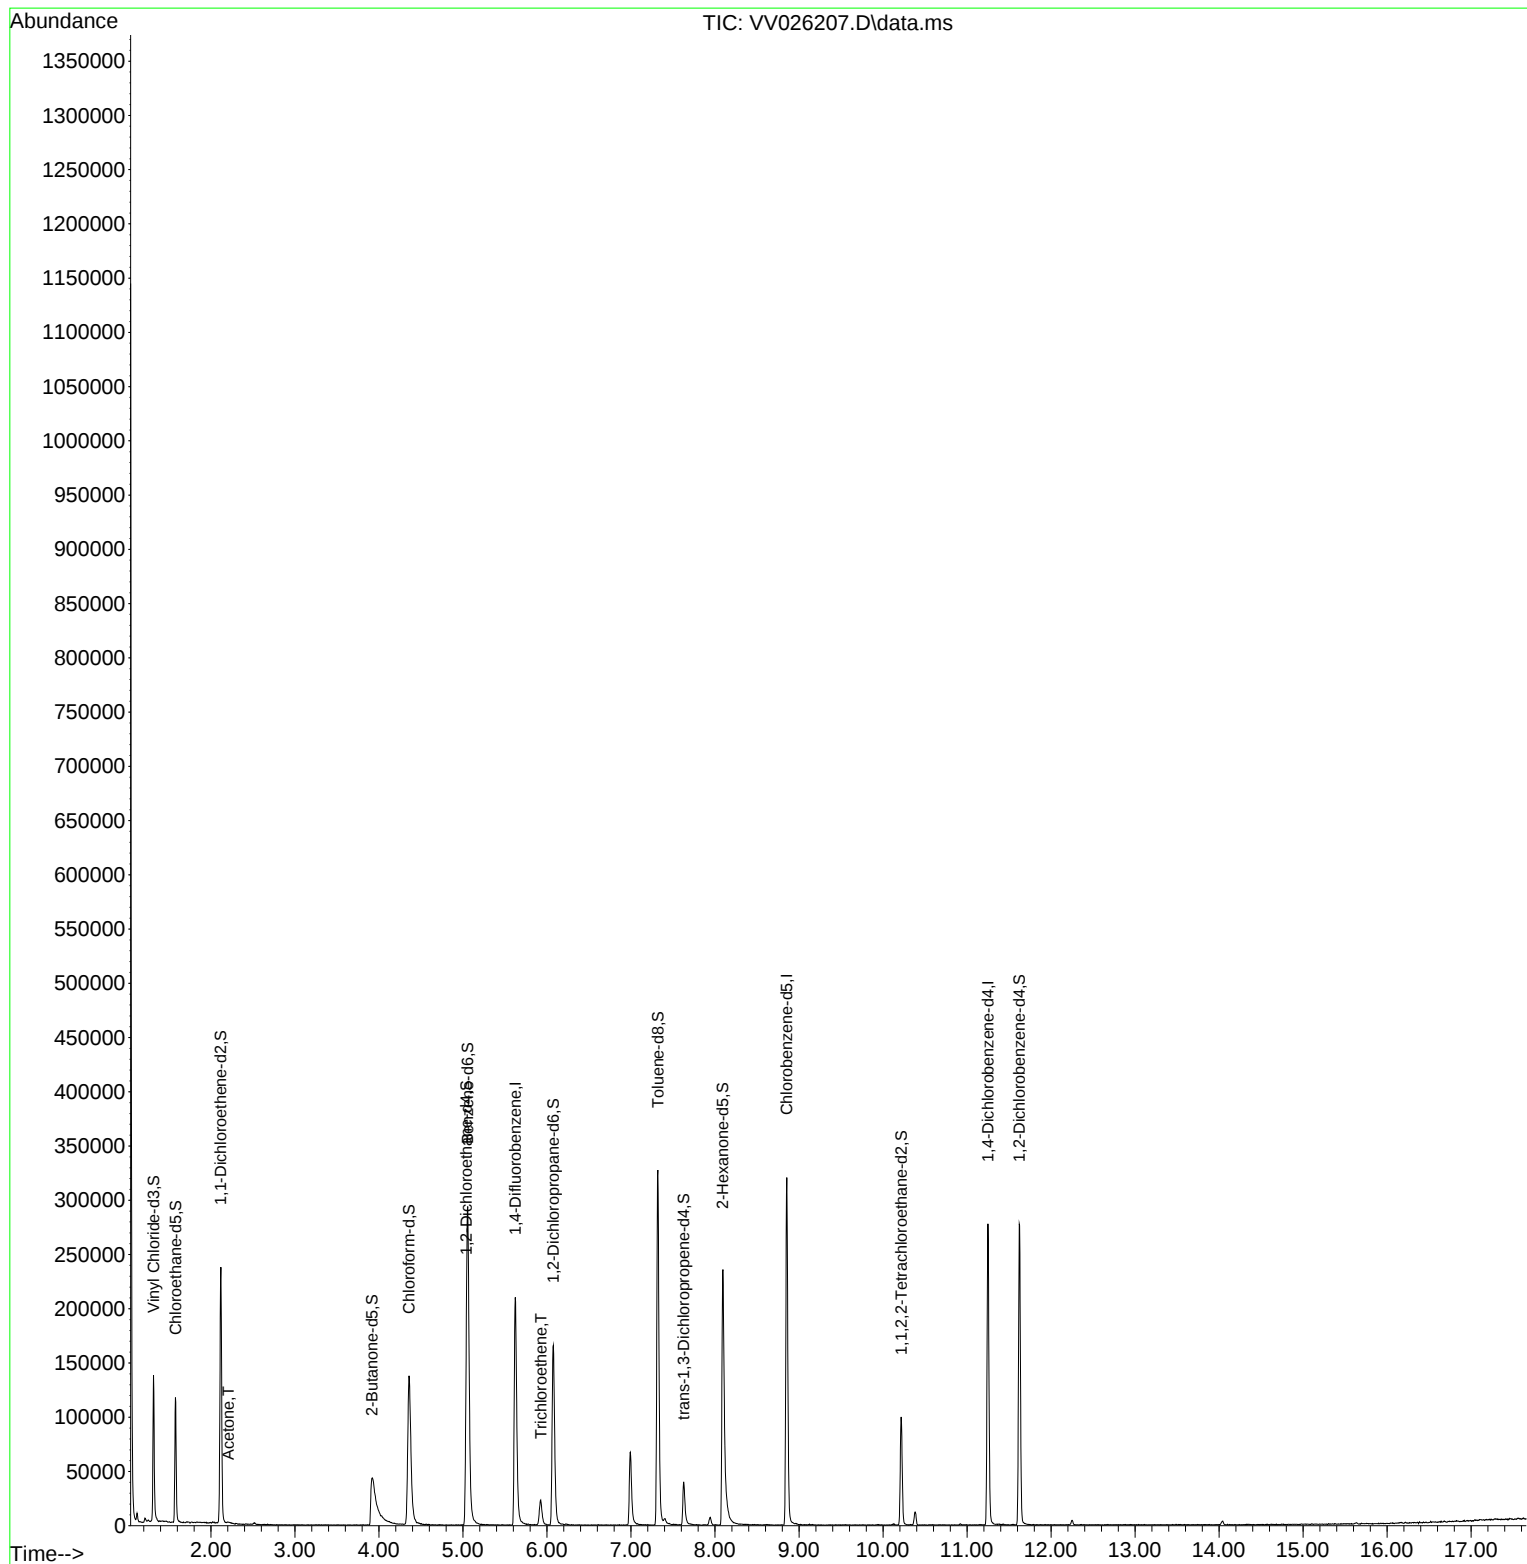


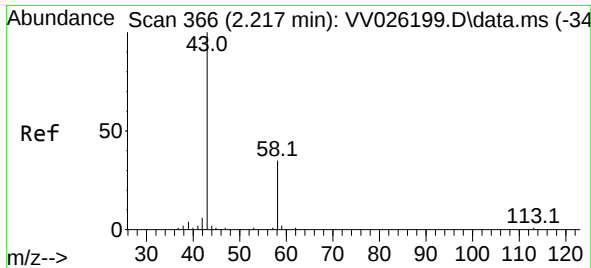

#13
Acetone
Concen: 4.429 ug/L
RT: 2.208 min Scan# 30
Delta R.T. -0.010 min
Lab File: VV026207.D
Acq: 13 Jun 2022 14:22

Instrument :
MSVOA_V
ClientSampleId :
C0DT3

Tgt Ion: 43 Resp: 4614
Ion Ratio Lower Upper
43 100
58 22.7 0.0 73.6

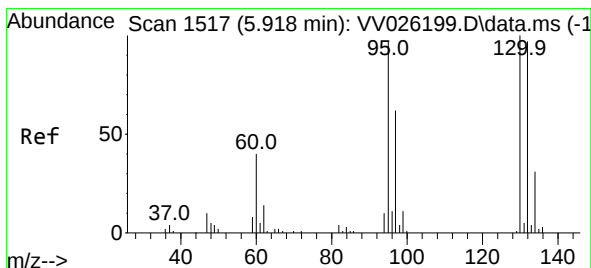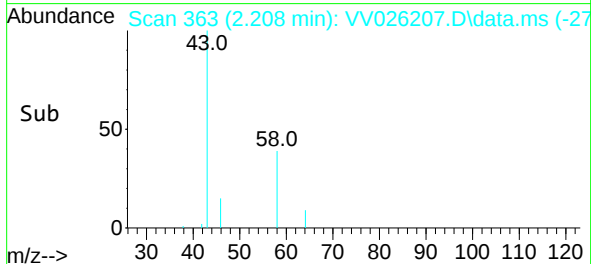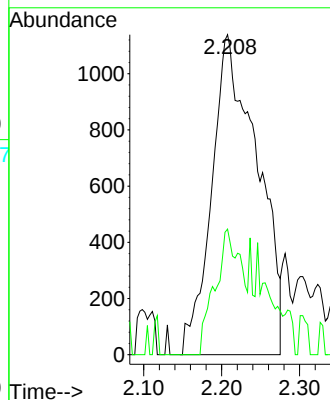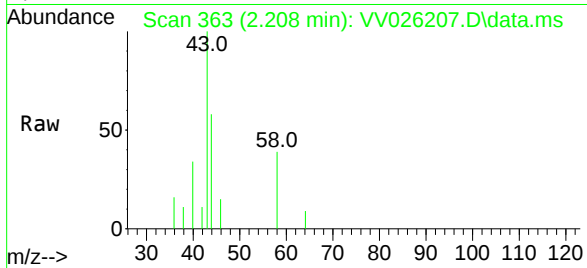

#34
Trichloroethene
Concen: 0.497 ug/L
RT: 5.928 min Scan# 1520
Delta R.T. 0.010 min
Lab File: VV026207.D
Acq: 13 Jun 2022 14:22

Tgt Ion: 95 Resp: 7415
Ion Ratio Lower Upper
95 100
97 67.4 43.3 80.3
132 90.1 67.5 125.4
130 102.1 70.9 131.7

