

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061322\
 Data File : VW026208.D
 Acq On : 13 Jun 2022 14:46
 Operator : SY/MD
 Sample : N3289-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DT4

Quant Time: Jun 14 02:39:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	165156	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	161902	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66986	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	88448	4.095	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.000%
7) Chloroethane-d5	1.577	69	72929	4.287	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.800%
11) 1,1-Dichloroethene-d2	2.118	63	118054	3.399	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.000%
20) 2-Butanone-d5	3.918	46	102862	63.838	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	127.680%
24) Chloroform-d	4.359	84	135407	4.421	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	5.040	65	57311	4.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	5.056	84	266103	4.216	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
36) 1,2-Dichloropropane-d6	6.076	67	81437	4.474	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.400%
41) Toluene-d8	7.320	98	212195	3.776	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.600%
43) trans-1,3-Dichloroprop...	7.629	79	23098	4.205	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.092	63	79134	46.263	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.520%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	48460	4.469	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	69539	4.631	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%
Target Compounds						
					Qvalue	
3) Chloromethane	1.249	50	1997	0.121	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026208.D
Acq On : 13 Jun 2022 14:46
Operator : SY/MD
Sample : N3289-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT4

Quant Time: Jun 14 02:39:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration

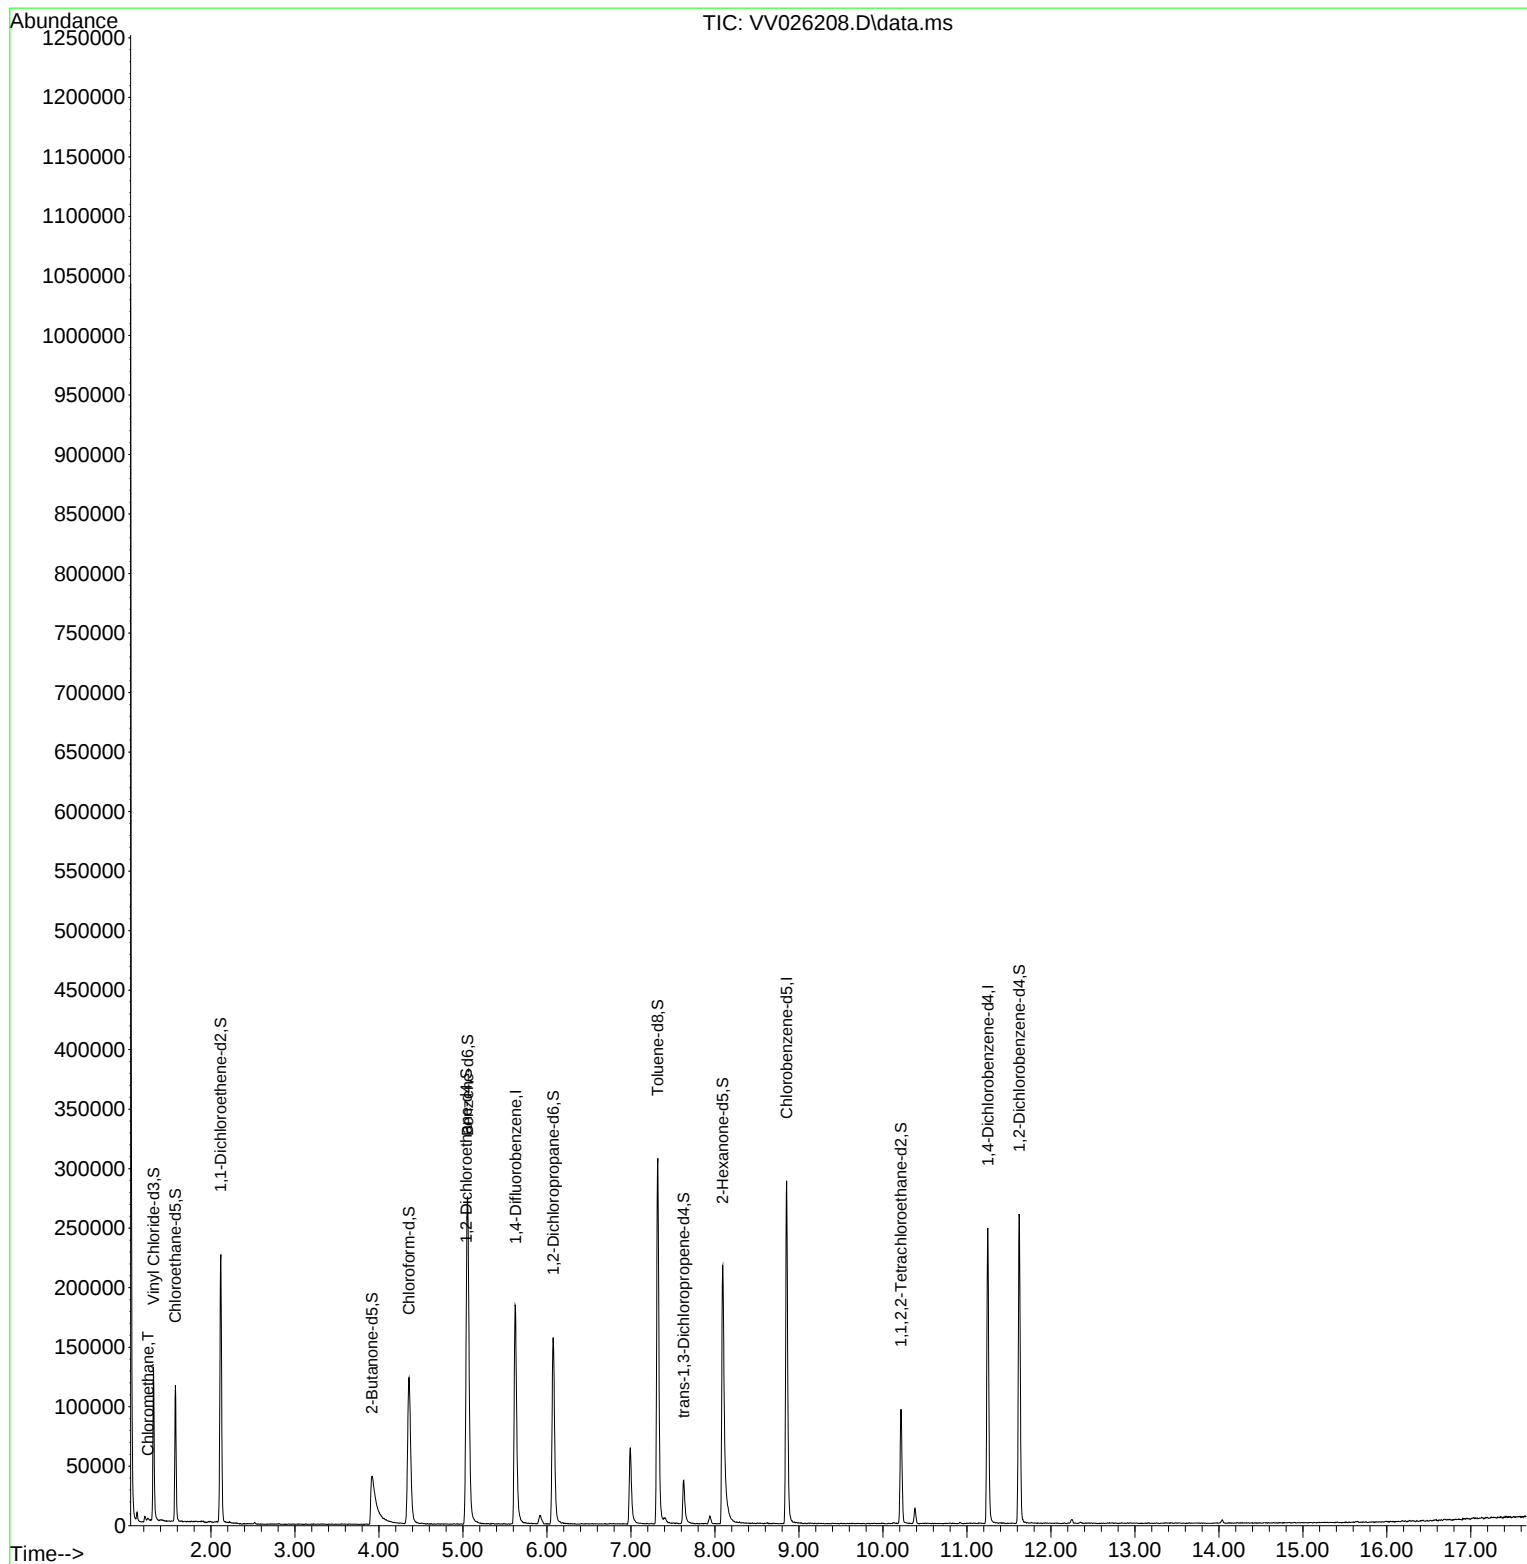


Abundance Scan 66 (1.252 min): VV026199.D\data.ms (-57)

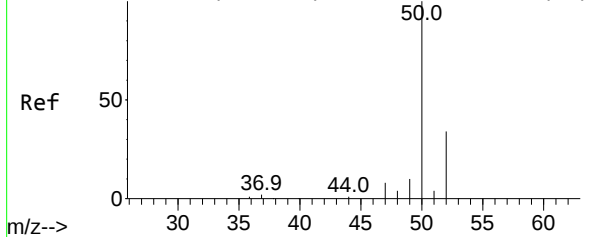

#3
Chloromethane
Concen: 0.121 ug/L
RT: 1.249 min Scan# 61
Delta R.T. -0.003 min
Lab File: VV026208.D
Acq: 13 Jun 2022 14:46

Instrument :
MSVOA_V
ClientSampleId :
C0DT4

Abundance Scan 65 (1.249 min): VV026208.D\data.ms

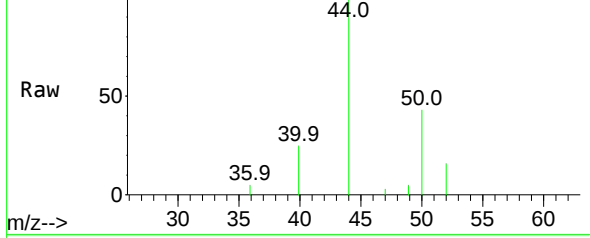

Tgt Ion: 50 Resp: 1997
Ion Ratio Lower Upper
50 100
52 36.7 23.6 43.8

Abundance Scan 65 (1.249 min): VV026208.D\data.ms (-1)

