

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061322\
 Data File : VW026209.D
 Acq On : 13 Jun 2022 15:10
 Operator : SY/MD
 Sample : N3289-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODW6

Quant Time: Jun 14 02:39:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	170054	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	167409	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68803	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	101808	4.578	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.600%	
7) Chloroethane-d5	1.577	69	82084	4.686	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.800%	
11) 1,1-Dichloroethene-d2	2.118	63	132170	3.696	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	74.000%	
20) 2-Butanone-d5	3.909	46	101735	61.320	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	122.640%	
24) Chloroform-d	4.359	84	149477	4.740	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.800%	
26) 1,2-Dichloroethane-d4	5.040	65	65620	5.161	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.200%	
32) Benzene-d6	5.056	84	300104	4.598	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.000%	
36) 1,2-Dichloropropane-d6	6.076	67	94209	5.006	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.200%	
41) Toluene-d8	7.320	98	243242	4.186	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	7.625	79	26178	4.608	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.200%	
46) 2-Hexanone-d5	8.092	63	94293	53.312	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	106.620%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	55589	4.958	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	78050	5.061	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.200%	
Target Compounds					Qvalue	
25) Chloroform	4.391	83	18211	0.728	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026209.D
Acq On : 13 Jun 2022 15:10
Operator : SY/MD
Sample : N3289-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DW6

Quant Time: Jun 14 02:39:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration

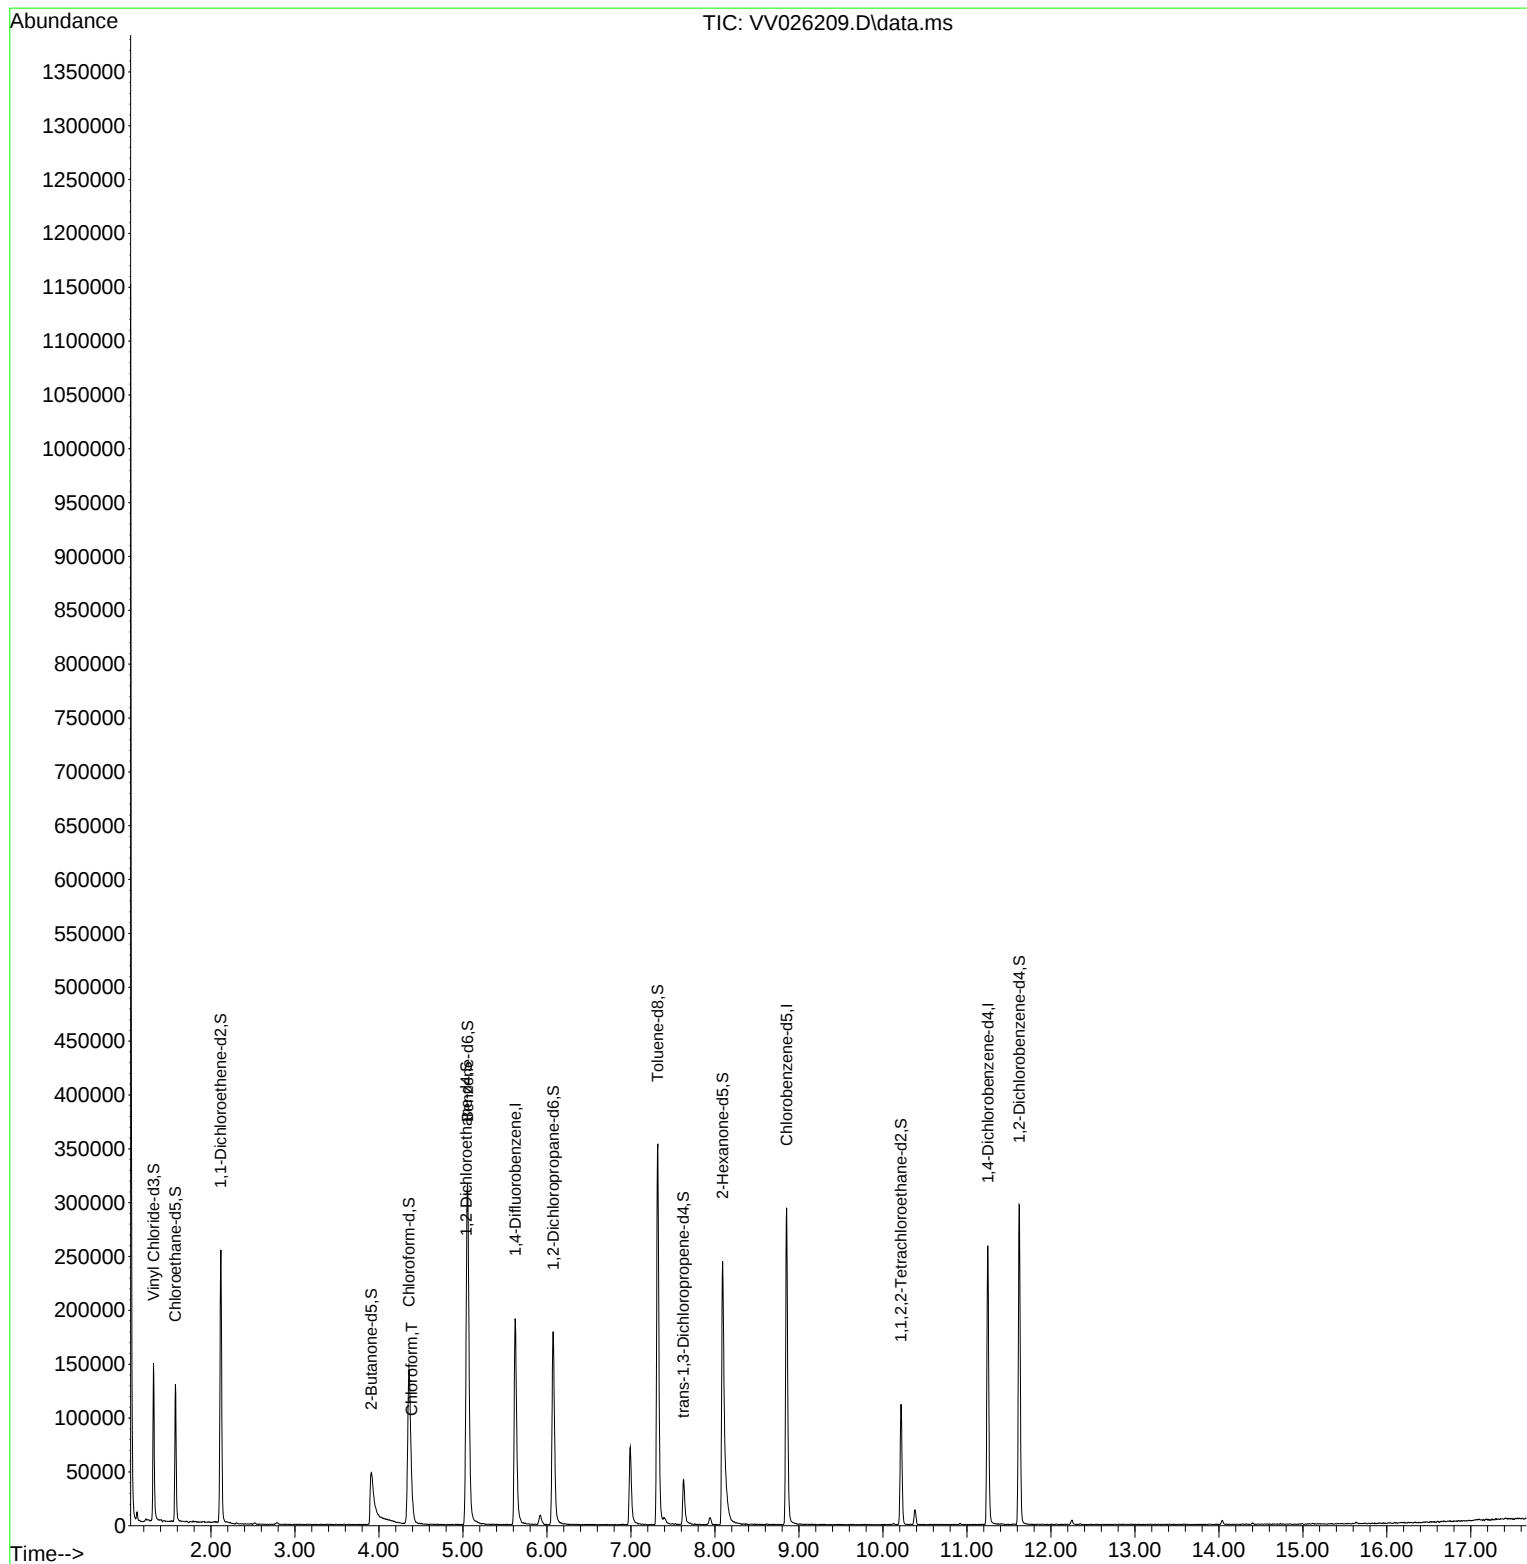

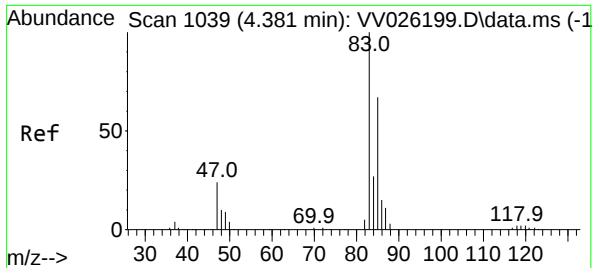

#25
 Chloroform
 Concen: 0.728 ug/L
 RT: 4.391 min Scan# 10
 Delta R.T. 0.010 min
 Lab File: VV026209.D
 Acq: 13 Jun 2022 15:10

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DW6

Tgt Ion: 83 Resp: 18211
 Ion Ratio Lower Upper
 83 100
 85 61.5 45.3 84.1

