

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061322\
 Data File : VW026211.D
 Acq On : 13 Jun 2022 15:58
 Operator : SY/MD
 Sample : N3312-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 14 02:39:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 14 02:36:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	162660	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	162612	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66613	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	84387	3.967	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.400%	
7) Chloroethane-d5	1.574	69	68321	4.078	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	81.600%	
11) 1,1-Dichloroethene-d2	2.114	63	110410	3.228	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.600%	
20) 2-Butanone-d5	3.908	46	80275	50.584	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	101.160%	
24) Chloroform-d	4.355	84	124029	4.112	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.200%	
26) 1,2-Dichloroethane-d4	5.040	65	55693	4.579	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.600%	
32) Benzene-d6	5.056	84	245213	3.868	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	77.400%	
36) 1,2-Dichloropropane-d6	6.075	67	76634	4.192	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	83.800%	
41) Toluene-d8	7.317	98	195783	3.468	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	69.400%#	
43) trans-1,3-Dichloroprop...	7.628	79	21423	3.883	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	77.600%	
46) 2-Hexanone-d5	8.091	63	75255	43.803	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	87.600%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45750	4.200	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	84.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	65441	4.383	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	87.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	3452	0.269	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026211.D
Acq On : 13 Jun 2022 15:58
Operator : SY/MD
Sample : N3312-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jun 14 02:39:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 14 02:36:38 2022
Response via : Initial Calibration

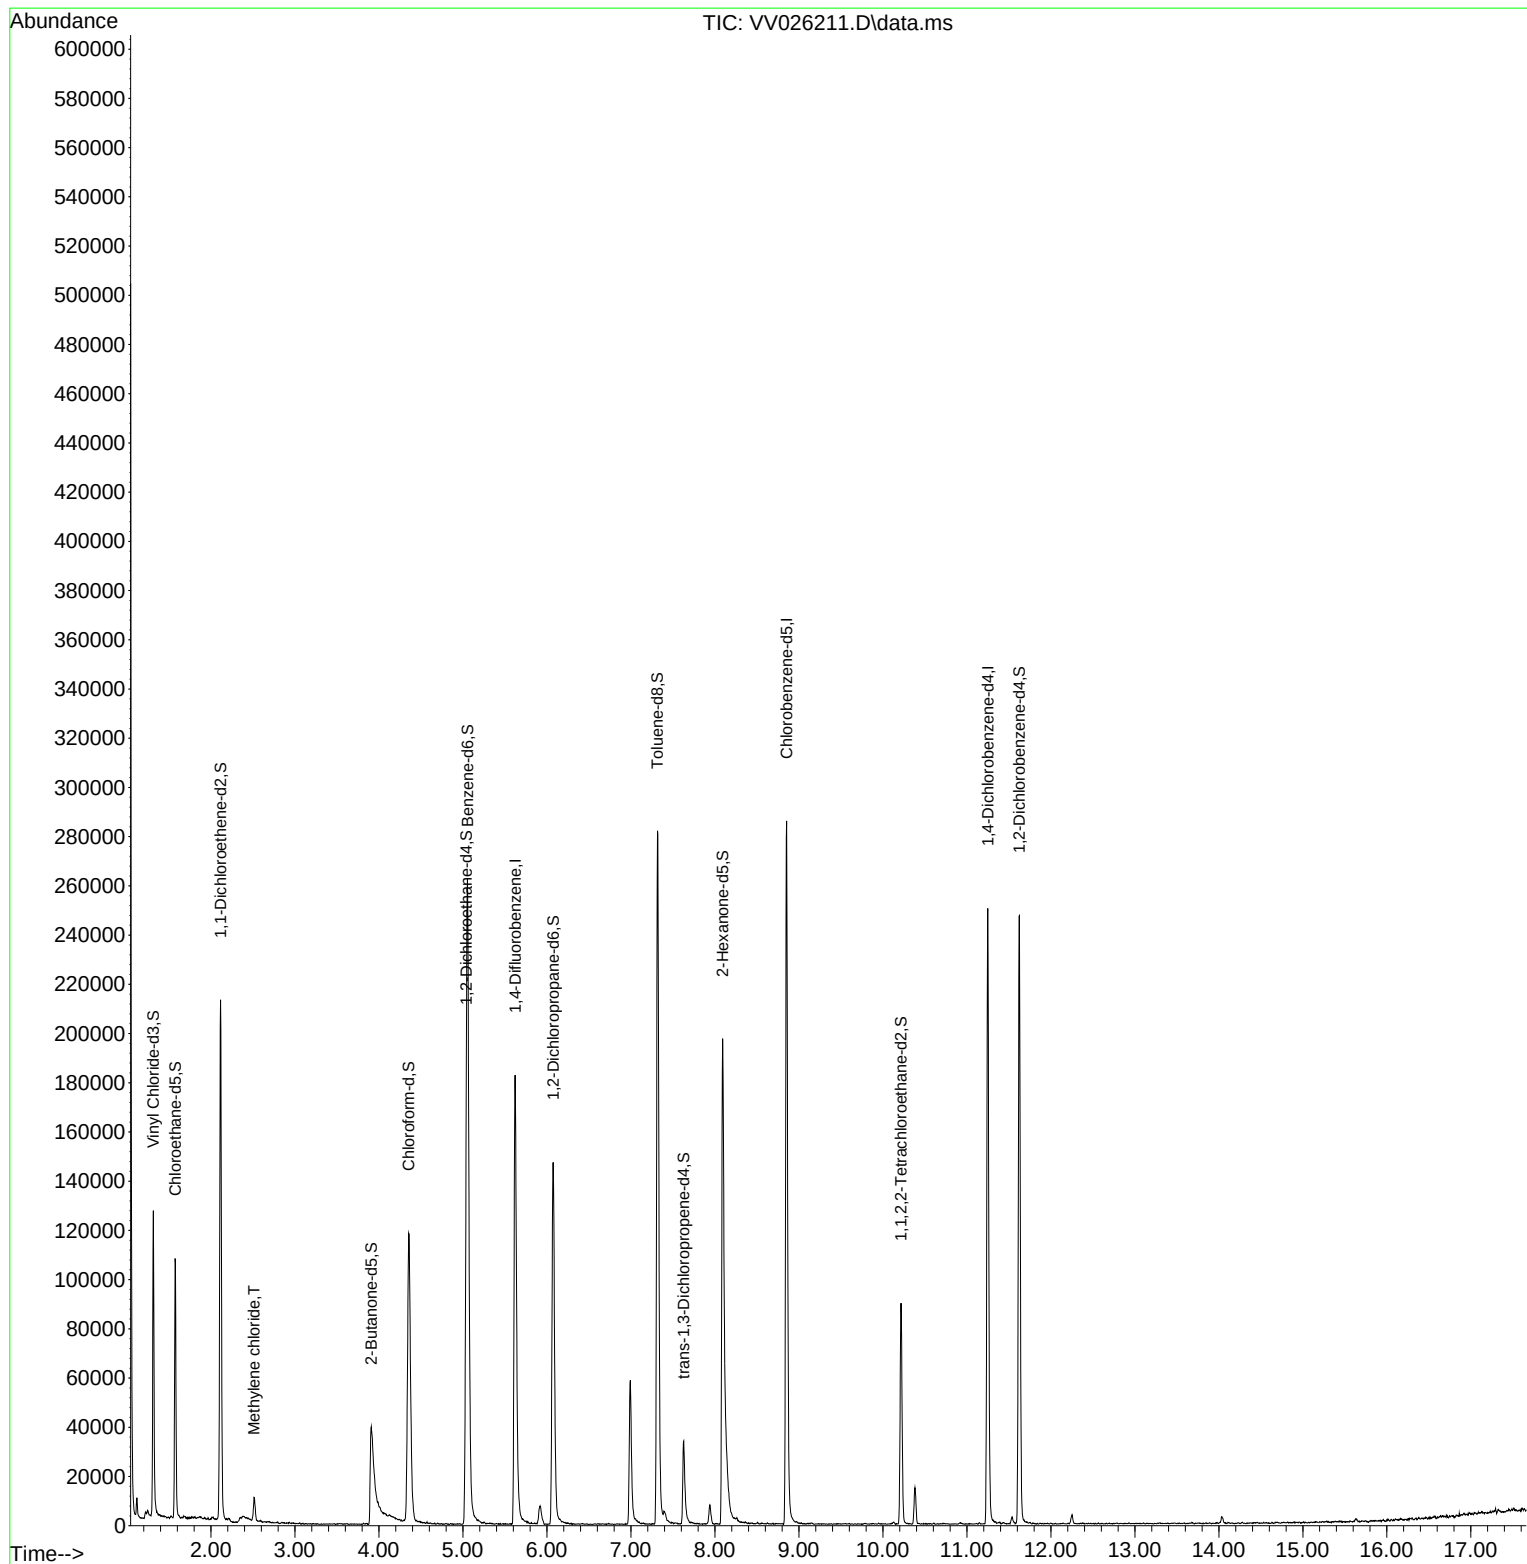

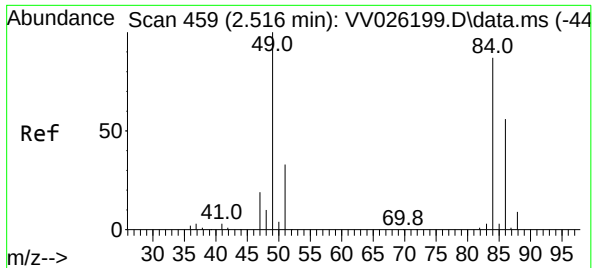

#16
Methylene chloride
Concen: 0.269 ug/L
RT: 2.513 min Scan# 4
Delta R.T. -0.003 min
Lab File: VV026211.D
Acq: 13 Jun 2022 15:58

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	3452
Ion	Ratio	Lower	Upper
84	100		
86	64.2	45.1	83.7
49	123.1	82.3	152.9

