

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026202.D
 Acq On : 13 Jun 2022 12:22
 Operator : SY/MD
 Sample : N3272-05DL 500X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B49DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026202.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	106	rVB	139517	152008	13.56%	2.290%
2	1.577	159	167	182	rBV	120404	135993	12.13%	2.048%
3	1.764	216	225	234	rVB	9689	12690	1.13%	0.191%
4	2.117	324	335	359	rVB	241277	348825	31.11%	5.254%
5	2.519	448	460	472	rBV	40680	66355	5.92%	0.999%
6	3.921	883	896	934	rBV3	44291	193123	17.22%	2.909%
7	4.362	1016	1033	1060	rBV	129155	326730	29.14%	4.921%
8	5.056	1233	1249	1279	rBV2	296950	735062	65.55%	11.072%
9	5.625	1414	1426	1446	rBV	188251	384617	34.30%	5.793%
10	5.918	1504	1517	1547	rBV	569655	1121338	100.00%	16.890%
11	6.075	1553	1566	1596	rVB	166081	347002	30.95%	5.227%
12	6.992	1841	1851	1870	rBV	68500	127083	11.33%	1.914%
13	7.320	1940	1953	1973	rBV	340658	593492	52.93%	8.940%
14	7.628	2040	2049	2072	rBV2	38123	73363	6.54%	1.105%
15	7.982	2151	2159	2170	rVB4	7393	12405	1.11%	0.187%
16	8.095	2183	2194	2236	rBV2	225009	501157	44.69%	7.549%
17	8.419	2284	2295	2312	rBV	13450	22327	1.99%	0.336%
18	8.853	2420	2430	2458	rBV	291131	482212	43.00%	7.263%
19	10.217	2840	2854	2868	rBV	103410	163436	14.58%	2.462%
20	11.249	3162	3175	3196	rBV	255750	400028	35.67%	6.025%
21	11.622	3279	3291	3313	rBV	276456	439698	39.21%	6.623%




Sum of corrected areas: 6638944

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026202.D
Acq On : 13 Jun 2022 12:22
Operator : SY/MD
Sample : N3272-05DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B49DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

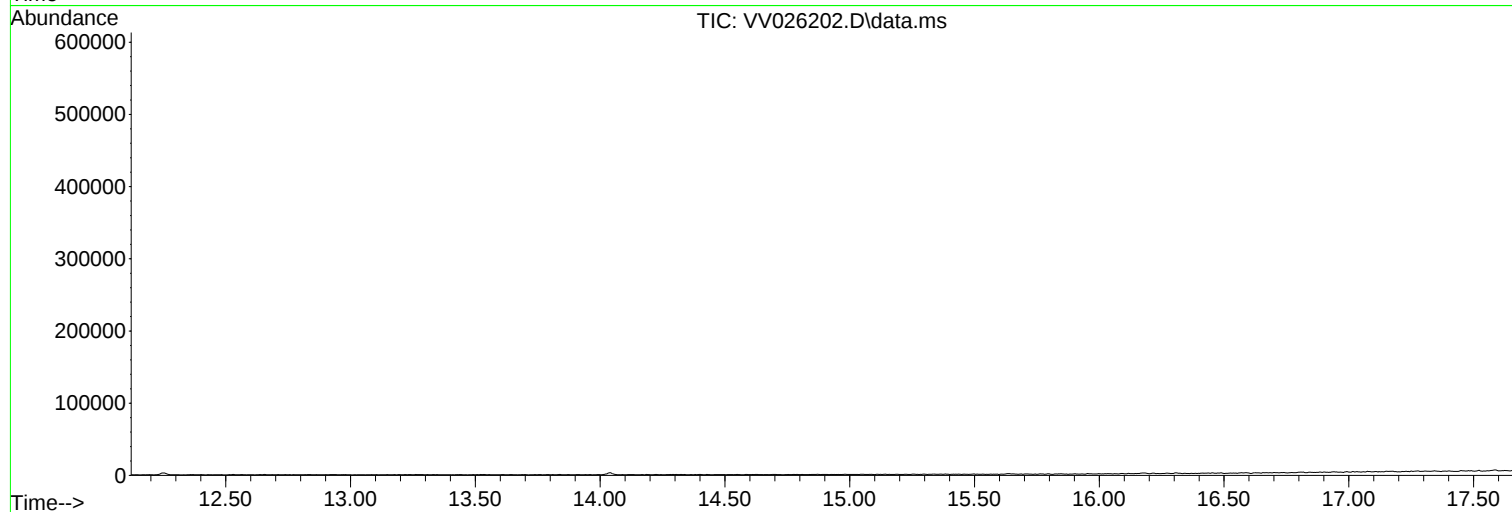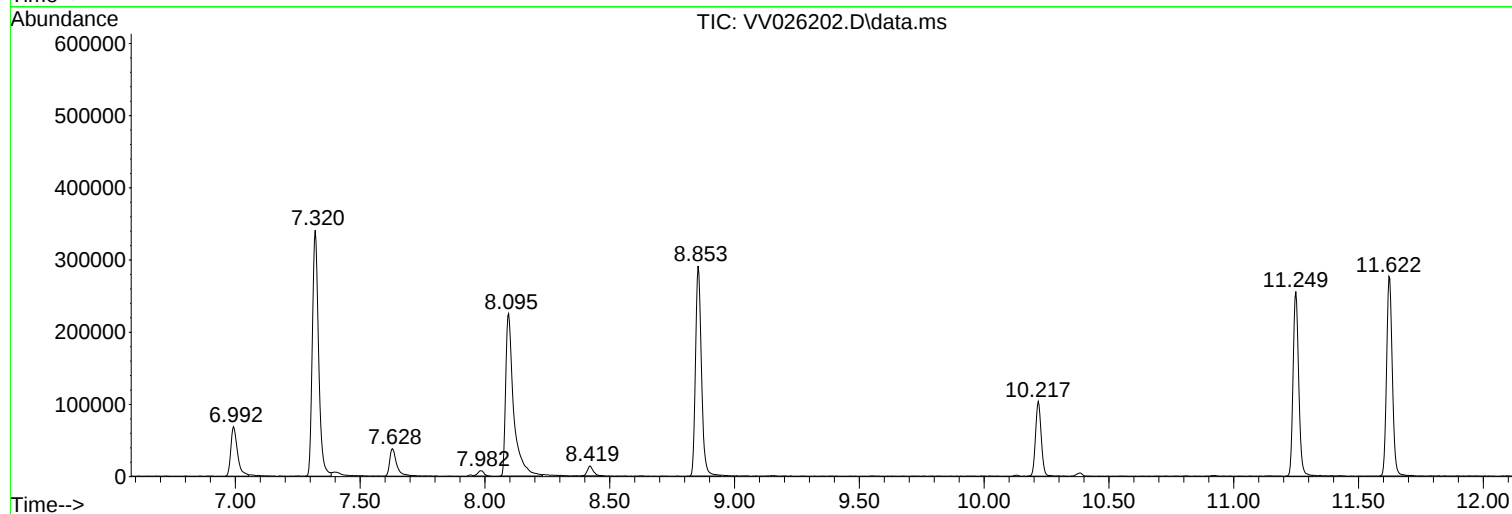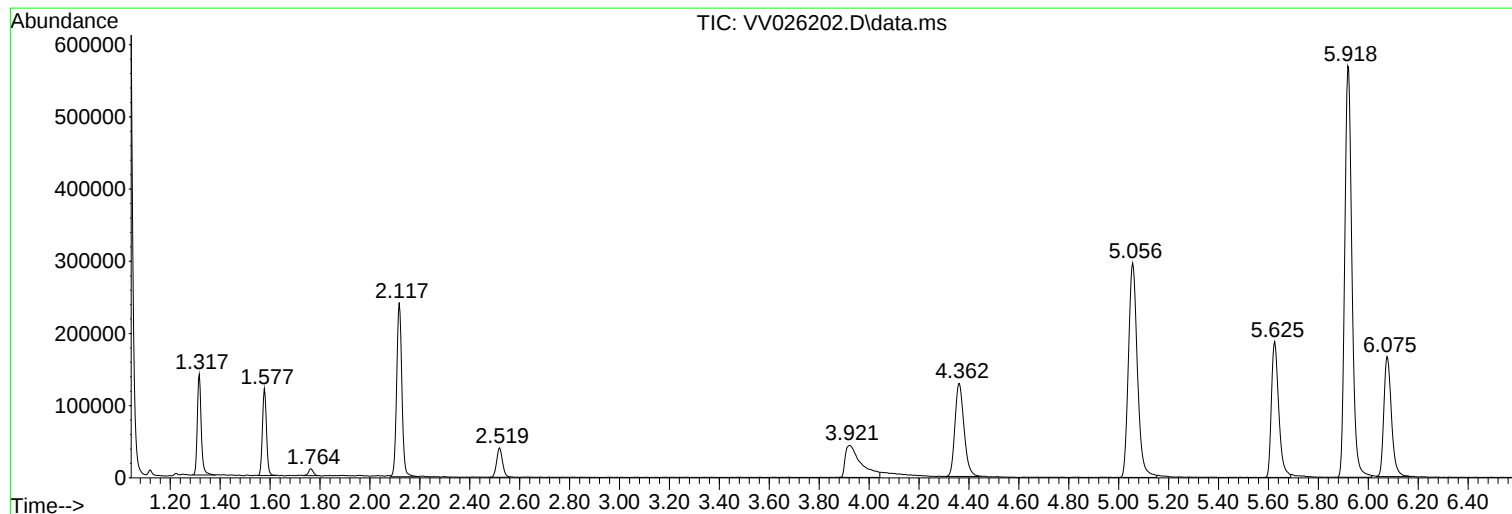

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026202.D
Acq On : 13 Jun 2022 12:22
Operator : SY/MD
Sample : N3272-05DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B49DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026202.D
Acq On : 13 Jun 2022 12:22
Operator : SY/MD
Sample : N3272-05DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B49DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc