

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026204.D
 Acq On : 13 Jun 2022 13:10
 Operator : SY/MD
 Sample : N3289-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DS8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	100	rBV	133240	145718	20.80%	2.703%
2	1.577	157	167	181	rBV	110437	126592	18.07%	2.349%
3	2.117	324	335	353	rVB	227576	331094	47.27%	6.143%
4	3.918	885	895	933	rBV	39512	174828	24.96%	3.243%
5	4.355	1011	1031	1057	rBV	125824	318524	45.48%	5.909%
6	5.053	1231	1248	1283	rBV2	284442	700427	100.00%	12.994%
7	5.622	1413	1425	1456	rBV	211941	434569	62.04%	8.062%
8	5.918	1507	1517	1534	rBV9	7391	17078	2.44%	0.317%
9	6.075	1553	1566	1593	rBV	159711	333655	47.64%	6.190%
10	6.992	1840	1851	1880	rBV	66073	126244	18.02%	2.342%
11	7.320	1938	1953	1973	rBV	314628	561407	80.15%	10.415%
12	7.628	2039	2049	2071	rBV	37090	71133	10.16%	1.320%
13	7.947	2133	2148	2158	rBV3	6256	11955	1.71%	0.222%
14	8.095	2184	2194	2232	rBV	223158	472686	67.49%	8.769%
15	8.853	2415	2430	2450	rBV	324463	530626	75.76%	9.844%
16	10.217	2843	2854	2873	rBV	97605	156193	22.30%	2.898%
17	10.384	2893	2906	2916	rVB2	12656	20194	2.88%	0.375%
18	11.249	3164	3175	3197	rBV	284699	438145	62.55%	8.129%
19	11.622	3280	3291	3310	rBV	263755	419127	59.84%	7.776%




Sum of corrected areas: 5390195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026204.D
Acq On : 13 Jun 2022 13:10
Operator : SY/MD
Sample : N3289-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

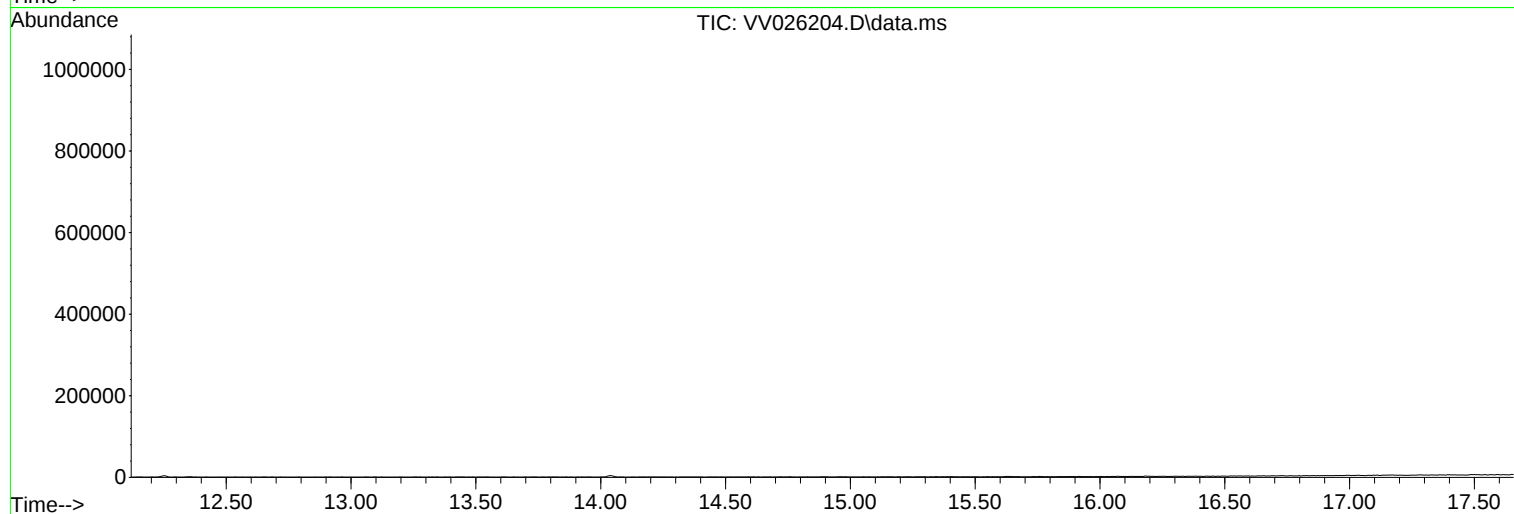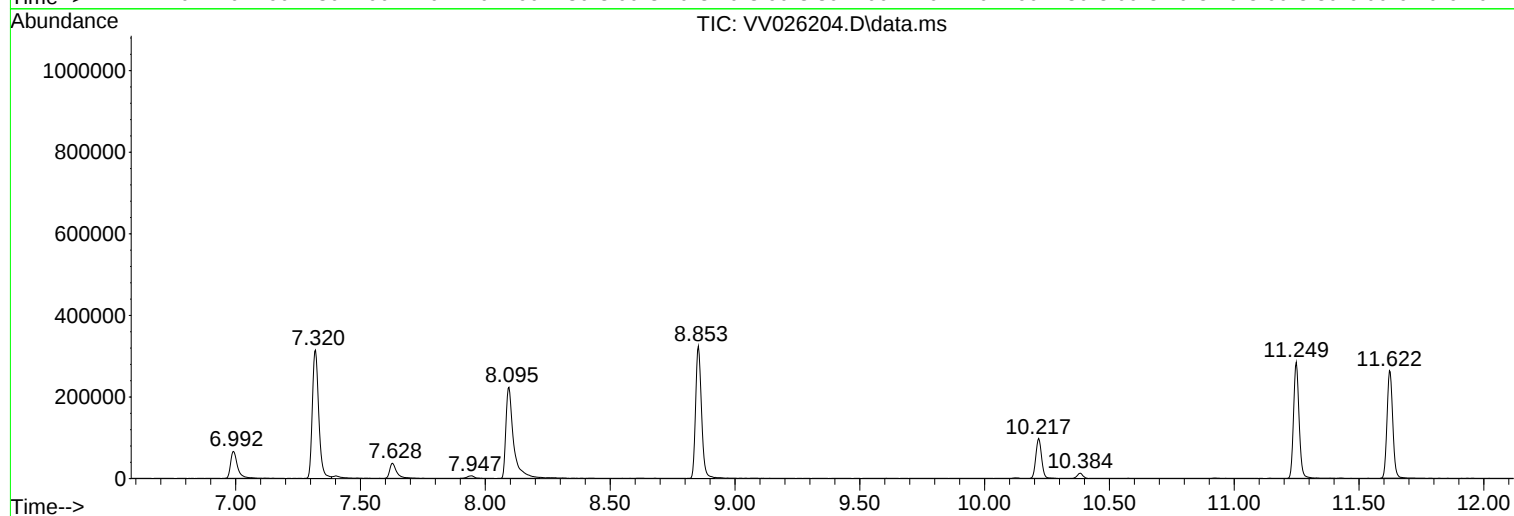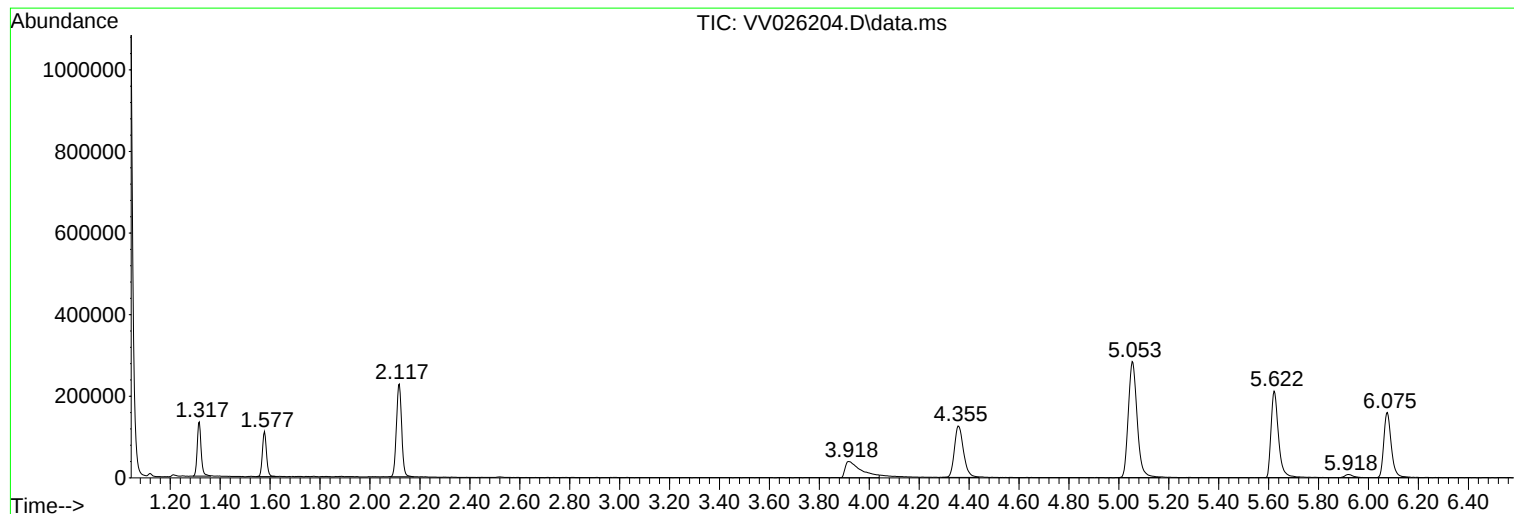

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026204.D
Acq On : 13 Jun 2022 13:10
Operator : SY/MD
Sample : N3289-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026204.D
Acq On : 13 Jun 2022 13:10
Operator : SY/MD
Sample : N3289-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc