

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026205.D
 Acq On : 13 Jun 2022 13:34
 Operator : SY/MD
 Sample : N3289-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DT1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	20	24	35	rVB2	8480	9408	1.32%	0.172%
2	1.317	78	86	102	rVB	132085	142065	19.96%	2.594%
3	1.577	159	167	185	rVB	114893	132036	18.55%	2.411%
4	2.118	323	335	355	rBV	228734	330068	46.37%	6.026%
5	3.915	884	894	927	rBV	41152	154486	21.70%	2.820%
6	4.359	1013	1032	1060	rBV	128495	319942	44.95%	5.841%
7	5.053	1232	1248	1278	rBV3	285410	711827	100.00%	12.996%
8	5.622	1414	1425	1453	rBV	219351	447172	62.82%	8.164%
9	5.918	1506	1517	1534	rVB7	7593	16783	2.36%	0.306%
10	6.076	1552	1566	1593	rBV	158751	335208	47.09%	6.120%
11	6.992	1840	1851	1874	rBV	65644	123791	17.39%	2.260%
12	7.320	1938	1953	1973	rBV	324020	565509	79.44%	10.325%
13	7.629	2038	2049	2074	rBV	37016	71012	9.98%	1.296%
14	7.940	2135	2146	2158	rBV2	8933	16044	2.25%	0.293%
15	8.092	2183	2193	2235	rBV	216395	487009	68.42%	8.891%
16	8.854	2418	2430	2464	rBV	334793	553028	77.69%	10.097%
17	10.217	2841	2854	2869	rBV	99219	158877	22.32%	2.901%
18	10.384	2895	2906	2916	rBV3	15279	24645	3.46%	0.450%
19	11.249	3163	3175	3198	rBV	289371	451622	63.45%	8.245%
20	11.622	3279	3291	3313	rBV	267854	426778	59.96%	7.792%




Sum of corrected areas: 5477310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026205.D
Acq On : 13 Jun 2022 13:34
Operator : SY/MD
Sample : N3289-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

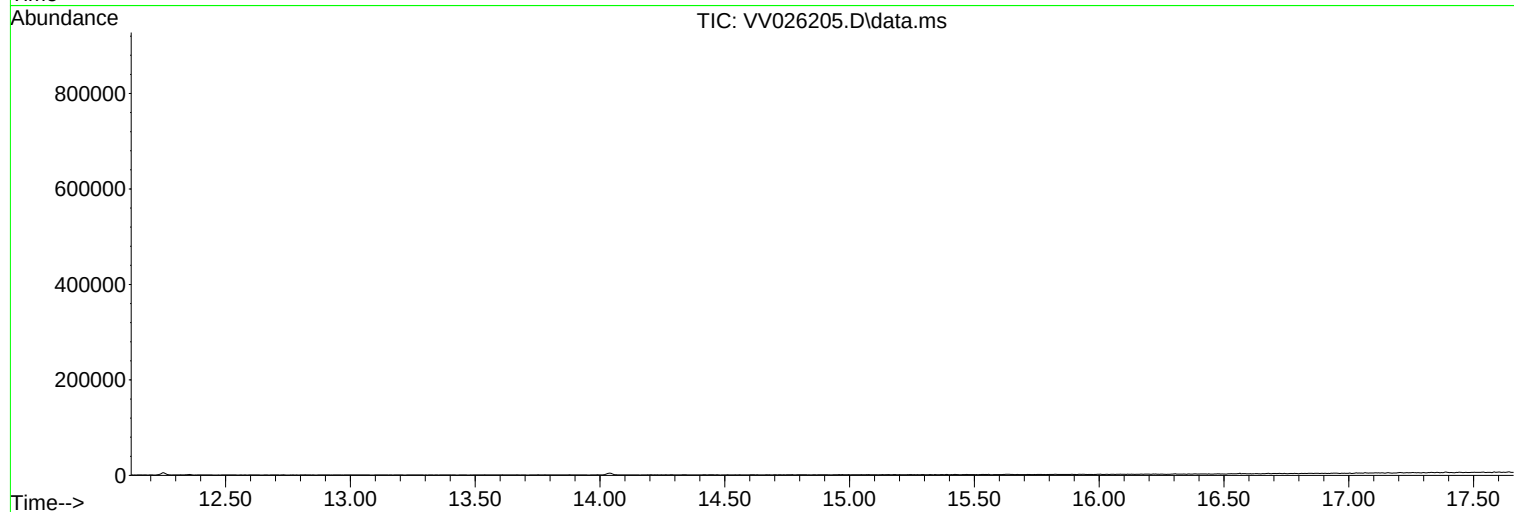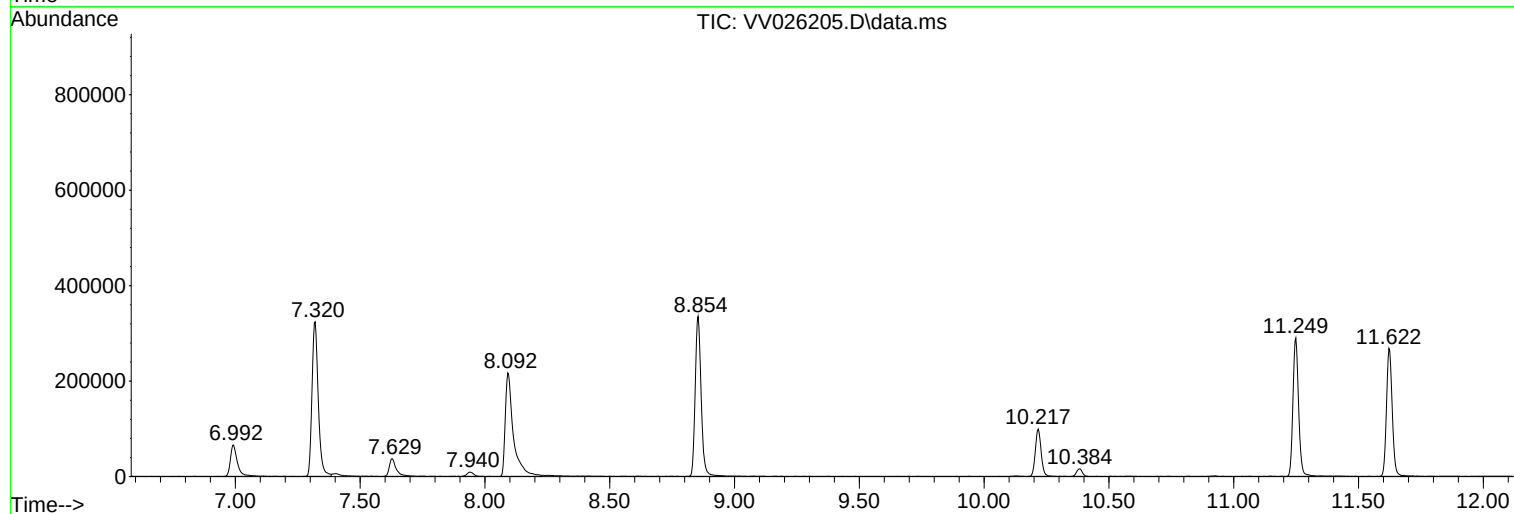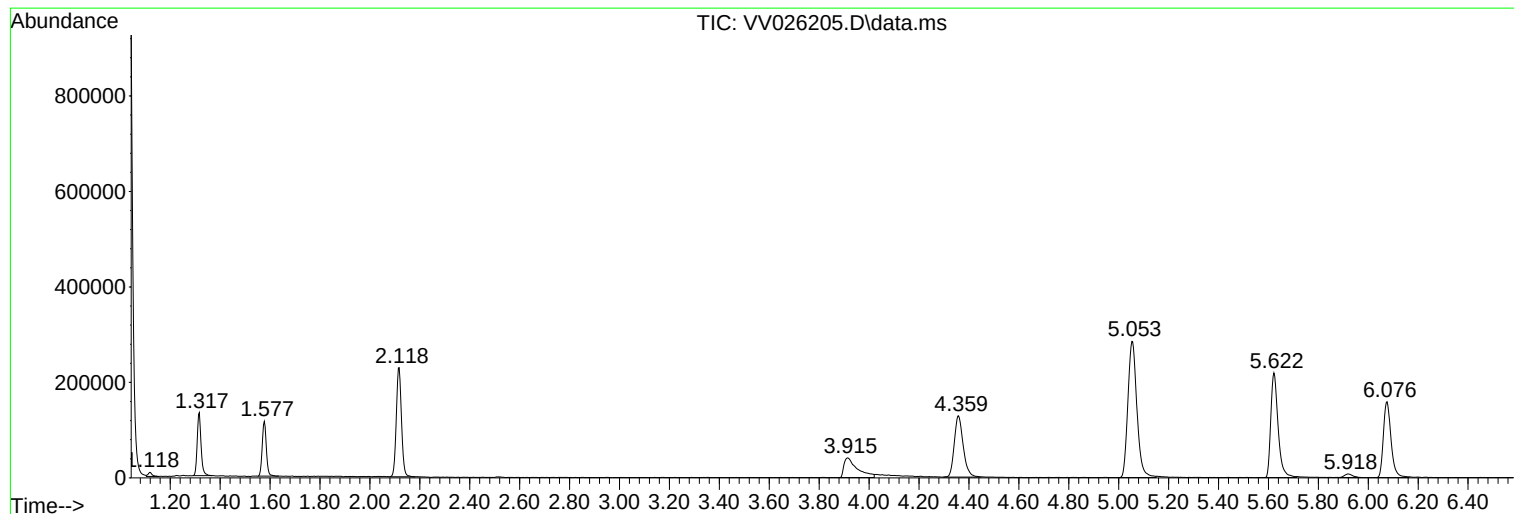

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026205.D
Acq On : 13 Jun 2022 13:34
Operator : SY/MD
Sample : N3289-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026205.D
Acq On : 13 Jun 2022 13:34
Operator : SY/MD
Sample : N3289-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc