

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026206.D
 Acq On : 13 Jun 2022 13:58
 Operator : SY/MD
 Sample : N3289-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DT2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	101	rBV	138655	143042	19.89%	2.610%
2	1.577	159	167	180	rVB	116102	131352	18.26%	2.396%
3	2.118	321	335	351	rBV	229444	329856	45.86%	6.018%
4	3.912	881	893	923	rBV	42856	157134	21.84%	2.867%
5	4.359	1015	1032	1061	rBV	127921	333785	46.40%	6.089%
6	5.056	1233	1249	1279	rBV2	288057	719337	100.00%	13.123%
7	5.622	1414	1425	1451	rBV	211198	429889	59.76%	7.843%
8	5.924	1506	1519	1536	rBV6	25918	57278	7.96%	1.045%
9	6.076	1550	1566	1594	rBV	160583	339446	47.19%	6.193%
10	6.992	1841	1851	1885	rBV2	63272	123795	17.21%	2.258%
11	7.320	1940	1953	1973	rBV	318934	563920	78.39%	10.288%
12	7.629	2037	2049	2072	rBV	37624	71071	9.88%	1.297%
13	7.940	2134	2146	2156	rBV	9241	16226	2.26%	0.296%
14	8.092	2183	2193	2233	rBV2	216332	489649	68.07%	8.933%
15	8.854	2418	2430	2453	rBV	323415	528977	73.54%	9.650%
16	10.217	2843	2854	2869	rBV	99577	159073	22.11%	2.902%
17	10.384	2896	2906	2918	rVB3	17052	28003	3.89%	0.511%
18	11.249	3164	3175	3199	rBV	280739	433434	60.25%	7.907%
19	11.622	3279	3291	3313	rBV	266555	426208	59.25%	7.775%




Sum of corrected areas: 5481475

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026206.D
Acq On : 13 Jun 2022 13:58
Operator : SY/MD
Sample : N3289-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

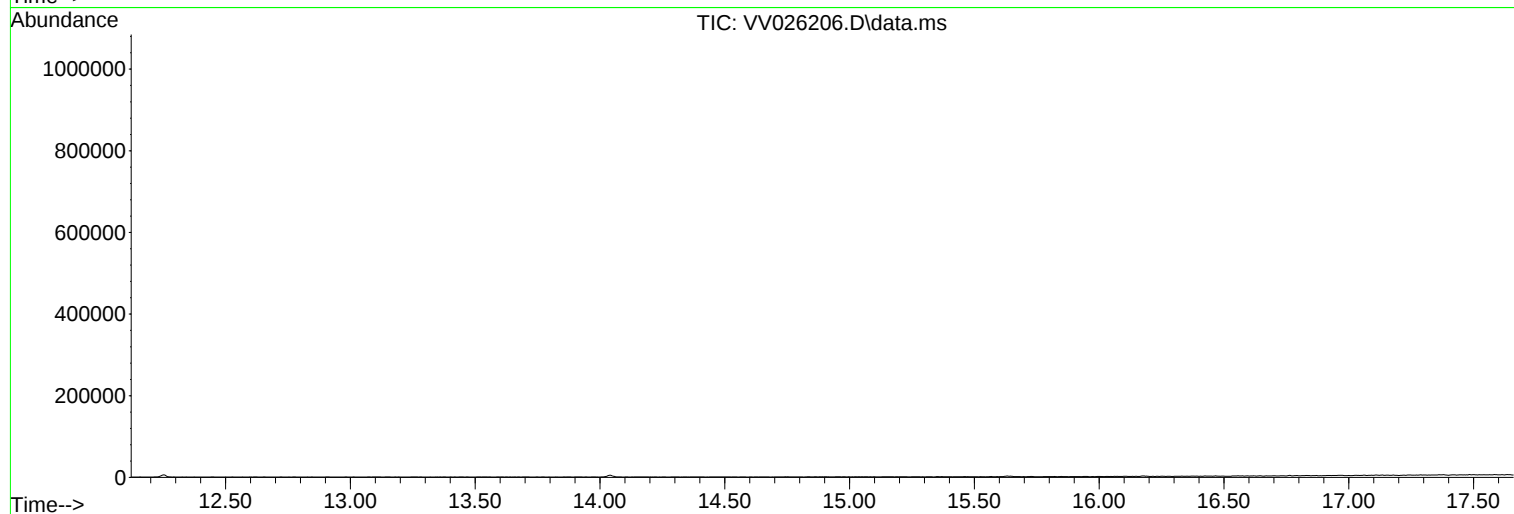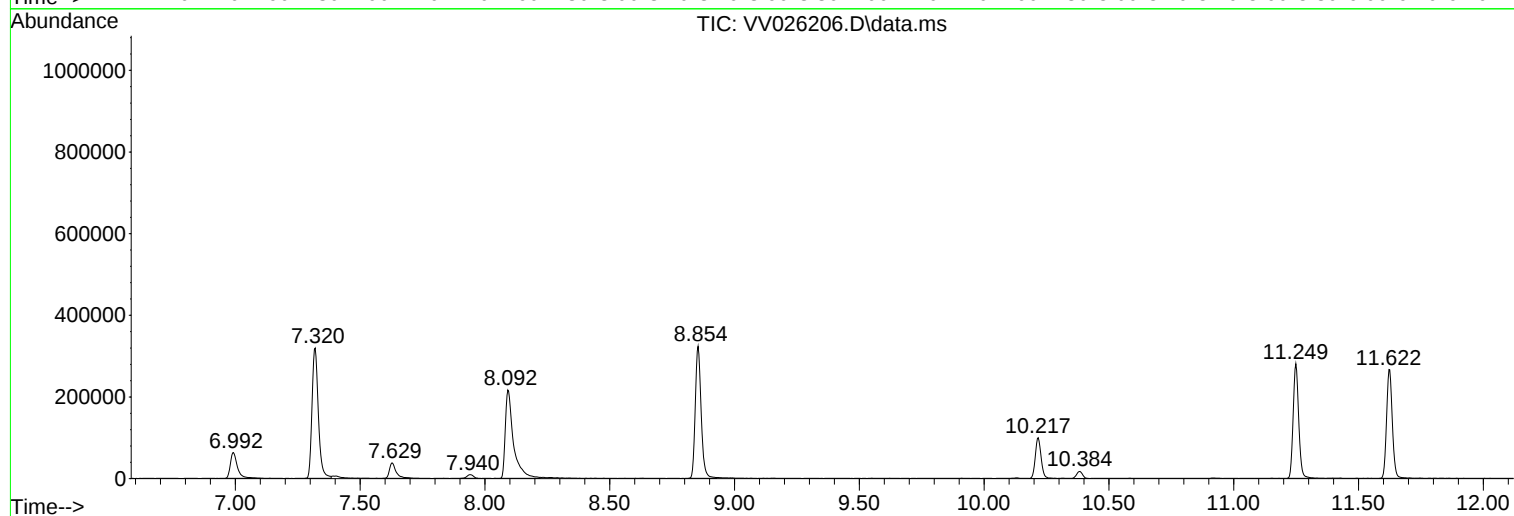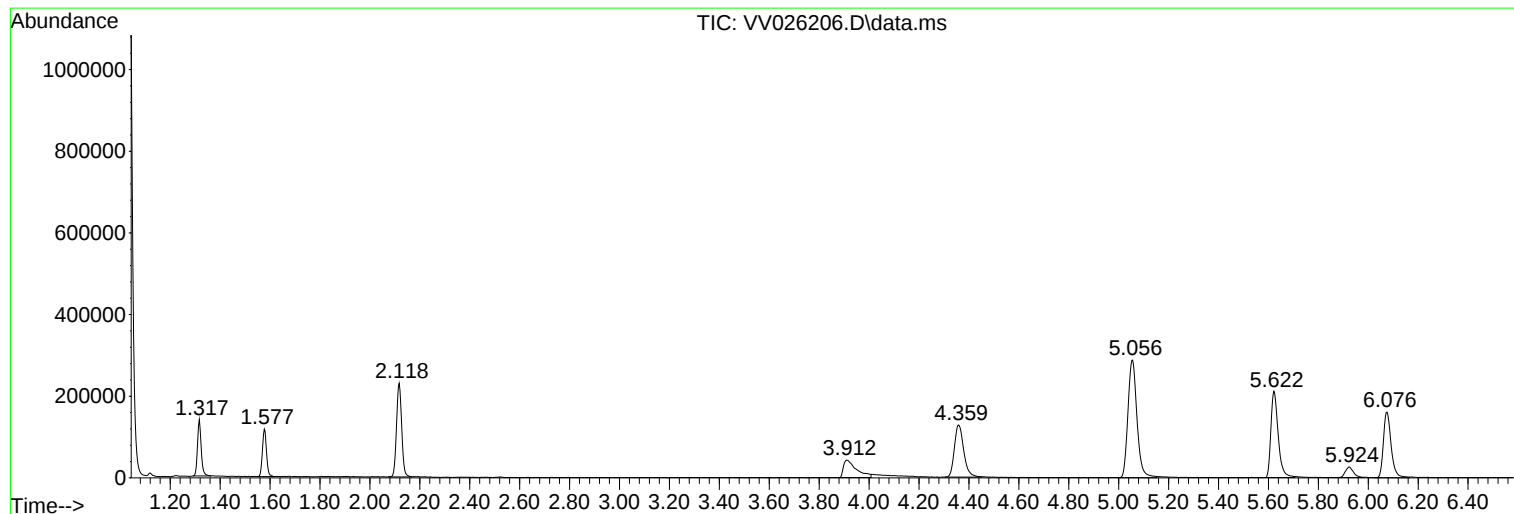

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026206.D
Acq On : 13 Jun 2022 13:58
Operator : SY/MD
Sample : N3289-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026206.D
Acq On : 13 Jun 2022 13:58
Operator : SY/MD
Sample : N3289-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
