

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026209.D
 Acq On : 13 Jun 2022 15:10
 Operator : SY/MD
 Sample : N3289-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DW6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	100	rBV	145481	159072	20.16%	2.773%
2	1.577	159	167	182	rBV	127418	145564	18.45%	2.538%
3	2.118	324	335	353	rBV	253156	362157	45.91%	6.314%
4	3.909	880	892	917	rBV	48058	159454	20.21%	2.780%
5	4.359	1016	1032	1060	rBV2	143113	383436	48.61%	6.685%
6	5.053	1232	1248	1279	rBV2	317098	788873	100.00%	13.753%
7	5.622	1414	1425	1454	rBV2	190911	389211	49.34%	6.785%
8	5.921	1507	1518	1533	rVB5	8817	19619	2.49%	0.342%
9	6.076	1545	1566	1588	rBV	179290	373269	47.32%	6.507%
10	6.992	1839	1851	1870	rBV	72225	136073	17.25%	2.372%
11	7.320	1940	1953	1972	rBV	353641	625254	79.26%	10.900%
12	7.625	2038	2048	2070	rBV	41253	76719	9.73%	1.337%
13	7.940	2138	2146	2156	rVB3	6285	11415	1.45%	0.199%
14	8.092	2182	2193	2227	rBV	244485	547513	69.40%	9.545%
15	8.854	2414	2430	2454	rBV	294192	487337	61.78%	8.496%
16	10.217	2842	2854	2872	rBV	111445	175099	22.20%	3.053%
17	10.381	2897	2905	2917	rVB3	13841	22409	2.84%	0.391%
18	11.249	3164	3175	3198	rBV	258952	403664	51.17%	7.037%
19	11.622	3280	3291	3315	rBV	297052	469880	59.56%	8.192%




Sum of corrected areas: 5736018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026209.D
Acq On : 13 Jun 2022 15:10
Operator : SY/MD
Sample : N3289-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

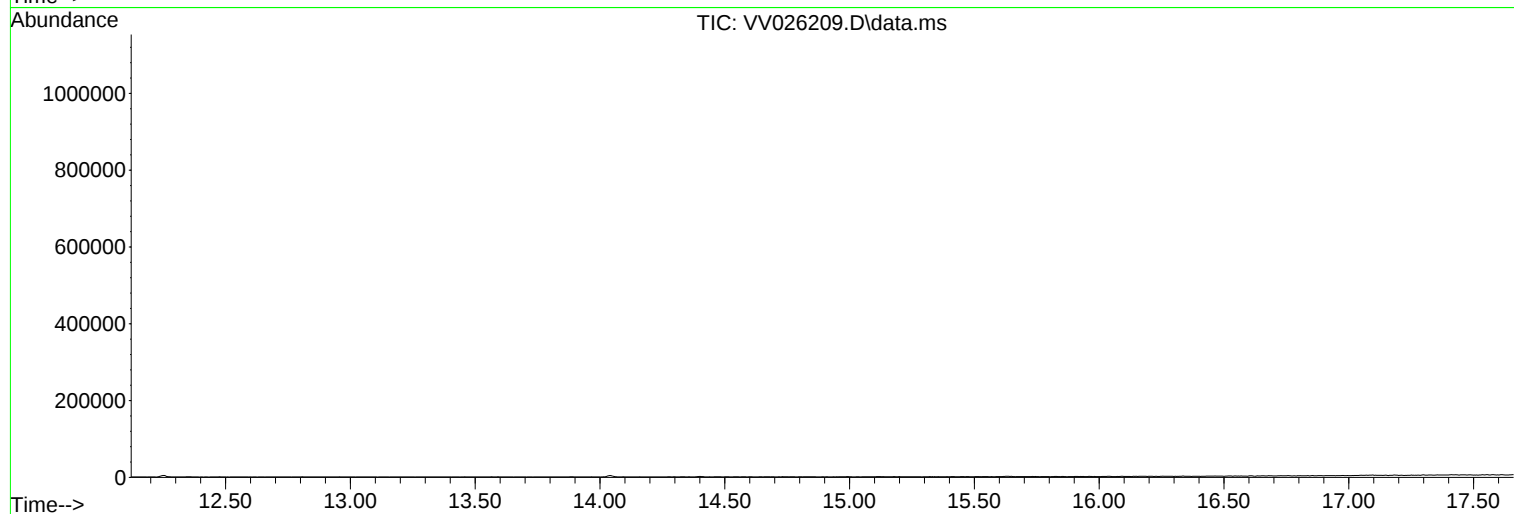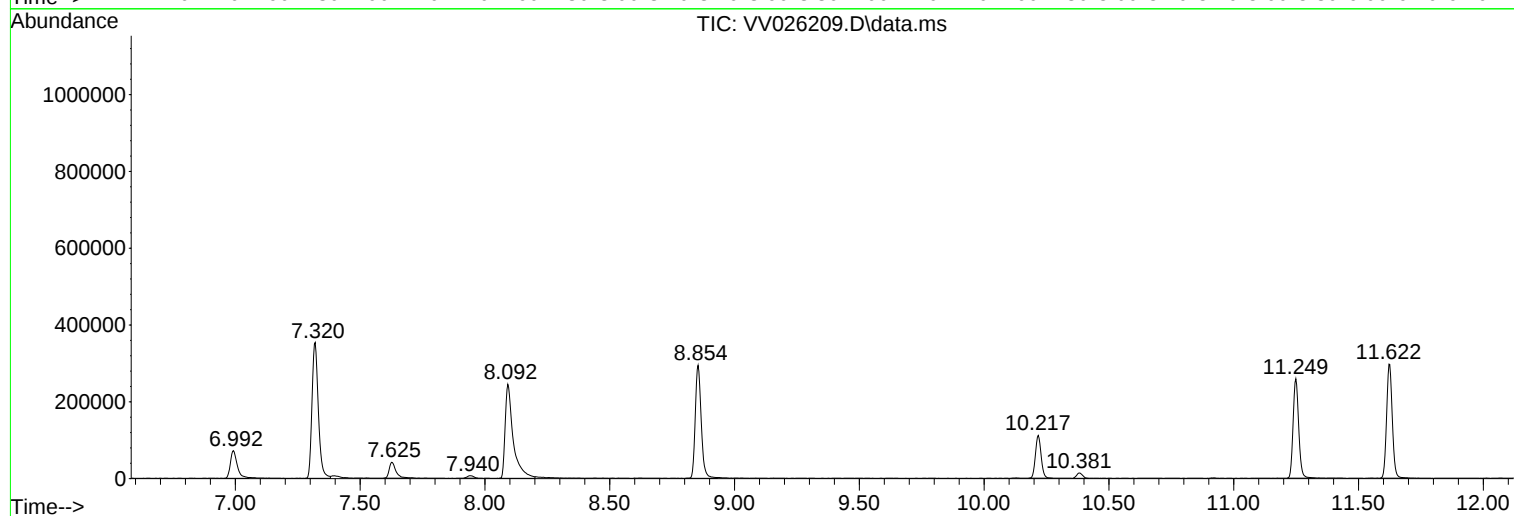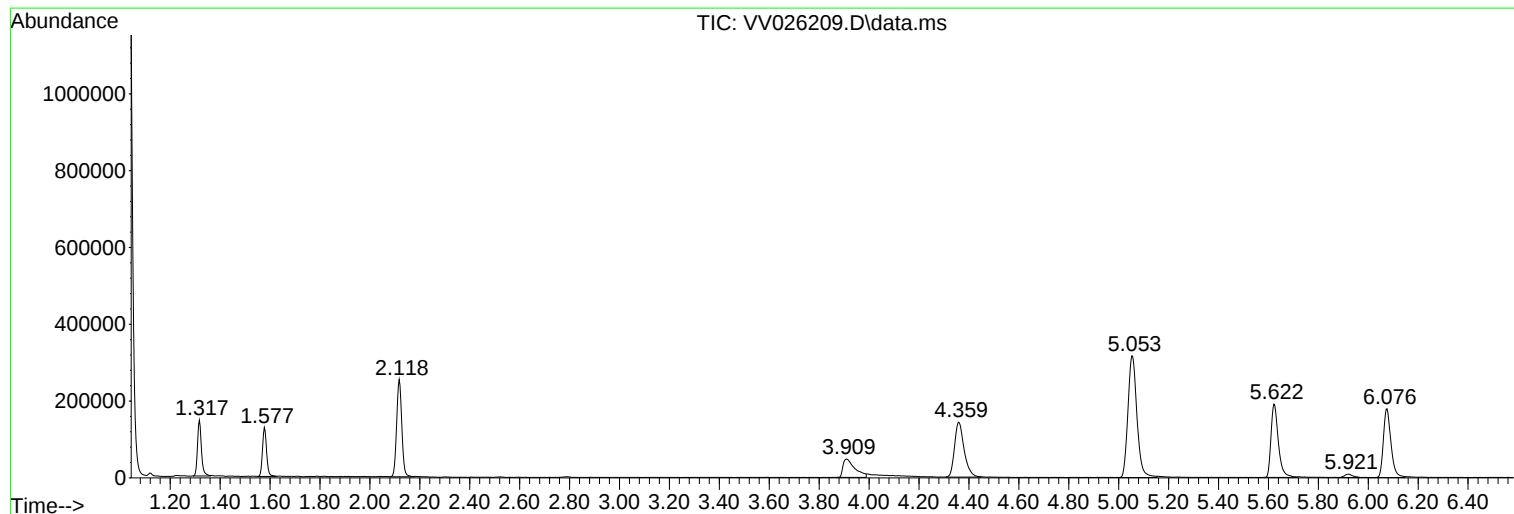

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026209.D
Acq On : 13 Jun 2022 15:10
Operator : SY/MD
Sample : N3289-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026209.D
Acq On : 13 Jun 2022 15:10
Operator : SY/MD
Sample : N3289-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc