

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026214.D
 Acq On : 13 Jun 2022 17:10
 Operator : SY/MD
 Sample : N3272-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B59

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	76	86	98	rBV	135920	149939	6.08%	1.662%
2	1.577	158	167	179	rBV	115954	134058	5.43%	1.486%
3	1.761	215	224	240	rVB	182071	235388	9.54%	2.610%
4	2.118	324	335	353	rVB	228148	329840	13.37%	3.657%
5	3.912	882	893	926	rBV	47378	173879	7.05%	1.928%
6	4.359	1012	1032	1055	rBV2	129696	328444	13.31%	3.641%
7	5.053	1232	1248	1280	rBV3	287332	708720	28.72%	7.857%
8	5.622	1414	1425	1451	rBV2	180199	371697	15.06%	4.121%
9	5.915	1498	1516	1550	rBV	1264727	2467327	100.00%	27.354%
10	6.072	1553	1565	1592	rVB	167532	345804	14.02%	3.834%
11	6.992	1840	1851	1872	rBV	64009	123499	5.01%	1.369%
12	7.320	1939	1953	1974	rBV	322003	574716	23.29%	6.372%
13	7.629	2039	2049	2069	rBV2	35369	68332	2.77%	0.758%
14	7.976	2135	2157	2181	rBV	591743	1010390	40.95%	11.202%
15	8.092	2183	2193	2232	rVV	238680	508716	20.62%	5.640%
16	8.854	2419	2430	2451	rBV	279430	459774	18.63%	5.097%
17	10.217	2843	2854	2870	rBV	102744	164097	6.65%	1.819%
18	10.381	2895	2905	2921	rVB2	22190	35331	1.43%	0.392%
19	11.249	3164	3175	3195	rBV	242074	375880	15.23%	4.167%
20	11.622	3280	3291	3308	rBV	269064	425715	17.25%	4.720%
21	16.178	4699	4708	4719	rBV5	19969	28372	1.15%	0.315%




Sum of corrected areas: 9019918

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026214.D
Acq On : 13 Jun 2022 17:10
Operator : SY/MD
Sample : N3272-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

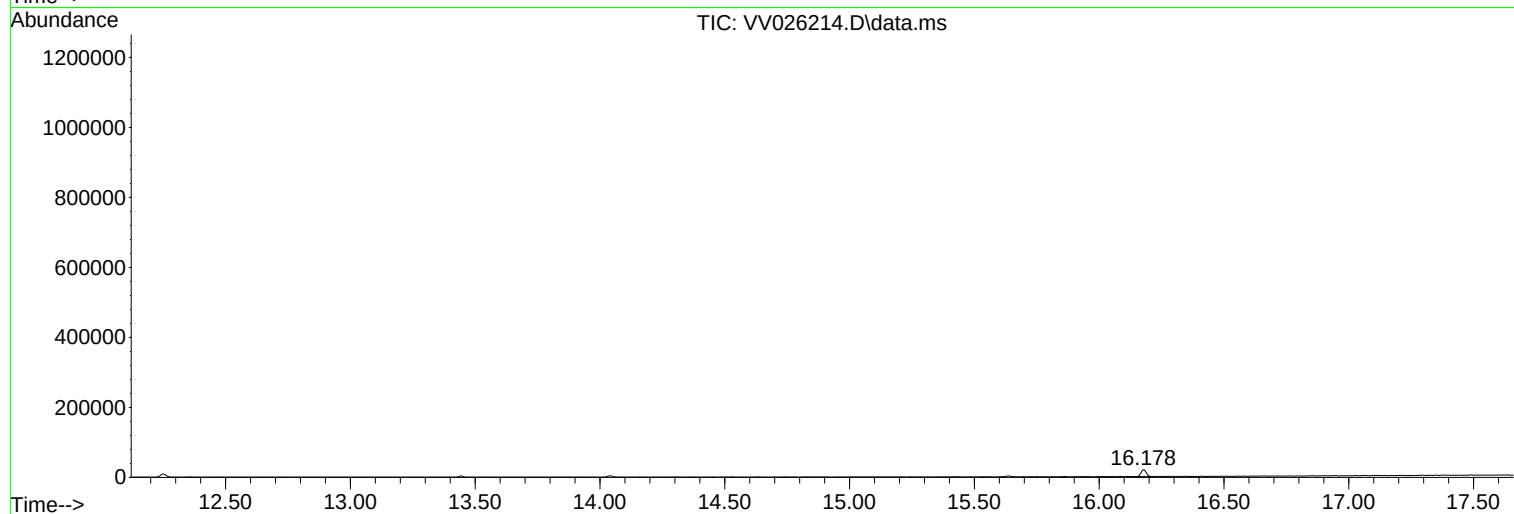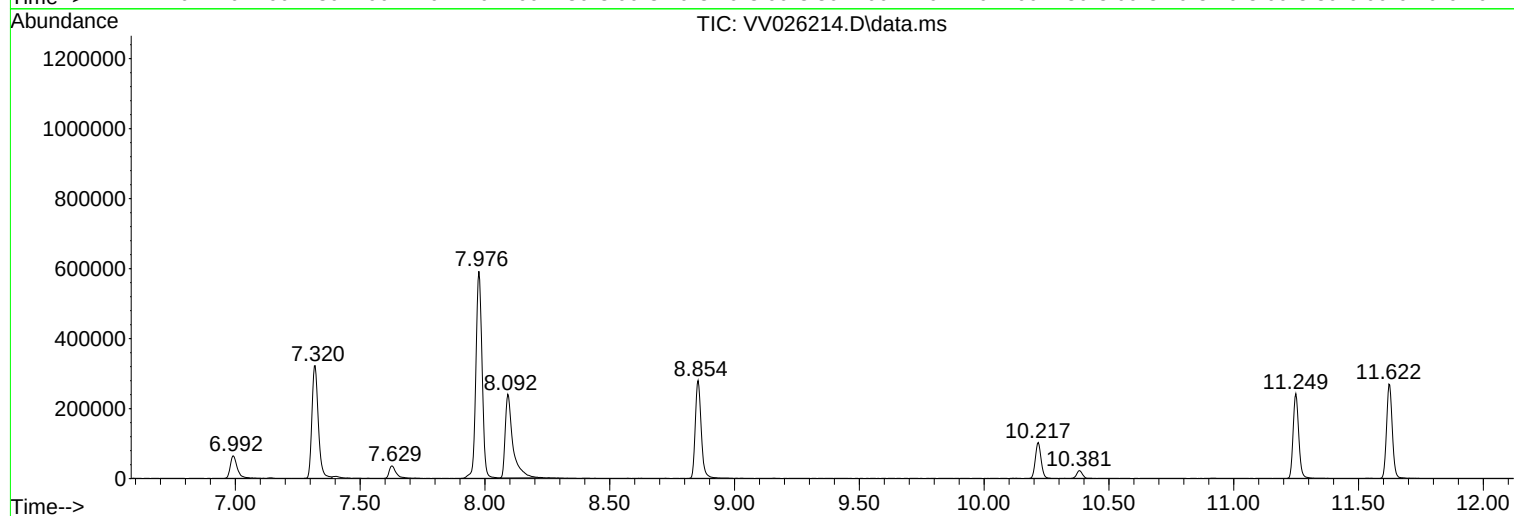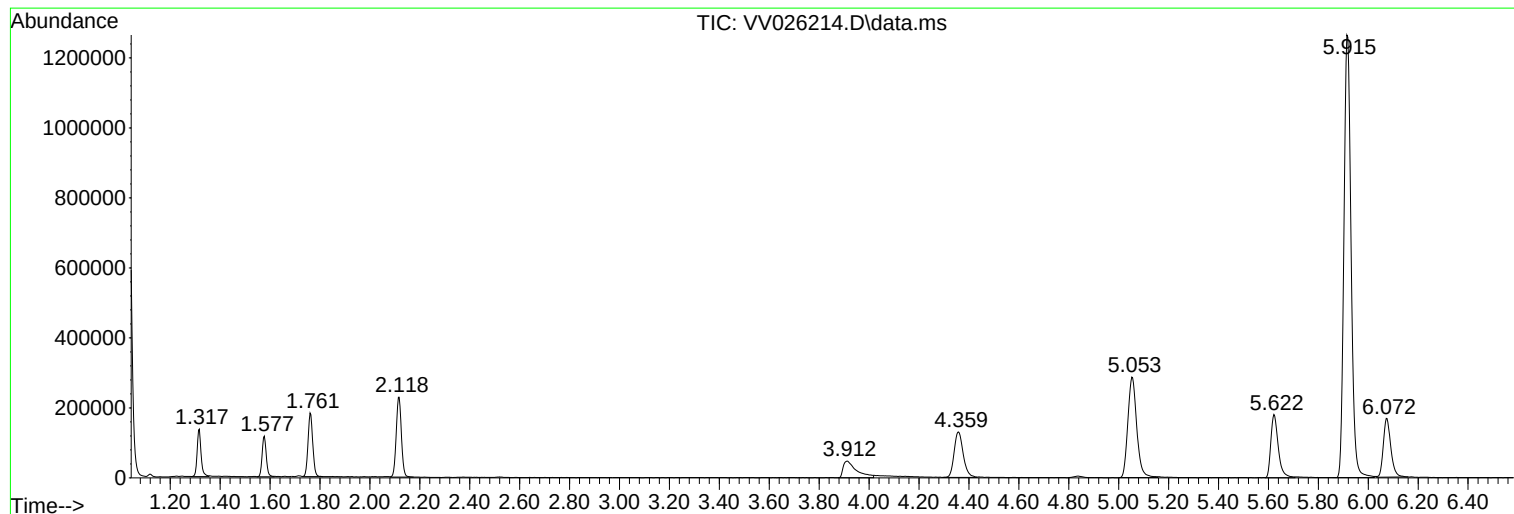

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026214.D
Acq On : 13 Jun 2022 17:10
Operator : SY/MD
Sample : N3272-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
Data File : VV026214.D
Acq On : 13 Jun 2022 17:10
Operator : SY/MD
Sample : N3272-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
