


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061322\
 Data File : VV026198.D
 Acq On : 13 Jun 2022 08:44
 Operator : SY/MD
 Sample : BFB327
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB327

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061222WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jun 14 02:36:38 2022

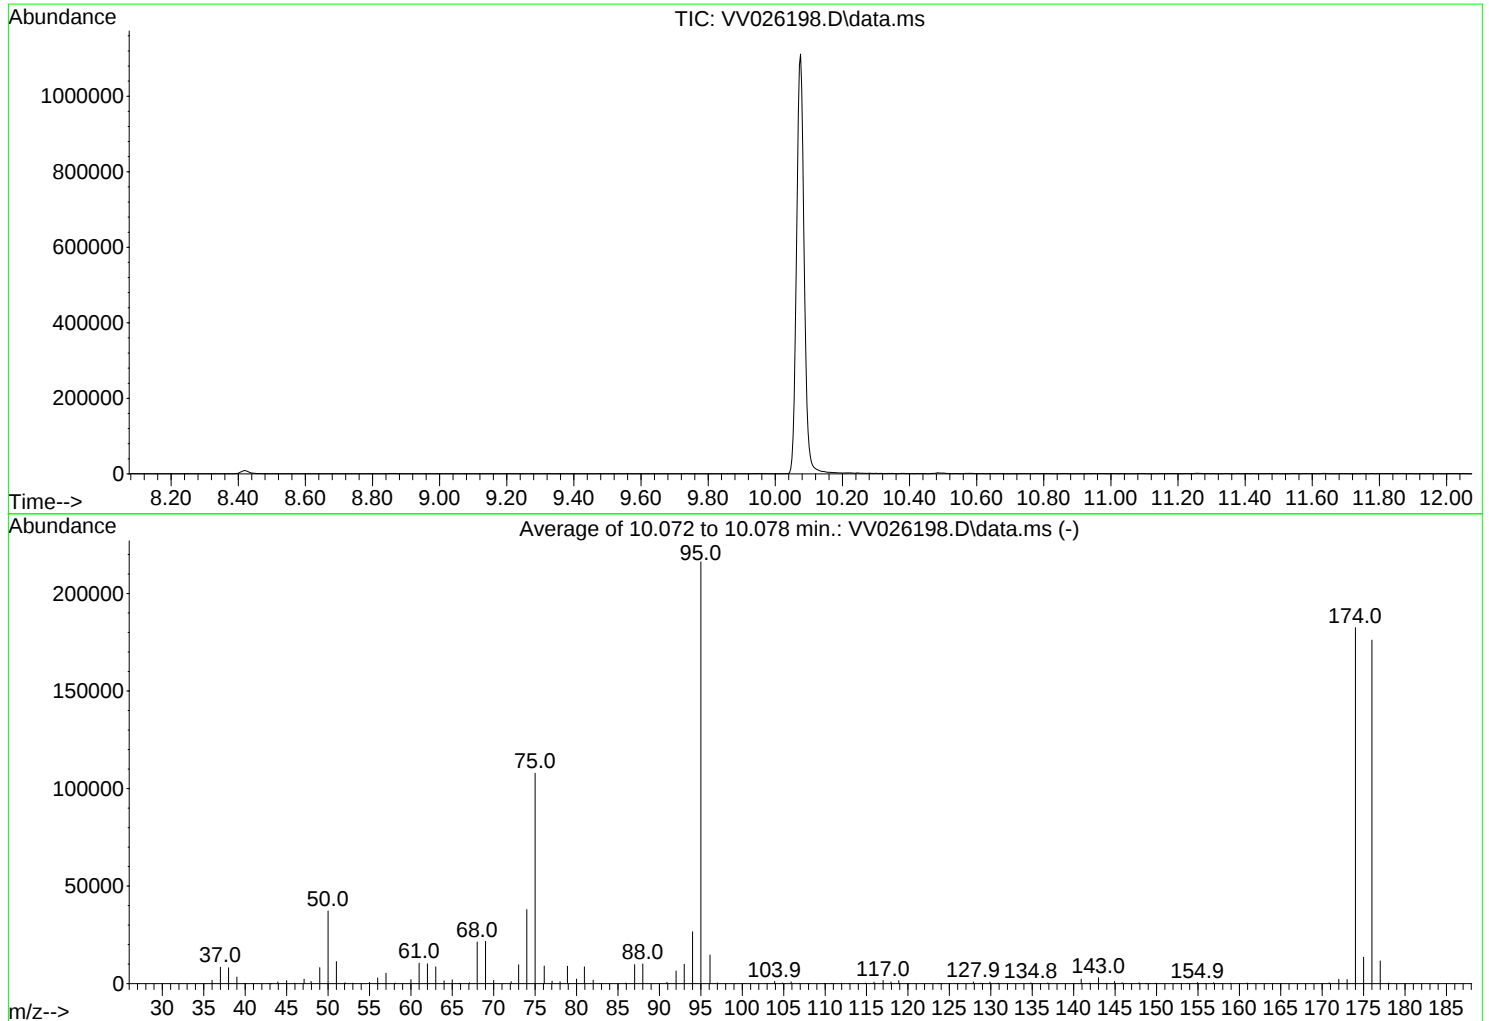

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	37237	PASS
75	95	30	80	49.9	107859	PASS
95	95	100	100	100.0	216213	PASS
96	95	5	9	6.8	14657	PASS
173	174	0.00	2	1.2	2162	PASS
174	95	50	120	84.4	182464	PASS
175	174	5	9	7.4	13567	PASS
176	174	95	105	96.5	176064	PASS
177	176	5	10	6.6	11665	PASS

m/z	Abundance
39.90	297.0
43.90	388.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	1766.0
37.00	8528.0
38.00	8376.0
39.00	3613.0
39.90	526.0
42.80	108.0
44.00	1242.0
45.00	1604.0
45.90	301.0
47.10	2236.0
48.00	1191.0
49.00	8281.0
50.00	38120.0
51.00	11339.0
52.10	470.0
52.90	344.0
54.00	211.0
55.00	580.0
56.00	3001.0
57.00	5285.0
58.10	305.0
60.00	2120.0
61.00	10666.0
62.00	10195.0
63.00	8609.0
64.00	1536.0
65.00	2105.0
65.90	267.0
67.10	512.0
68.00	21632.0
69.00	22136.0
70.00	1760.0
72.10	1083.0
73.00	10238.0
74.00	38608.0
75.00	109808.0
76.10	9196.0
77.00	1387.0
78.10	1025.0
78.90	9299.0
80.00	2417.0
80.90	8978.0
82.00	1744.0
82.80	155.0
83.10	152.0
86.00	351.0
87.00	9770.0
88.00	10159.0
90.90	732.0
92.00	6531.0
93.00	10146.0
94.00	27432.0
95.00	216704.0
96.10	15108.0
97.00	503.0
103.00	133.0
103.90	1135.0
104.80	321.0
105.90	958.0
106.90	172.0
108.10	155.0
110.00	145.0
110.80	207.0
111.90	239.0
113.00	191.0
114.90	357.0
115.90	852.0
117.00	1758.0
118.00	868.0
118.90	1558.0
123.70	104.0
124.00	107.0
125.90	115.0
127.90	842.0
128.80	330.0
129.90	793.0
130.90	314.0
134.80	466.0
136.90	436.0
140.00	166.0
140.90	2378.0
141.90	309.0
143.00	3237.0
144.00	254.0
145.00	1266.0
145.80	476.0
147.00	111.0
147.90	478.0
148.70	105.0
149.10	115.0
149.90	228.0
152.80	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

153.70	148.0
155.00	526.0
155.90	106.0
156.90	449.0
157.80	123.0
158.90	255.0
160.90	275.0
170.90	624.0
172.00	2203.0
173.00	2288.0
174.00	181888.0
175.00	13819.0
176.00	175552.0
177.00	11943.0
178.00	320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	1795.0
37.00	8760.0
38.00	8370.0
39.00	3445.0
39.90	491.0
40.90	126.0
42.80	106.0
44.00	1284.0
45.00	1615.0
45.90	271.0
47.10	2395.0
47.90	1237.0
49.00	8489.0
50.00	38648.0
51.00	11584.0
52.10	470.0
53.00	304.0
54.00	191.0
55.00	583.0
56.00	3022.0
57.00	5552.0
58.10	339.0
60.00	2147.0
61.00	10942.0
62.00	10502.0
63.00	8870.0
64.00	1506.0
65.00	2069.0
65.90	287.0
67.10	476.0
68.00	22112.0
69.00	22440.0
70.00	1734.0
72.10	1124.0
73.00	10001.0
74.00	39040.0
75.00	111744.0
76.10	9361.0
77.00	1405.0
78.00	949.0
78.90	9280.0
80.00	2446.0
80.90	8915.0
82.00	1841.0
83.00	183.0
85.90	305.0
87.00	10182.0
88.00	10628.0
90.90	754.0
92.00	6712.0
93.00	10313.0
94.00	27472.0
95.00	224000.0
96.10	15206.0
97.00	450.0
103.00	170.0
103.90	1171.0
104.90	337.0
105.90	988.0
106.90	213.0
107.80	151.0
109.90	147.0
110.80	198.0
111.90	257.0
112.90	193.0
114.80	368.0
115.90	857.0
117.00	1724.0
118.00	941.0
118.90	1619.0
127.90	957.0
128.80	331.0
129.10	307.0
129.90	846.0
130.90	338.0
134.90	426.0
136.90	423.0
140.00	193.0
140.90	2407.0
141.90	330.0
143.00	3080.0
144.00	240.0
145.00	1158.0
145.90	491.0
146.90	109.0
147.90	564.0
149.20	109.0
149.90	226.0
152.80	110.0
153.80	176.0
155.00	570.0
155.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

156.90	502.0
157.80	142.0
159.00	285.0
160.90	341.0
170.80	562.0
172.00	2405.0
173.00	2237.0
174.00	188992.0
175.00	14036.0
176.00	182336.0
177.00	12107.0
178.10	332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

m/z	Abundance
36.00	1580.0
37.00	8066.0
38.00	7524.0
39.00	3115.0
40.00	478.0
41.00	123.0
43.10	116.0
44.00	1232.0
45.00	1501.0
46.00	230.0
47.10	2296.0
47.90	1038.0
49.00	7802.0
50.00	34944.0
51.00	10934.0
52.00	455.0
52.90	229.0
54.10	165.0
55.00	528.0
56.00	2771.0
57.00	5275.0
58.10	299.0
60.00	1970.0
61.00	9881.0
62.00	9718.0
63.00	8406.0
64.00	1308.0
65.00	1756.0
65.90	272.0
66.90	424.0
68.00	20160.0
69.00	20352.0
70.00	1516.0
72.10	1076.0
73.00	8764.0
74.00	36248.0
75.00	102024.0
76.10	8559.0
77.10	1276.0
77.90	915.0
78.90	8246.0
80.00	2175.0
81.00	7986.0
82.00	1740.0
83.00	195.0
85.90	247.0
87.00	9386.0
88.00	9510.0
90.90	754.0
92.00	6173.0
93.00	9240.0
94.00	24904.0
95.00	207936.0
96.10	13657.0
97.00	338.0
103.00	171.0
103.90	1061.0
104.90	322.0
105.90	937.0
106.90	222.0
107.80	157.0
109.90	167.0
111.00	190.0
112.00	272.0
112.80	185.0
114.80	344.0
115.90	815.0
117.00	1449.0
117.90	893.0
118.90	1485.0
120.00	117.0
127.90	931.0
128.80	333.0
129.90	773.0
130.90	304.0
134.90	326.0
136.90	344.0
140.00	199.0
140.90	2105.0
142.00	297.0
143.00	2870.0
144.00	206.0
144.90	970.0
145.90	430.0
146.90	108.0
147.90	556.0
149.90	187.0
152.90	123.0
153.80	190.0
154.90	580.0
155.90	118.0
156.90	471.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327

157.80	117.0
159.00	288.0
161.00	345.0
170.80	419.0
172.00	2331.0
173.00	1962.0
174.00	176512.0
175.00	12847.0
176.00	170304.0
177.00	10944.0
178.10	330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB327