

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061323\
 Data File : VW031508.D
 Acq On : 13 Jun 2023 11:33
 Operator : SY/MD
 Sample : 03101-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES2

Quant Time: Jun 13 23:48:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 13 23:48:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	231551	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	241798	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	118994	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	98509	48.354	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.700%
7) Chloroethane-d5	1.532	69	86181	52.250	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.500%
11) 1,1-Dichloroethene-d2	2.059	65	50156	51.946	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	103.900%
21) 2-Butanone-d5	3.796	46	139300	94.613	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.610%
24) Chloroform-d	4.252	84	200632	51.773	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.540%
26) 1,2-Dichloroethane-d4	4.947	65	142137	54.674	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.340%
32) Benzene-d6	4.963	84	379243	53.124	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.240%
36) 1,2-Dichloropropane-d6	5.992	67	133730	53.893	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.780%
41) Toluene-d8	7.249	98	335765	51.200	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.400%
43) trans-1,3-Dichloroprop...	7.558	79	58976	47.183	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.360%
47) 2-Hexanone-d5	8.030	63	66200	70.833	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	70.830%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	119382	38.123	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.240%
66) 1,2-Dichlorobenzene-d4	11.567	152	132018	59.807	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	119.620%
Target Compounds						
13) Acetone	2.121	43	8180	6.211	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061323\
Data File : VV031508.D
Acq On : 13 Jun 2023 11:33
Operator : SY/MD
Sample : 03101-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES2

Quant Time: Jun 13 23:48:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 13 23:48:05 2023
Response via : Initial Calibration

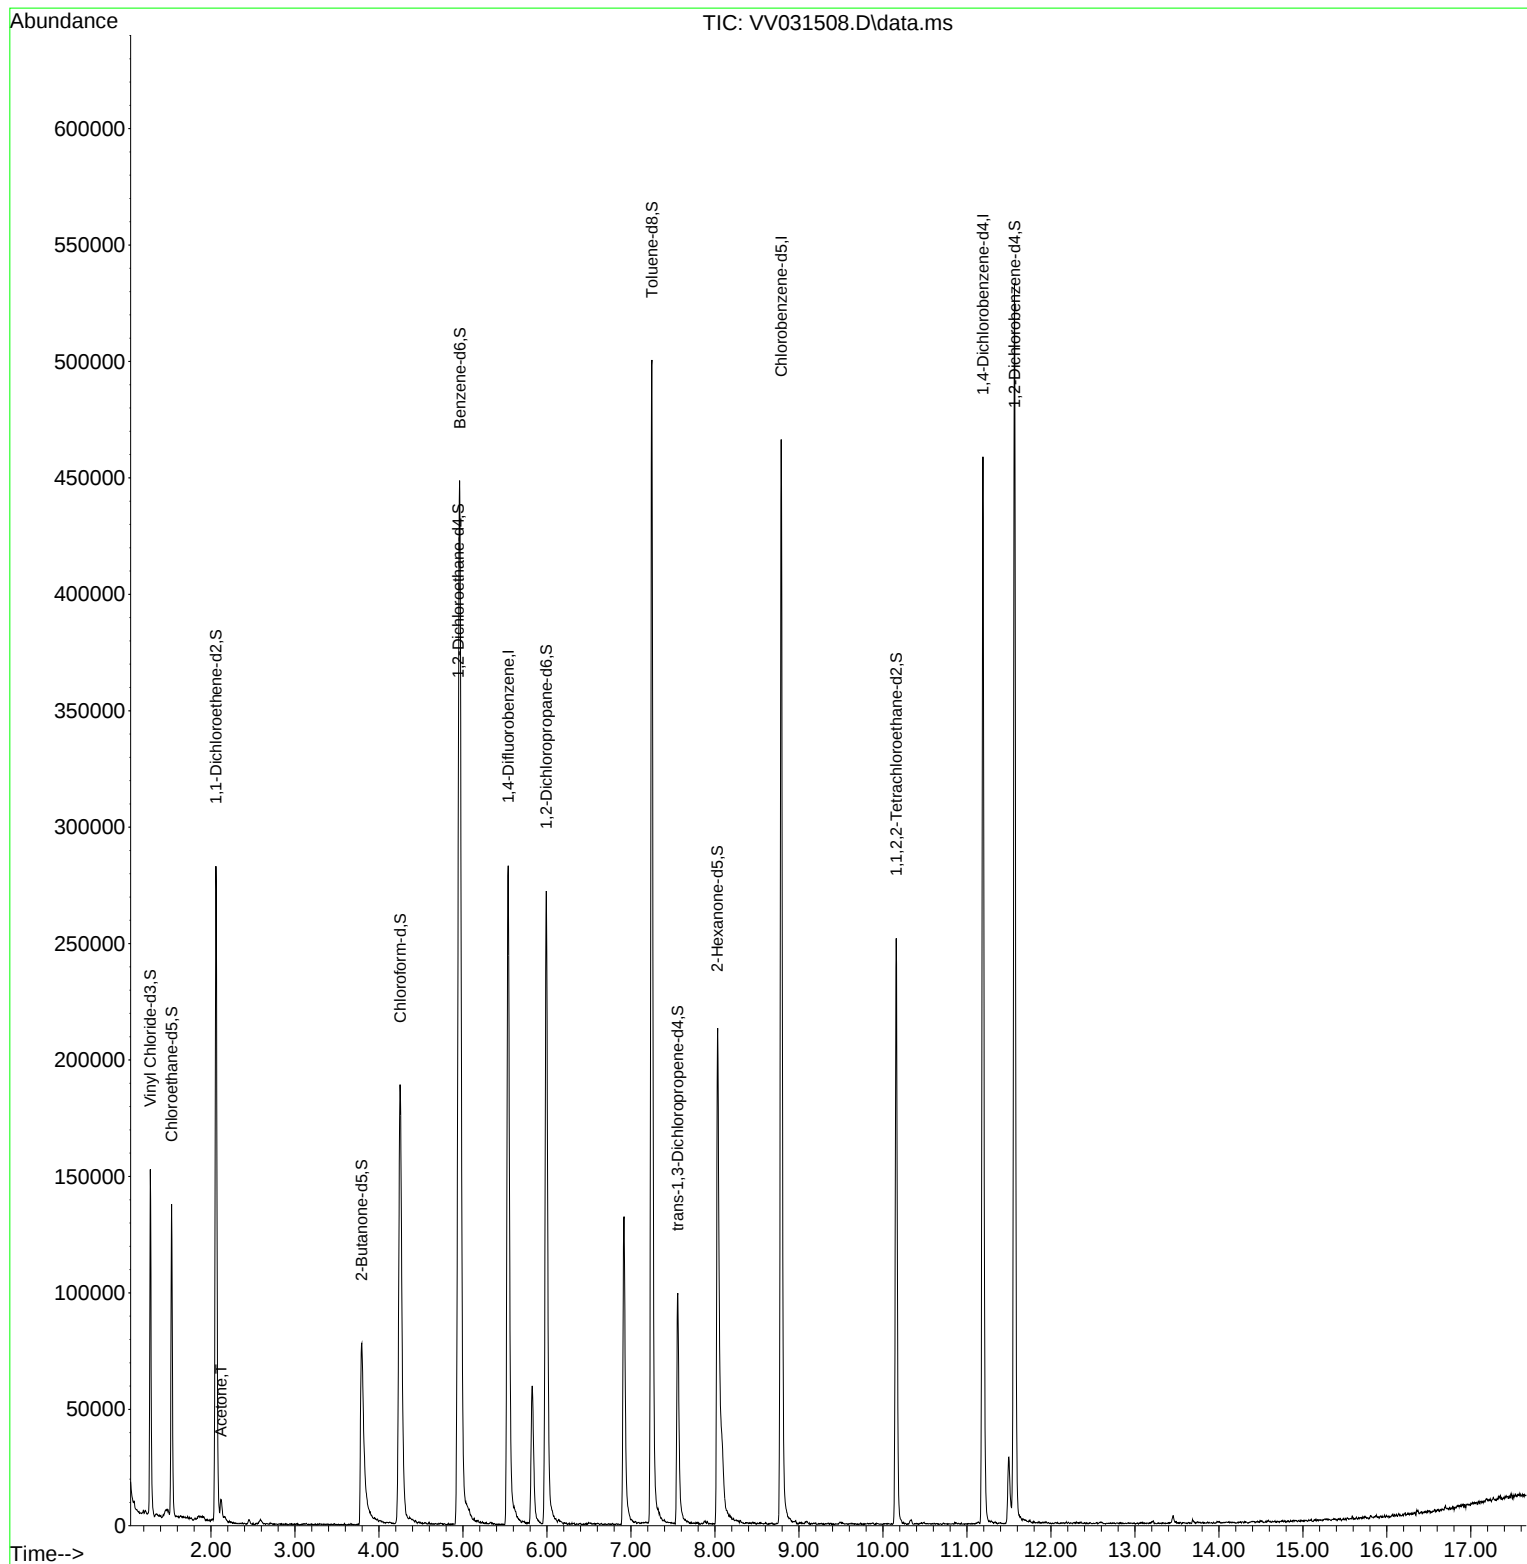

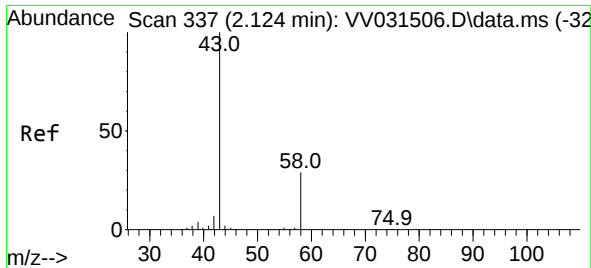

#13

Acetone

Concen: 6.211 ug/L

RT: 2.121 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV031508.D

Acq: 13 Jun 2023 11:33

Instrument :

MSVOA_V

ClientSampleId :

EZES2

Tgt Ion: 43 Resp: 8180

Ion Ratio Lower Upper

43 100

58 31.4 0.0 61.0

