

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW061323\
 Data File : VW031508.D
 Acq On : 13 Jun 2023 11:33
 Operator : SY/MD
 Sample : 03101-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VW031508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	149120	162635	13.45%	1.892%
2	1.532	146	153	167	rVB	134305	157000	12.98%	1.826%
3	2.059	307	317	331	rBV	280742	412591	34.12%	4.799%
4	2.500	452	454	458	rVB2	644	311	0.03%	0.004%
5	2.529	461	463	464	rBV	376	162	0.01%	0.002%
6	2.561	470	473	474	rBV2	642	291	0.02%	0.003%
7	2.703	515	517	519	rBV	415	167	0.01%	0.002%
8	2.802	546	548	550	rBV	252	174	0.01%	0.002%
9	2.834	555	558	559	rBV	293	111	0.01%	0.001%
10	2.867	566	568	572	rBV	289	187	0.02%	0.002%
11	2.886	572	574	577	rVB	326	141	0.01%	0.002%
12	2.998	607	609	611	rVB2	337	140	0.01%	0.002%
13	3.037	619	621	626	rVB2	571	374	0.03%	0.004%
14	3.063	626	629	630	rBV	227	152	0.01%	0.002%
15	3.076	630	633	635	rVB2	284	142	0.01%	0.002%
16	3.092	635	638	639	rBV2	357	214	0.02%	0.002%
17	3.227	678	680	681	rBV	165	51	0.00%	0.001%
18	3.272	692	694	697	rBV2	436	289	0.02%	0.003%
19	3.294	697	701	702	rBV2	349	190	0.02%	0.002%
20	3.346	715	717	719	rBV2	392	193	0.02%	0.002%
21	3.400	733	734	736	rBV	243	96	0.01%	0.001%
22	3.432	741	744	745	rBV3	246	147	0.01%	0.002%
23	3.471	751	756	758	rBV2	457	346	0.03%	0.004%
24	3.519	768	771	774	rVB	337	243	0.02%	0.003%
25	3.548	774	780	781	rBV2	285	257	0.02%	0.003%
26	3.590	789	793	799	rVB2	702	640	0.05%	0.007%
27	3.616	799	801	805	rBV2	310	233	0.02%	0.003%
28	3.641	805	809	813	rBV4	346	311	0.03%	0.004%
29	3.667	813	817	820	rVV2	471	319	0.03%	0.004%
30	3.703	825	828	832	rBV2	236	189	0.02%	0.002%
31	3.754	841	844	846	rVB2	412	229	0.02%	0.003%
32	3.796	846	857	886	rBV	77943	228615	18.91%	2.659%
33	4.252	984	999	1022	rBV2	187631	488579	40.41%	5.682%
34	4.641	1117	1120	1123	rBV3	351	246	0.02%	0.003%
35	4.715	1141	1143	1146	rBV	326	122	0.01%	0.001%
36	4.828	1176	1178	1180	rVB	478	175	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061323\
 Data File : VV031508.D
 Acq On : 13 Jun 2023 11:33
 Operator : SY/MD
 Sample : 03101-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	4.854	1184	1186	1188	rBV	349	181	0.01%	0.002%
38	4.960	1201	1219	1253	rBV2	448270	1209175	100.00%	14.063%
39	5.397	1354	1355	1357	rVB2	378	107	0.01%	0.001%
40	5.413	1357	1360	1362	rBV	330	245	0.02%	0.003%
41	5.426	1362	1364	1365	rVB	252	79	0.01%	0.001%
42	5.461	1373	1375	1376	rBV	253	60	0.00%	0.001%
43	5.471	1376	1378	1380	rVB	238	72	0.01%	0.001%
44	5.481	1380	1381	1384	rVB	264	128	0.01%	0.001%
45	5.538	1385	1399	1419	rBV	283003	593094	49.05%	6.898%
46	5.825	1477	1488	1509	rBV	59090	128079	10.59%	1.490%
47	5.992	1526	1540	1567	rBV	271645	572639	47.36%	6.660%
48	6.201	1603	1605	1609	rBV4	609	550	0.05%	0.006%
49	6.297	1633	1635	1637	rVB	497	151	0.01%	0.002%
50	6.355	1649	1653	1656	rBV3	473	363	0.03%	0.004%
51	6.439	1677	1679	1681	rBV3	300	145	0.01%	0.002%
52	6.477	1689	1691	1693	rBV	386	167	0.01%	0.002%
53	6.493	1693	1696	1698	rBV3	729	433	0.04%	0.005%
54	6.580	1721	1723	1726	rBV2	519	384	0.03%	0.004%
55	6.635	1738	1740	1741	rBV	288	120	0.01%	0.001%
56	6.683	1752	1755	1757	rBV2	268	198	0.02%	0.002%
57	6.767	1780	1781	1784	rBV2	273	178	0.01%	0.002%
58	6.809	1791	1794	1796	rBV2	265	128	0.01%	0.001%
59	6.918	1817	1828	1853	rBV	132234	257307	21.28%	2.993%
60	7.249	1919	1931	1953	rBV	499098	893837	73.92%	10.396%
61	7.558	2017	2027	2048	rBV	99145	183585	15.18%	2.135%
62	7.773	2093	2094	2097	rBV3	486	231	0.02%	0.003%
63	7.841	2111	2115	2119	rBV3	461	427	0.04%	0.005%
64	7.908	2134	2136	2142	rVB3	1223	906	0.07%	0.011%
65	7.934	2142	2144	2147	rBV2	388	277	0.02%	0.003%
66	7.972	2155	2156	2158	rBV	441	172	0.01%	0.002%
67	8.034	2164	2175	2208	rBV2	213035	509397	42.13%	5.924%
68	8.789	2398	2410	2435	rBV	465377	763270	63.12%	8.877%
69	9.075	2495	2499	2501	rBV3	834	644	0.05%	0.007%
70	9.127	2513	2515	2517	rVB2	568	197	0.02%	0.002%
71	9.140	2517	2519	2520	rBV	307	112	0.01%	0.001%
72	9.288	2563	2565	2569	rVB2	484	266	0.02%	0.003%
73	9.313	2570	2573	2575	rBV	478	335	0.03%	0.004%
74	9.410	2601	2603	2605	rBV	403	230	0.02%	0.003%
75	9.490	2621	2628	2634	rBV3	974	1431	0.12%	0.017%
76	9.516	2634	2636	2640	rVV4	616	338	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061323\
 Data File : VV031508.D
 Acq On : 13 Jun 2023 11:33
 Operator : SY/MD
 Sample : 03101-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	9.596	2657	2661	2662	rBV2	406	267	0.02%	0.003%
78	9.677	2682	2686	2689	rBV3	354	248	0.02%	0.003%
79	9.734	2702	2704	2708	rVB	554	269	0.02%	0.003%
80	9.783	2716	2719	2721	rBV3	439	250	0.02%	0.003%
81	9.908	2756	2758	2760	rVB	349	137	0.01%	0.002%
82	9.924	2760	2763	2765	rBV	571	309	0.03%	0.004%
83	10.069	2804	2808	2811	rBV	342	239	0.02%	0.003%
84	10.159	2825	2836	2861	rVB	251267	401237	33.18%	4.667%
85	10.294	2876	2878	2879	rBV	337	173	0.01%	0.002%
86	10.329	2882	2889	2890	rBV4	1711	1676	0.14%	0.019%
87	10.439	2921	2923	2925	rBV2	451	271	0.02%	0.003%
88	10.615	2976	2978	2981	rVB2	447	229	0.02%	0.003%
89	10.718	3005	3010	3012	rBV3	697	553	0.05%	0.006%
90	10.857	3050	3053	3056	rBV2	906	676	0.06%	0.008%
91	11.191	3146	3157	3179	rBV	458100	724900	59.95%	8.431%
92	11.500	3243	3253	3263	rBV2	27981	53719	4.44%	0.625%
93	11.567	3264	3274	3291	rVB	529742	836406	69.17%	9.728%
94	13.049	3733	3735	3738	rBV2	571	406	0.03%	0.005%
95	13.564	3892	3895	3896	rBV3	490	292	0.02%	0.003%




Sum of corrected areas: 8598157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061323\
Data File : VV031508.D
Acq On : 13 Jun 2023 11:33
Operator : SY/MD
Sample : 03101-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

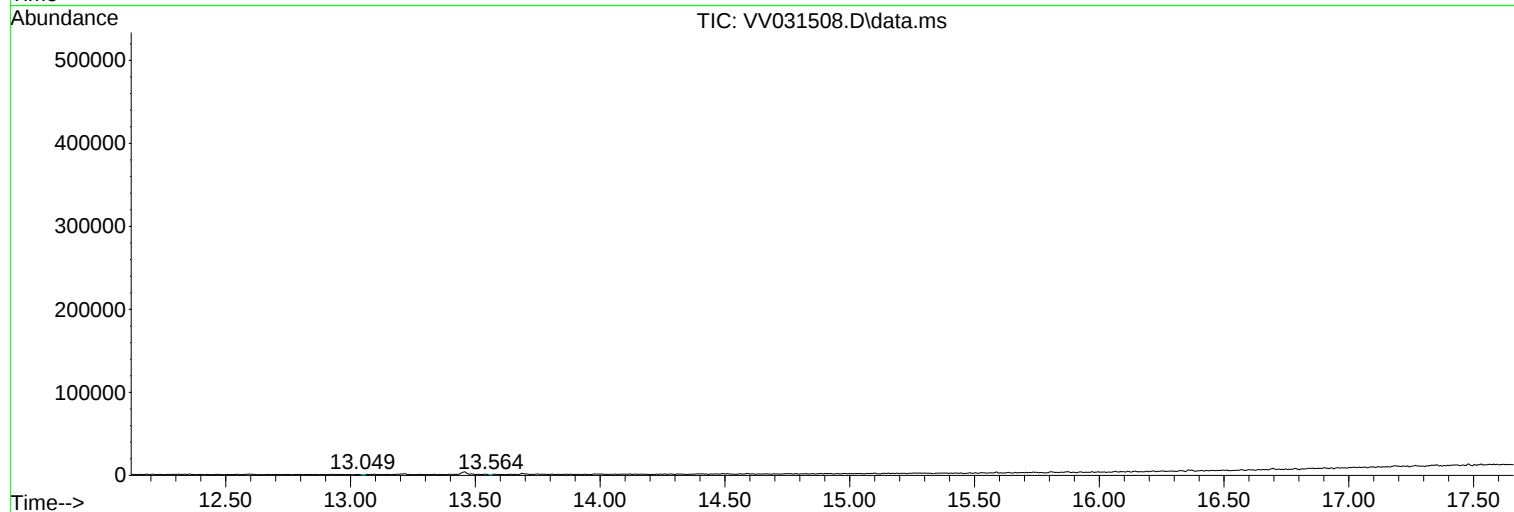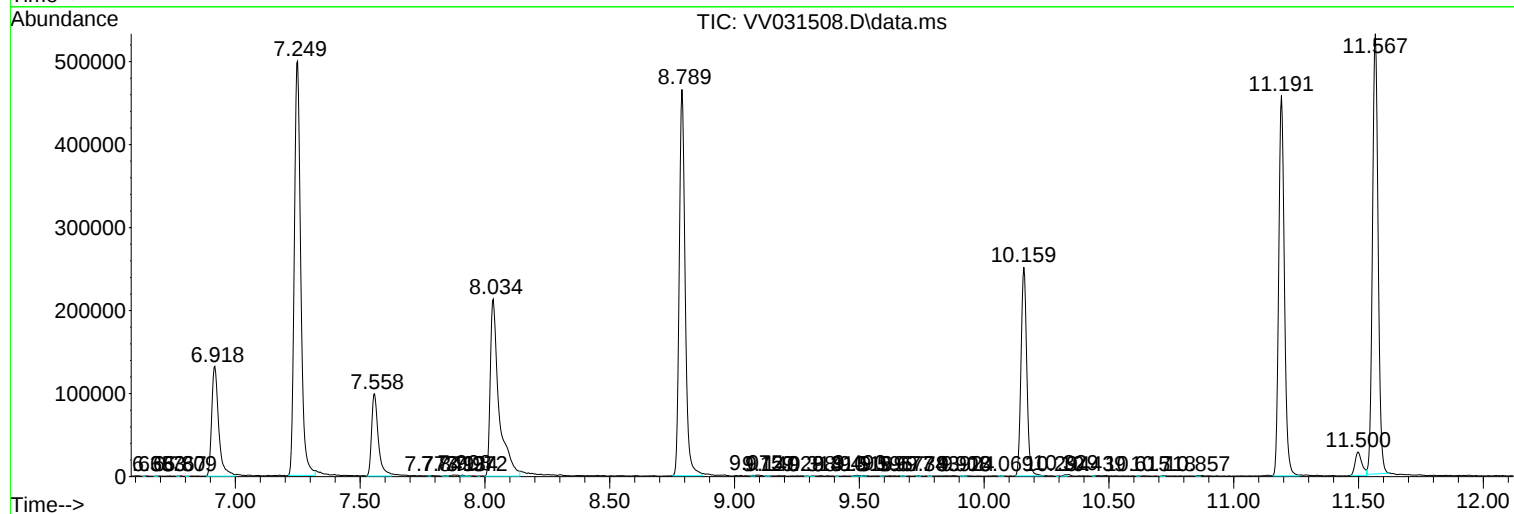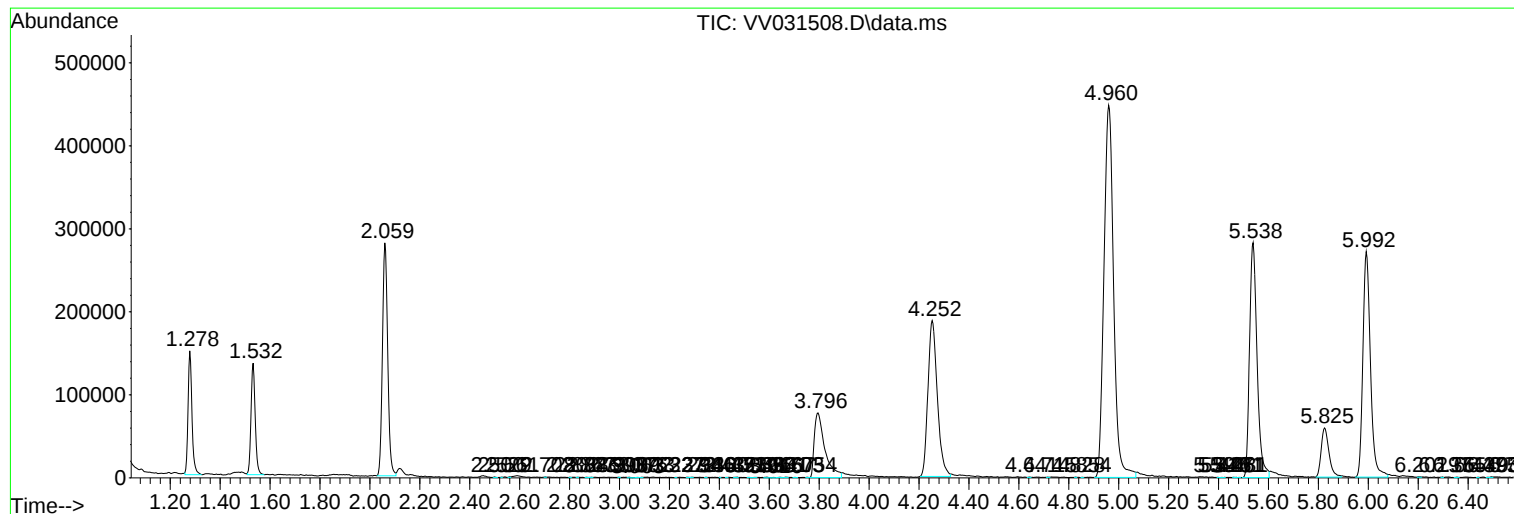

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061323\
Data File : VV031508.D
Acq On : 13 Jun 2023 11:33
Operator : SY/MD
Sample : 03101-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061323\
Data File : VV031508.D
Acq On : 13 Jun 2023 11:33
Operator : SY/MD
Sample : 03101-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc