


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061323\
Data File : VV031505.D
Acq On : 13 Jun 2023 09:26
Operator : SY/MD
Sample : BFB386
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB386

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Title : VOC Analysis
Last Update : Tue Jun 13 23:48:05 2023

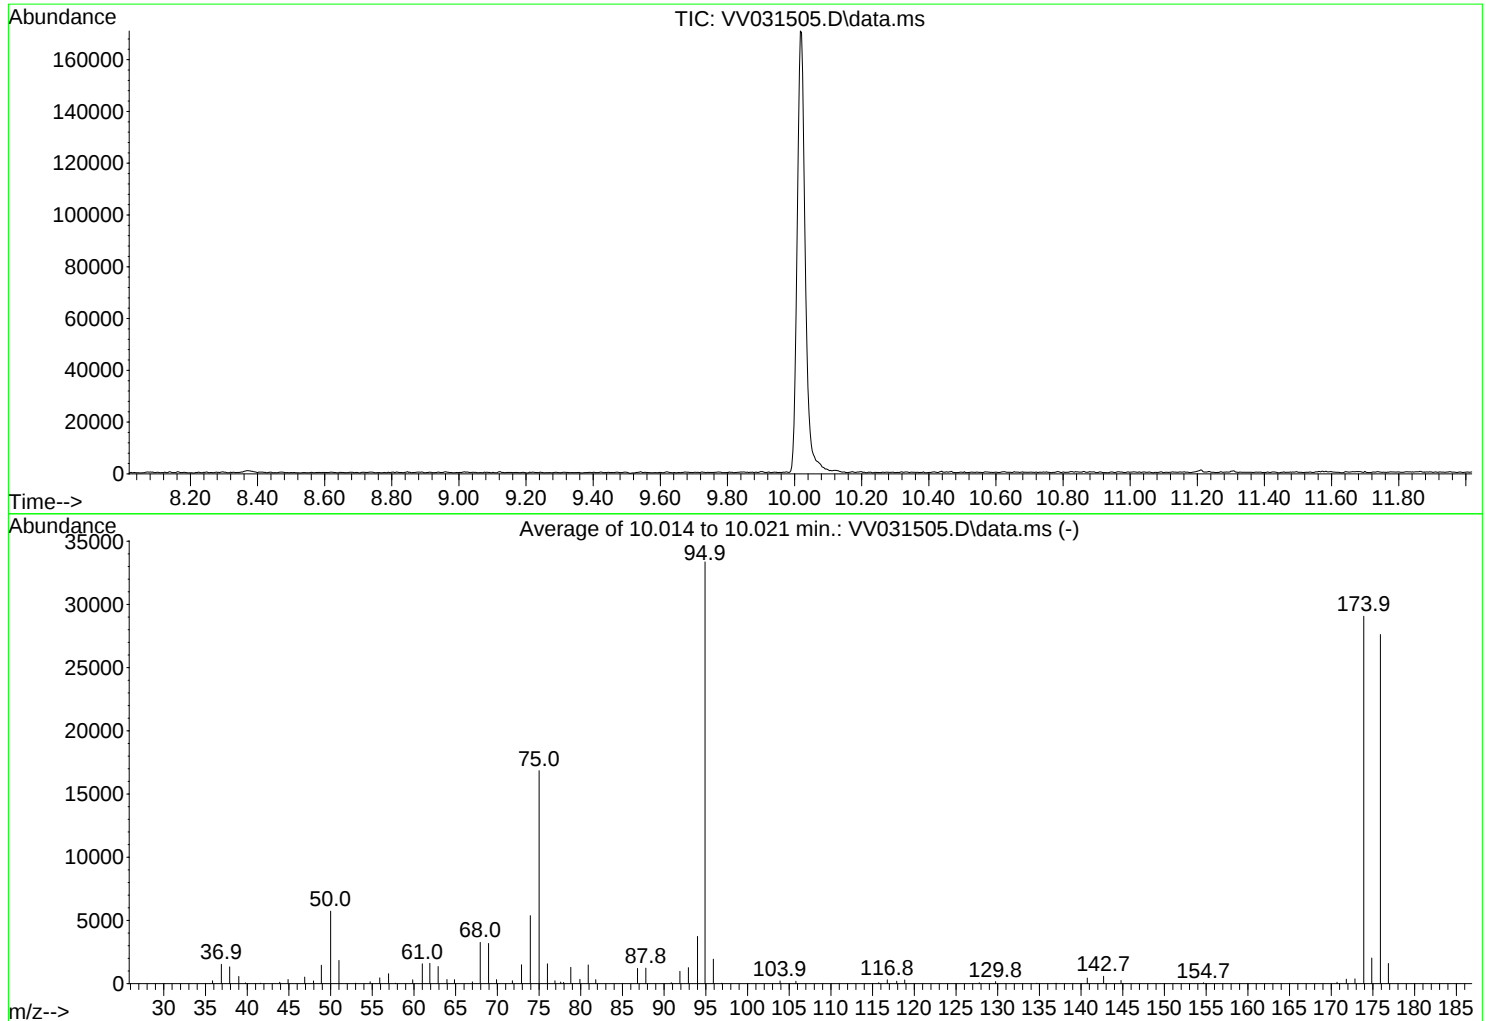

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	5740	PASS
75	95	30	80	50.5	16849	PASS
95	95	100	100	100.0	33373	PASS
96	95	5	9	5.8	1934	PASS
173	174	0.00	2	1.3	385	PASS
174	95	50	120	87.1	29067	PASS
175	174	5	9	7.0	2022	PASS
176	174	95	105	95.0	27619	PASS
177	176	5	10	5.8	1600	PASS

m/z	Abundance
39.90	181.0
43.90	376.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386

m/z	Abundance
35.80	235.0
36.90	1563.0
37.90	1257.0
38.90	601.0
39.70	269.0
43.90	478.0
44.90	307.0
46.90	433.0
48.00	229.0
48.90	1452.0
50.00	5408.0
51.00	1830.0
53.00	105.0
54.80	169.0
55.90	413.0
56.90	686.0
59.90	310.0
61.00	1338.0
61.90	1487.0
62.90	1271.0
64.00	347.0
64.80	327.0
67.20	118.0
68.00	2976.0
68.90	2990.0
69.90	284.0
71.80	218.0
72.90	1571.0
73.90	5078.0
75.00	16124.0
76.00	1289.0
76.90	226.0
77.60	221.0
78.10	101.0
78.80	1130.0
79.90	304.0
80.90	1482.0
81.80	316.0
86.80	1165.0
87.80	1143.0
90.90	127.0
91.90	906.0
92.90	1163.0
94.00	3465.0
94.90	31224.0
95.90	1761.0
96.90	111.0
103.90	210.0
105.80	196.0
116.70	274.0
117.90	184.0
118.80	254.0
129.80	134.0
140.80	446.0
142.70	503.0
144.80	306.0
154.70	104.0
170.70	107.0
171.80	302.0
172.80	329.0
173.90	27392.0
174.90	2050.0
175.90	25392.0
176.80	1525.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386

m/z	Abundance
35.90	233.0
36.90	1570.0
37.90	1382.0
39.00	563.0
39.70	256.0
43.90	483.0
44.90	356.0
46.90	575.0
48.00	198.0
48.90	1511.0
50.00	5949.0
51.00	1887.0
54.80	174.0
55.90	473.0
56.90	794.0
59.80	315.0
61.00	1637.0
61.90	1654.0
62.90	1380.0
64.00	334.0
64.80	337.0
67.00	139.0
68.00	3428.0
68.90	3269.0
69.90	320.0
71.80	242.0
72.90	1540.0
74.00	5493.0
75.00	17400.0
76.00	1601.0
76.90	244.0
77.60	178.0
78.80	1325.0
79.90	340.0
80.90	1516.0
81.80	347.0
86.80	1215.0
87.80	1312.0
90.80	107.0
91.90	999.0
92.90	1304.0
94.00	3831.0
94.90	34632.0
95.90	1957.0
103.90	234.0
105.80	188.0
115.70	106.0
116.70	313.0
117.90	212.0
118.90	313.0
127.80	108.0
129.70	158.0
140.80	467.0
142.70	602.0
144.80	247.0
154.70	117.0
170.70	132.0
171.80	348.0
172.80	400.0
173.90	30048.0
174.90	2075.0
175.90	28584.0
176.90	1614.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386

m/z	Abundance
35.80	235.0
36.90	1470.0
37.90	1354.0
39.10	565.0
39.80	223.0
41.60	111.0
43.90	496.0
44.90	329.0
46.90	568.0
47.90	202.0
48.90	1389.0
50.00	5863.0
51.00	1800.0
54.70	135.0
55.90	468.0
57.00	892.0
57.80	102.0
59.90	285.0
61.00	1753.0
61.90	1673.0
62.90	1412.0
63.90	309.0
64.90	282.0
66.90	174.0
67.90	3411.0
69.00	3286.0
69.90	345.0
71.80	228.0
72.90	1364.0
74.00	5557.0
75.00	17024.0
76.00	1801.0
76.90	206.0
77.90	211.0
78.80	1433.0
79.90	373.0
80.90	1437.0
81.80	301.0
86.80	1223.0
87.80	1231.0
91.90	1010.0
92.90	1328.0
94.00	3917.0
94.90	34264.0
95.90	2083.0
103.90	196.0
105.80	198.0
115.80	142.0
116.80	323.0
117.90	192.0
118.90	300.0
127.80	137.0
129.70	208.0
134.70	114.0
137.00	109.0
140.70	417.0
142.70	651.0
144.80	215.0
170.70	118.0
171.80	413.0
172.90	427.0
173.90	29760.0
174.80	1940.0
175.90	28880.0
176.90	1661.0

Instrument :
MSVOA_V
ClientSampleId :
BFB386