

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061419\
 Data File : VV011506.D
 Acq On : 14 Jun 2019 22:36
 Operator : SY/MD
 Sample : K3289-18
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFC6

Quant Time: Jun 15 01:49:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 15 01:30:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	186037	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	171562	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	69186	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	64517	4.60	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.00%
7) Chloroethane-d5	1.58	69	43935	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.60%
11) 1,1-Dichloroethene-d2	2.12	63	100731	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.96	46	197318	49.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.84%
24) Chloroform-d	4.40	84	129091	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.08	65	75275	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
32) Benzene-d6	5.09	84	258348	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.12	67	80101	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.36	98	224542	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
43) trans-1,3-Dichloropropene-	7.66	79	23498	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.14	63	151825	48.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	56275	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	73406	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
13) Acetone	2.22	43	7450	2.797 ug/L	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061419\
Data File : VV011506.D
Acq On : 14 Jun 2019 22:36
Operator : SY/MD
Sample : K3289-18
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCS6

Quant Time: Jun 15 01:49:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 15 01:30:25 2019
Response via : Initial Calibration

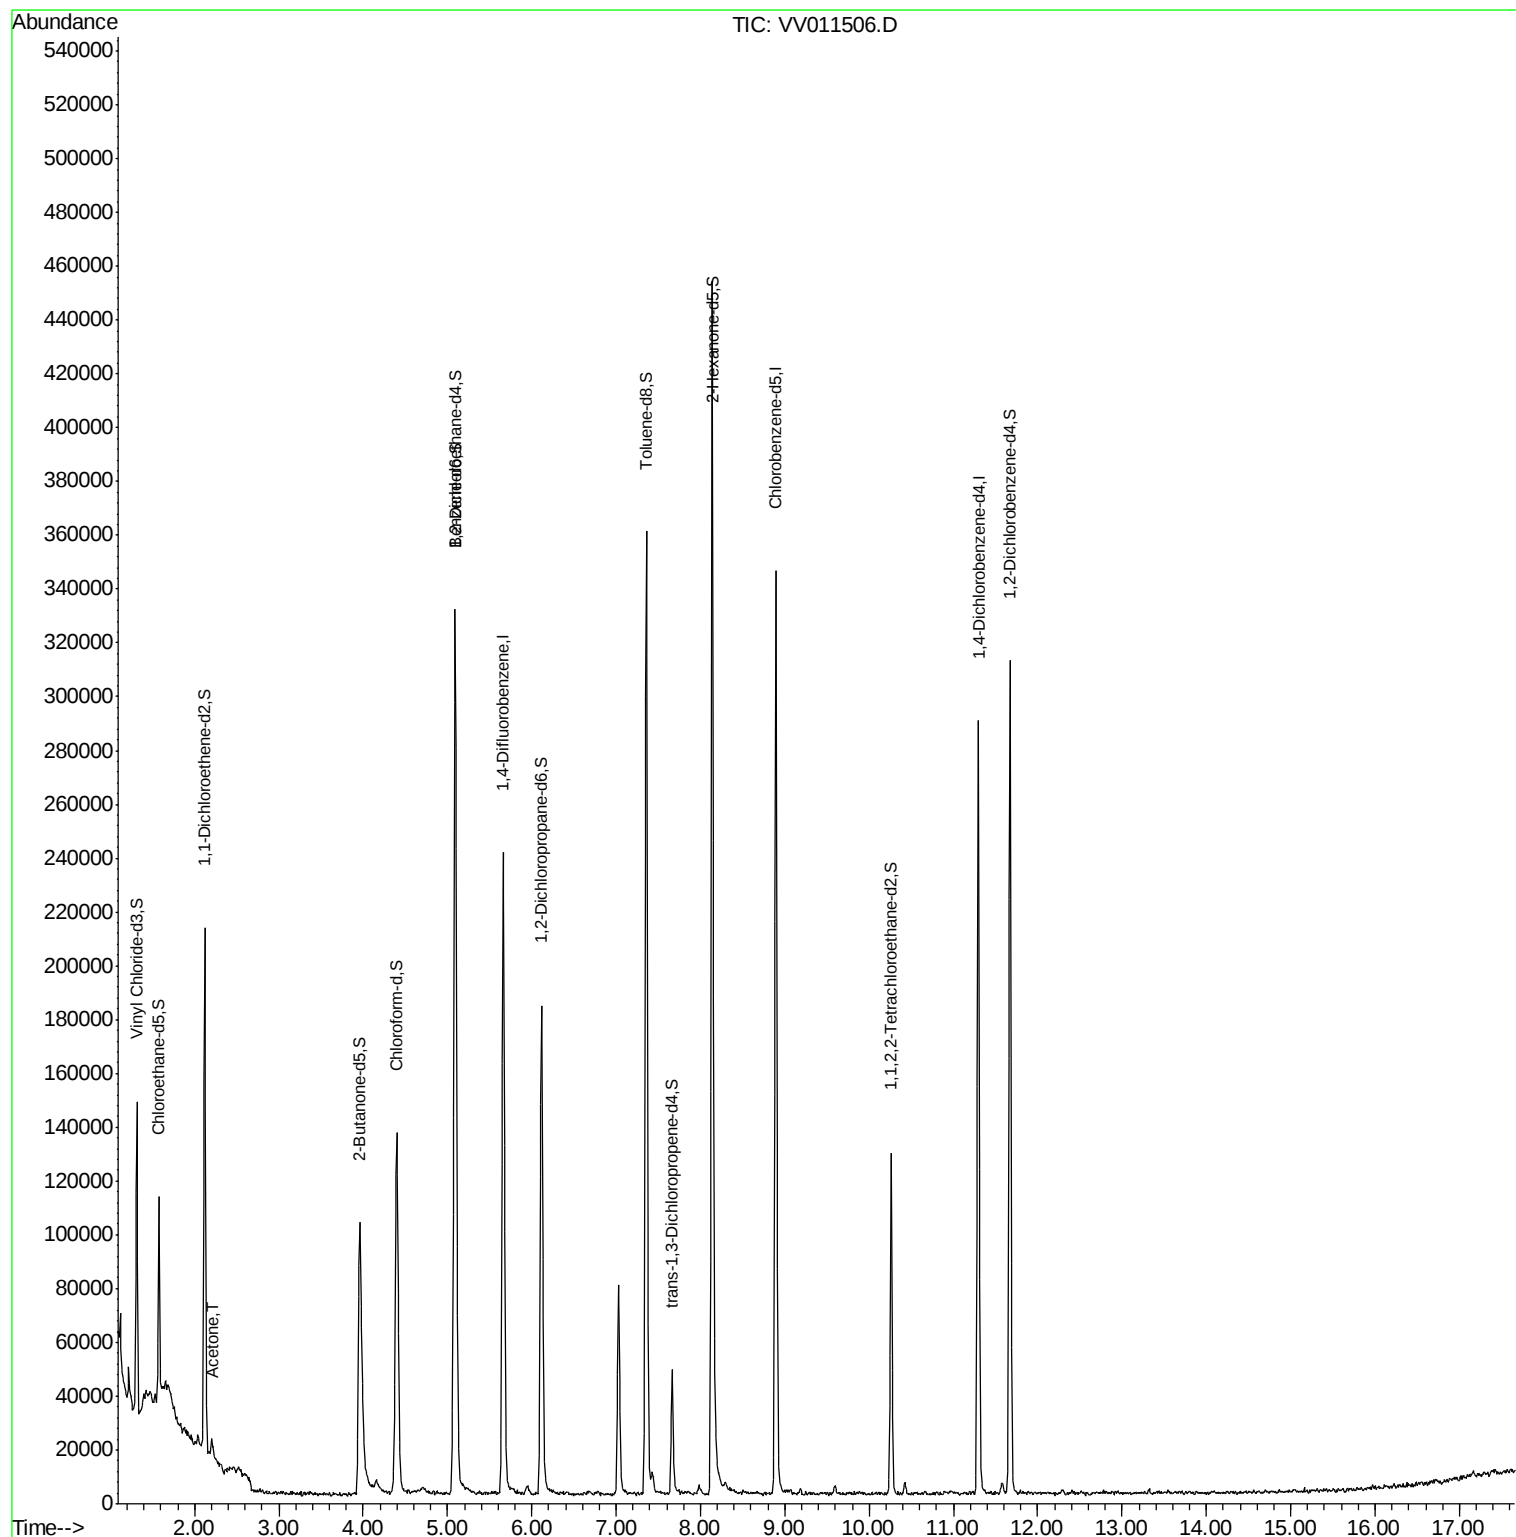

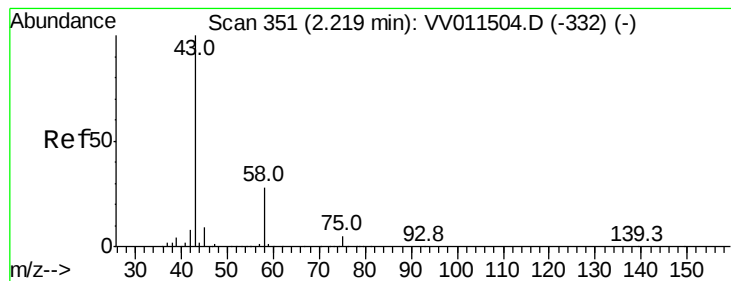

#13

Acetone

Concen: 2.797 ug/L

RT: 2.22 min Scan# 350

Delta R.T. -0.00 min

Lab File: VV011506.D

Acq: 14 Jun 2019 22:36

Instrument :
MSVOA_V
ClientSampleId :
BFCS6

Tot Ion: 43 Resp: 7450

Ion Ratio Lower Upper

43 100

58 6.6 0.0 57.8

