

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061419\
 Data File : VV011521.D
 Acq On : 15 Jun 2019 05:40
 Operator : SY/MD
 Sample : K3314-17
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM49

Quant Time: Jun 16 20:23:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 15 04:37:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	180812	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	162287	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	64214	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	60704	4.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.00%
7) Chloroethane-d5	1.56	69	41842	4.84	ug/L	-0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.12	63	91808	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	3.95	46	186820	48.63	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.26%
24) Chloroform-d	4.40	84	122447	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.08	65	73771	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.09	84	244829	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	6.11	67	76266	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.36	98	209829	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
43) trans-1,3-Dichloropropene-	7.66	79	21867	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.13	63	140503	47.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.22%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	50505	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	68039	5.31	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	7866	3.039 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061419\
Data File : VV011521.D
Acq On : 15 Jun 2019 05:40
Operator : SY/MD
Sample : K3314-17
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM49

Quant Time: Jun 16 20:23:13 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 15 04:37:55 2019
Response via : Initial Calibration

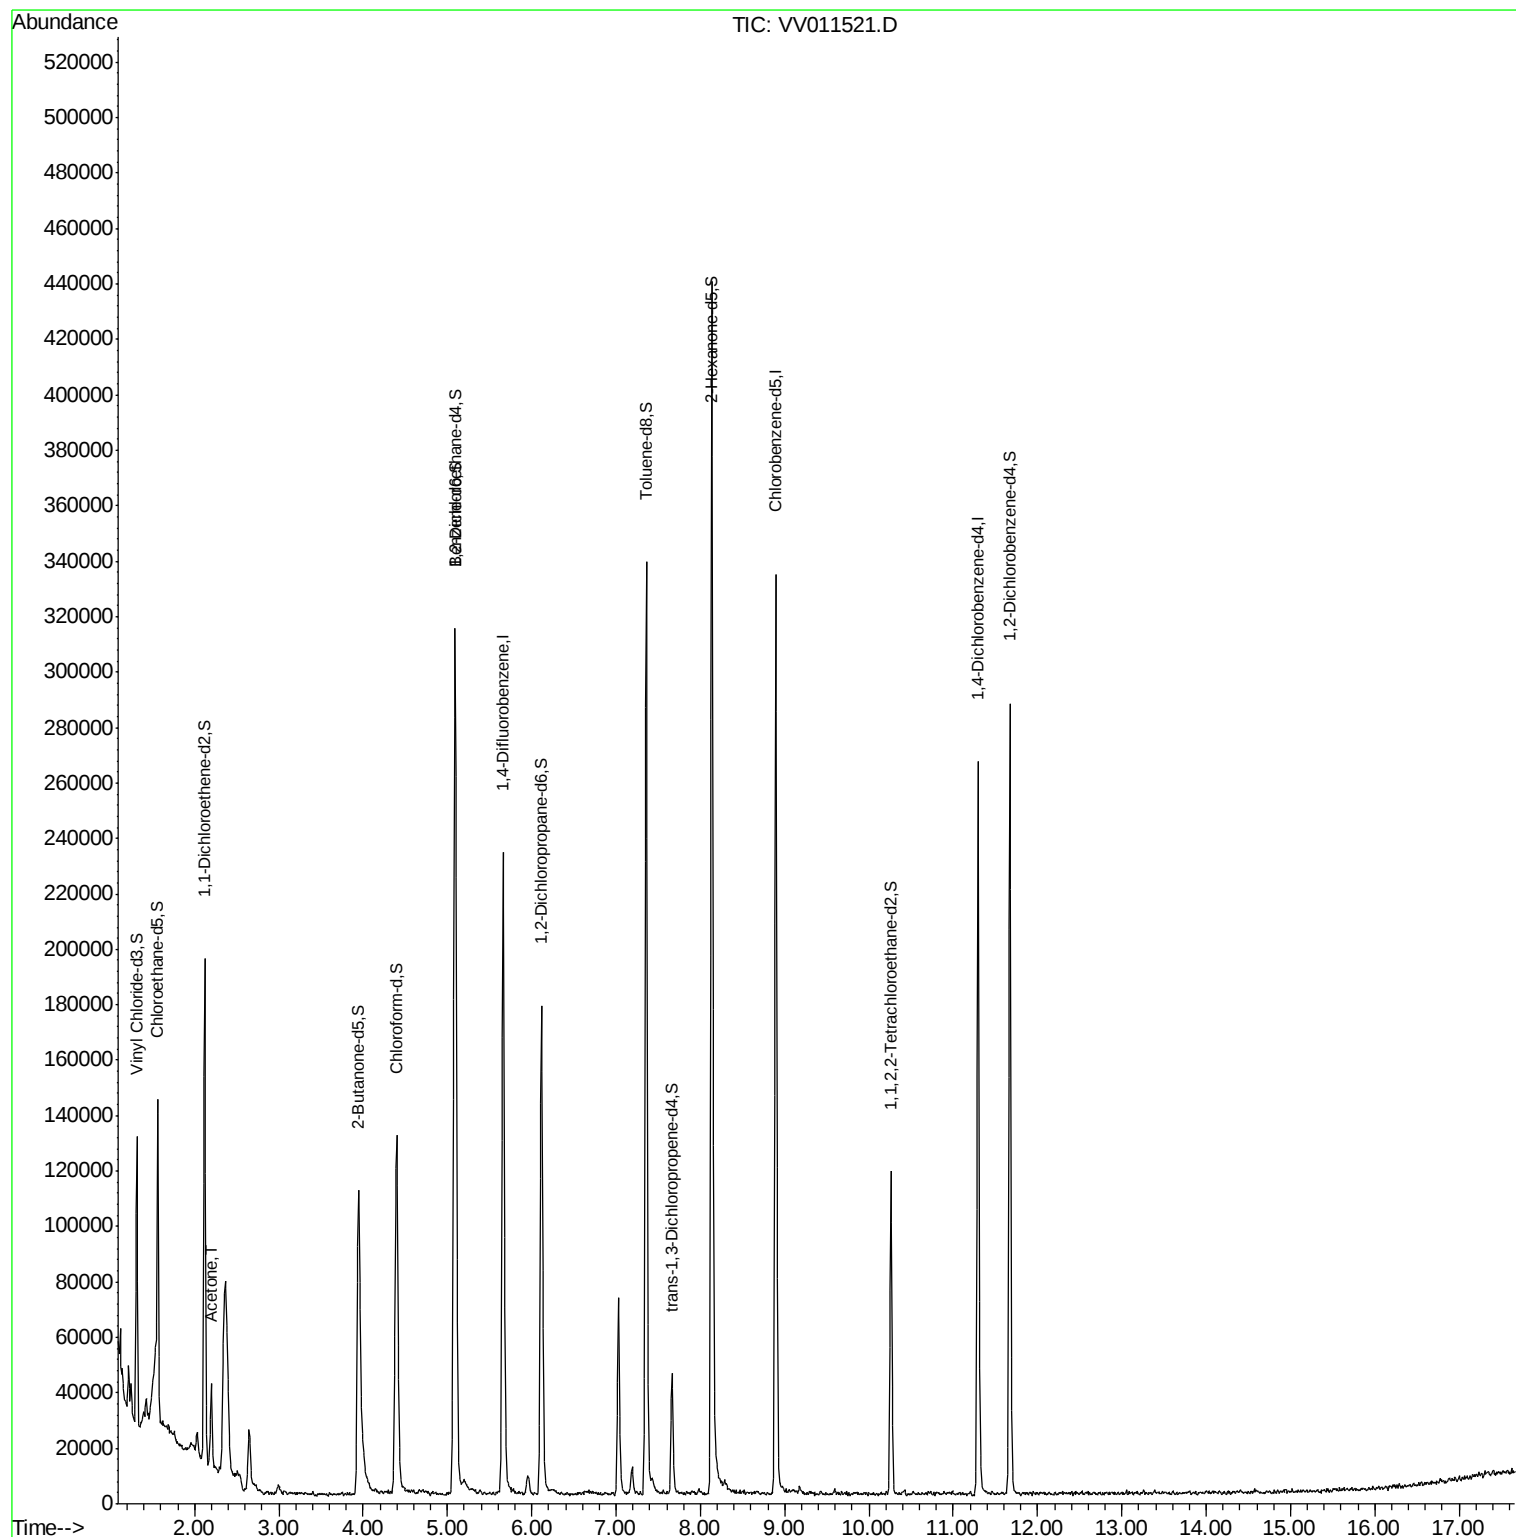

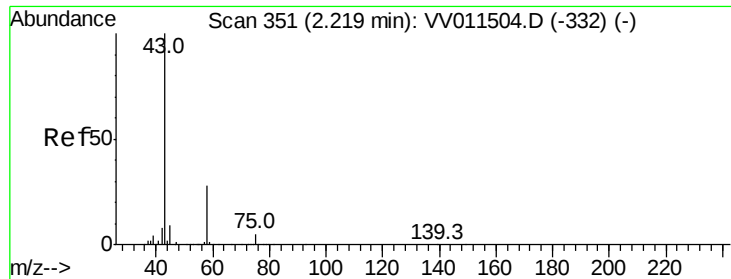

#13

Acetone

Concen: 3.039 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.02 min

Lab File: VV011521.D

Acq: 15 Jun 2019 05:40

Instrument :
MSVOA_V
ClientSampleId :
COM49

Tot Ion: 43 Resp: 7866

Ion Ratio Lower Upper

43 100

58 32.2 0.0 57.8

